


a Standard negative controls: Field DNA reads



b Standard negative controls: Standard DNA reads

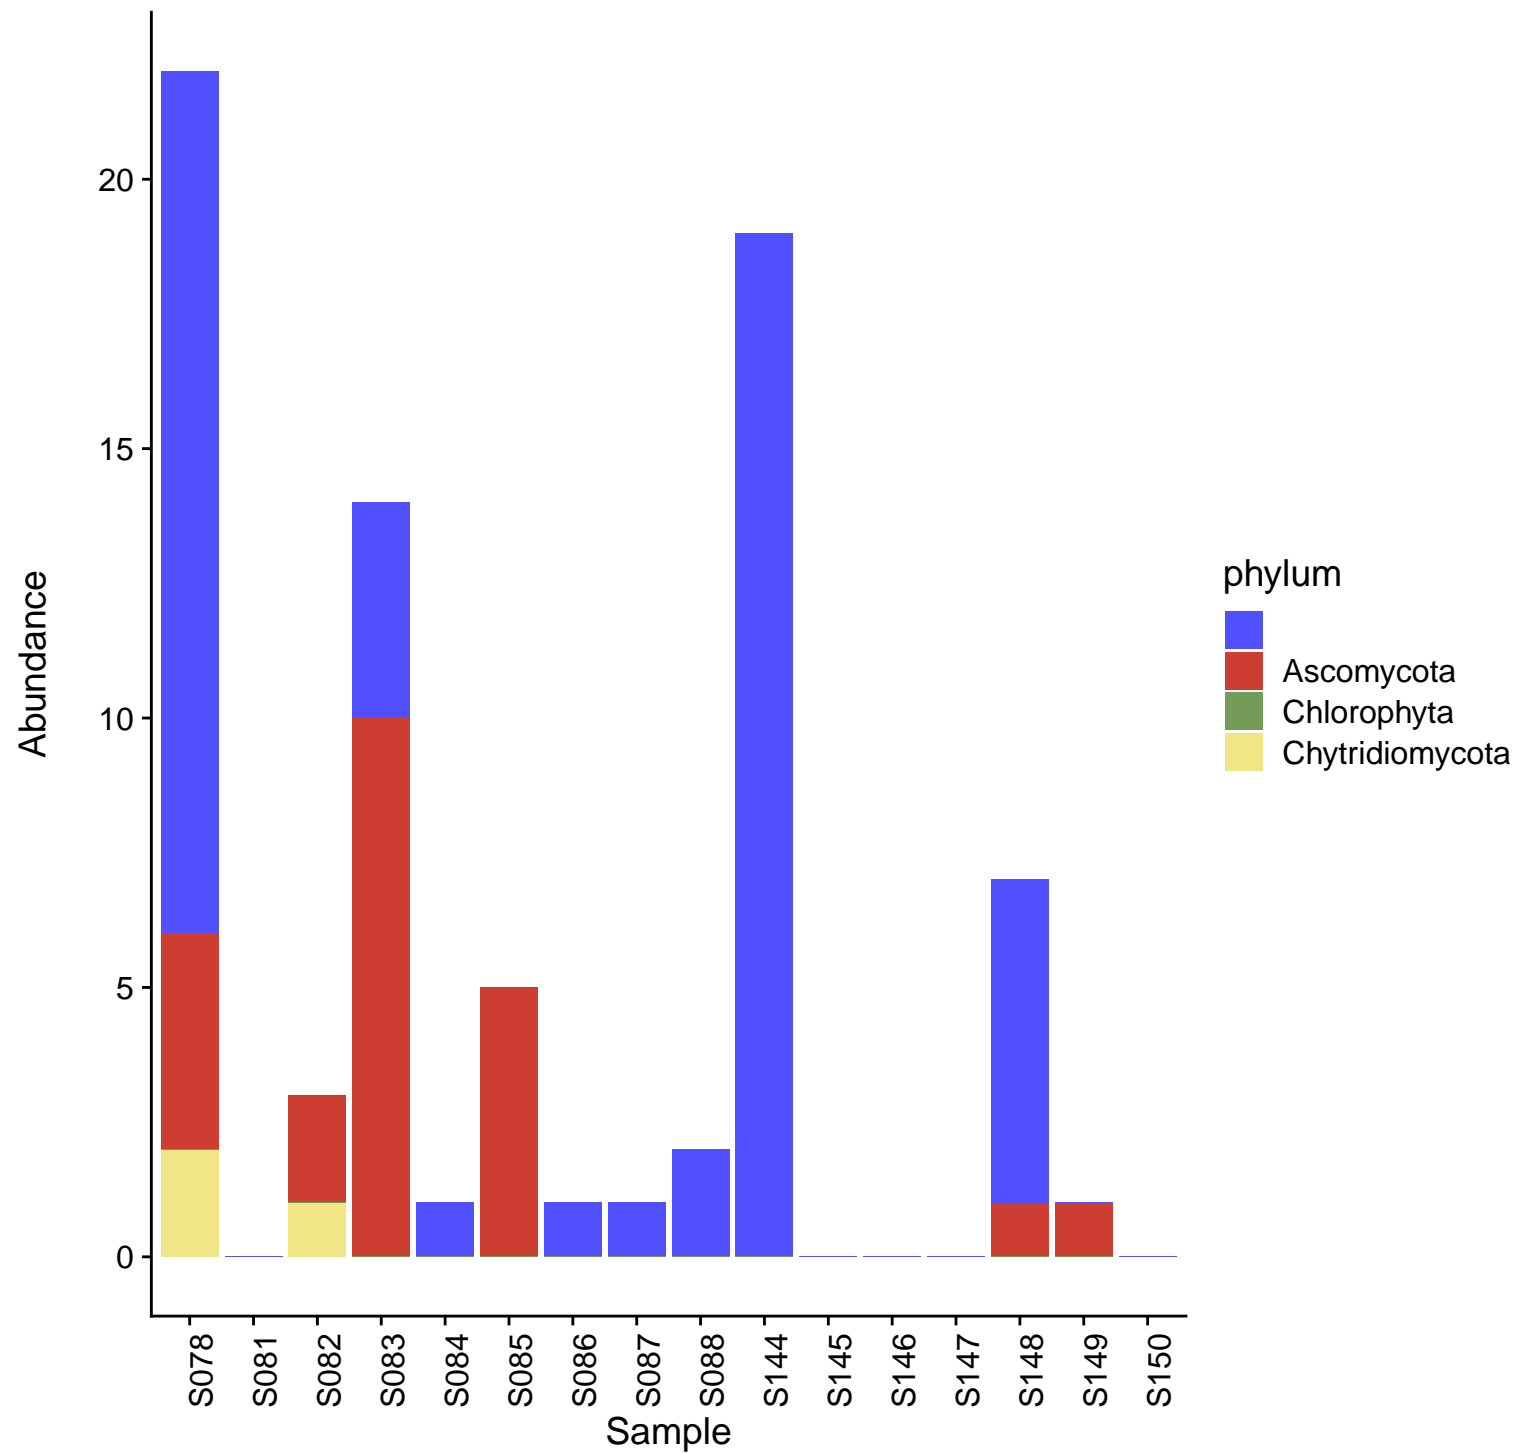