


External Test 1

DenseNet121, n = 108 (62 malignant / 46 benign)

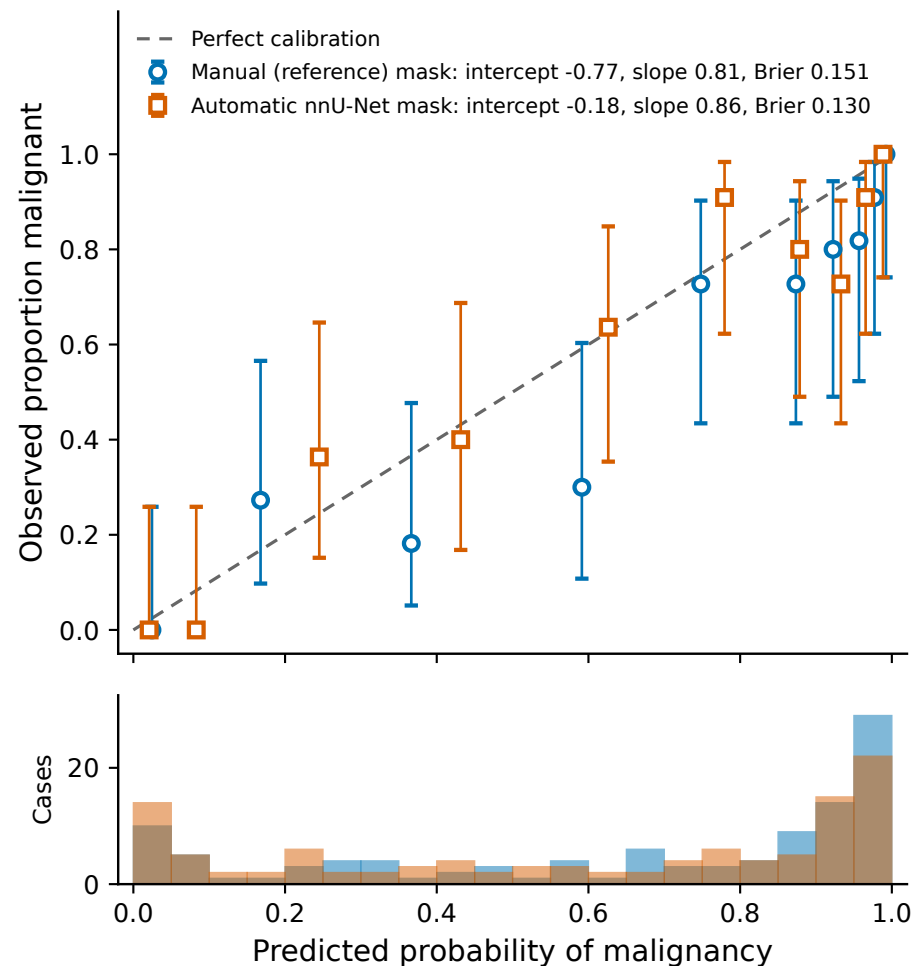

Calibration points use 10 quantile bins (cases per bin Manual (reference) mask: 10-11; Automatic nnU-Net mask: 10-11); error bars are Wilson 95% CI.
Lower panel: distribution of predicted probabilities in 20 fixed-width bins.