


Internal validation (tuning) cohort DenseNet121, n = 257 (155 malignant / 102 benign)

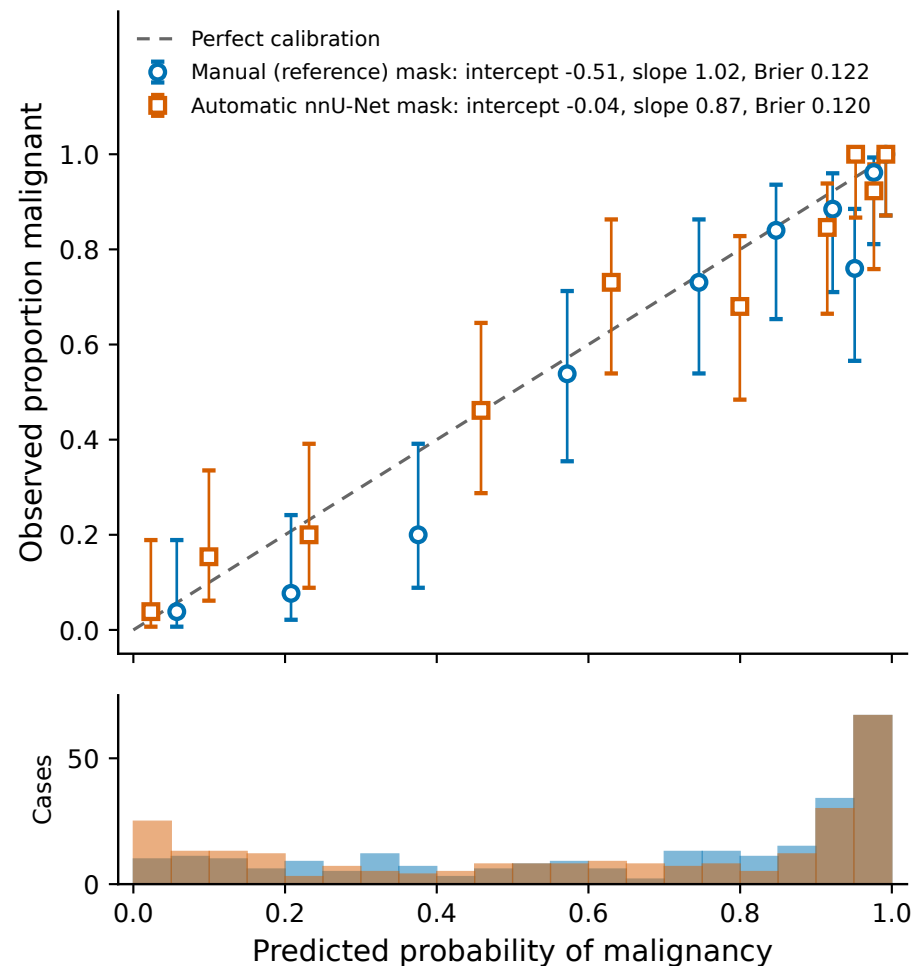

Calibration points use 10 quantile bins (cases per bin Manual (reference) mask: 25-26; Automatic nnU-Net mask: 25-26); error bars are Wilson 95% CI.
Lower panel: distribution of predicted probabilities in 20 fixed-width bins.