


## External Test 2

DenseNet121, n = 94 (67 malignant / 27 benign)

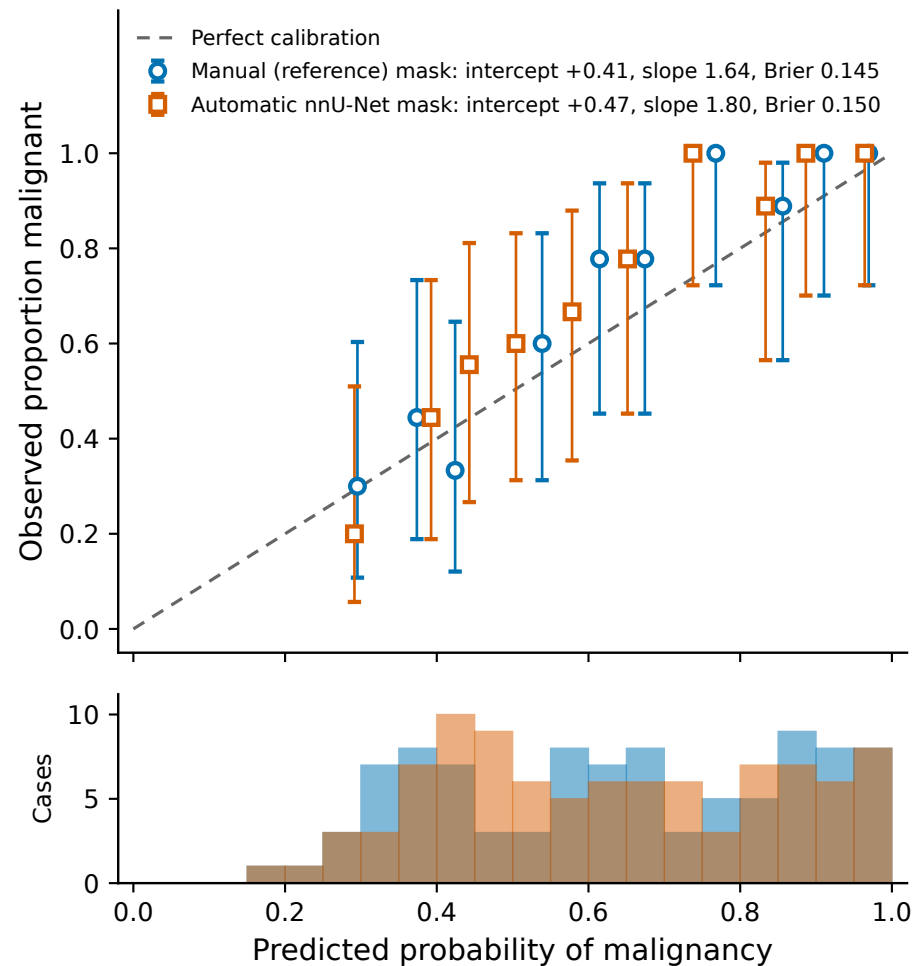

Calibration points use 10 quantile bins (cases per bin Manual (reference) mask: 9-10; Automatic nnU-Net mask: 9-10); error bars are Wilson 95% CI.  
Lower panel: distribution of predicted probabilities in 20 fixed-width bins.