

Supporting Information — QCM frequency and dissipation estimation using DDS excitation, gain–phase detection and complex-admittance reconstruction

openQCM NEXT impedance-analysis working group*

Draft v0.2 — 2026-10-08

Every number in this document is regenerated from the raw data by the scripts in `research/paper/analysis/` (`run_estimators.py`, `run_glucose.py`, `run_v2.py`, `run_bias_theory.py`, `run_forward_model.py`, `make_figures_v2.py`, `make_si.py`); the tables below are written by `make_si.py` from `results/v2/asis/*.csv`. Variant "as acquired" unless stated; the firmware-corrected variant is in `results/v2/fwfix/` and Section S7.

1 Literature comparison, full table

The full comparison table (hardware architecture, sweep method, measured quantities, phase measured, complex Y/Z reconstructed, BVD fitting, Lorentzian fitting, frequency estimator, dissipation estimator, liquid validation, multi-overtone, real-time suitability, computational complexity, cost class), with the verification grade of each entry, is `research/paper/literature/comparison_table.md`; the literature review and the novelty assessment are `literature_review.md` and `novelty_assessment.md` in the same folder. The compact Table 1 of the main text is its first block.

2 Small-load approximation to Kanazawa–Gordon: sources and checks

The derivation of main-text Eqs. (1)–(4) was carried out twice independently (`notes/derivations.md` §6 and `notes/theory_sla_to_kg_check.md`). The points verified against the sources: (i) the SLA normalises the complex shift to the *fundamental* f_F and is applied at the overtone frequency $f_n = nf_F$ inside the load impedance, which is what produces $\Delta f_n \propto \sqrt{n}$ [1, 2]; (ii) with $\exp(i\omega t)$ the imaginary part of the shift is $+\Delta\Gamma$ and the Newtonian impedance is $(1+i)\sqrt{\omega\rho\eta/2}$, so $\Delta\Gamma_n = -\Delta f_n > 0$; (iii) for $n = 1$ Eq. (4) is the relation of Kanazawa and Gordon [3]. Numerical check with $\rho_q = 2648 \text{ kg m}^{-3}$, $\mu_q = 2.947 \times 10^{10} \text{ Pa}$ ($Z_q = 8.83 \times 10^6 \text{ kg m}^{-2} \text{ s}^{-1}$), $f_F = 5\,004\,596 \text{ Hz}$ (DS-2) and $5\,000\,107 \text{ Hz}$ (DS-3): coefficient 715.04 and 714.08 Hz per $\sqrt{n}$ per unit $\sqrt{\rho\eta}$; water ($\sqrt{\rho\eta} = 0.9420 \text{ kg m}^{-2} \text{ s}^{-1/2}$, NIST Chemistry WebBook, IAPWS-95 density and IAPWS 2008 viscosity [4]) 673.6 and 672.7 Hz $\cdot\sqrt{n}$; isopropanol (1.2616, handbook values 781.0 kg m⁻³ and 2.038 mPa s; Kerscher et al. [5] measure 780.9 and 2.07) 902.1 Hz $\cdot\sqrt{n}$ (910 Hz with Kerscher's values). The 2021 tutorial writes the SLA as its Eq. (23) with f_0 the fundamental and derives its Eq. (29), $(-1+i)\sqrt{n}\sqrt{f_0}\sqrt{\rho\eta}/(\sqrt{\pi}Z_q)$, for the Newtonian liquid, which is Eq. (4) of the main text; the 2008 and 1985 primary texts were not reachable from this session and their equation numbers are not cited (see `notes/theory_sla_to_kg_check.md` for the grading). Temperature sensitivity of the prediction: $\partial \ln \sqrt{\rho\eta} / \partial T = -1.15 \text{ \% / K}$ for water near 25 °C (NIST values at 23 and 27 °C) and $-1.6 \text{ \% / K}$ for isopropanol [5], so $\pm 2 \text{ K}$ on the unmeasured liquid temperature is $\pm 2\text{--}3 \text{ \%}$ on Δf_{KG} and $\Delta\Gamma_{\text{KG}}$ and nothing on KG-1 and KG-2. The water constants of the

* Author list and affiliations to be finalised.

earlier internal document (1.102933 g cm⁻³, 0.010665 g cm⁻¹ s⁻¹) would raise the prediction by $\sqrt{1.102933 \cdot 1.0665 / (0.99705 \cdot 0.890)} = 1.151$, i.e. by 15 %; they are not used.

3 The phase reading: fold detection, offset, sign, and the locus

Model and rule. $r(f) = |\phi(f) + \phi_b| - \delta$ (main text, Section 4). The instrument declares a fold when the reading's minimum reaches at least 88 % of the way from its off-resonance level to 0° and sits within 5 Γ of the conductance maximum; the decision is latched over two consecutive sweeps. With a fold, $\delta = -\min r$ is subtracted and the branch past the vertex is negated for B ; without a fold the reading is used unsigned and uncorrected. On DS-2 the fold is present on all overtones in air (vertex from +0.6° at $n = 9$ to -6.4° at $n = 5$, i.e. $\delta = -0.6 \dots +6.4^\circ$), on the fundamental in both liquids, and on none of the overtones $n \geq 3$ in liquid, where the minimum stays 9–45° above zero; on DS-3 the same, with the fold also on $n = 3$ in all four liquids. One sweep of 120 (DS-2, water, $n = 3$, third replica) has a minimum depth of 0.880, exactly at the threshold: the instrument's datalog shows the logged pair alternating between two states 105 Hz and 7.7×10^{-6} apart from 13:12 onwards, and the 0.2 % firmware correction flips its decision (Section S7). This is the fragility of the rule, and it is the one failure observed.

****Why G is even in the sign and not in the offset.**** G depends on ϕ through $\cos \phi$ and $\sin^2 \phi$ only, so the unsigned reading suffices for G and for everything derived from it; B depends on $\sin \phi$ and needs the sign. An additive δ is not removed: $\partial G / \partial \phi \propto \sin \phi$ vanishes at resonance and not on the flanks, so an uncorrected offset distorts the peak shape more than its position; the forward model (S6) gives ≤ 11 Hz on f_{res} (15 Hz where the offset triggers a spurious fold) and ≤ 7 Hz on Γ for $\pm 5^\circ$ in liquid, and an almost one-to-one entry of δ into the fitted angle, $\varphi_{\text{fit}} \approx \phi_b - \delta$.

What the rule must not do. Flipping the sign on a damped load (no fold) splits the locus into two arcs (step of 28–89 % of the range of B); zeroing the minimum on a damped load subtracts 9–45° and takes r_n to 0.5–0.8; estimating δ by making the locus round buys roundness by breaking the trajectory. The repository documents these three failed variants (`research/air-ipa-water-1920-2026-09-11/fold-hypothesis.md`). The locus $B(G)$ is a circle to 1–7 % of its radius in air and 5–18 % in liquid, visibly rotated with respect to the G axis (Fig. S2); the out-of-roundness in liquid coincides with the divider ratio sitting at -22 to -37 dB, the edge of the AD8302's specified range, and with the Möbius distortion of a phase error (S6).

Fold rounding. The smoothing (Savitzky–Golay 51/3 + spline) rounds the V of the fold over 20–50 Hz; on synthetic air-like data the recovered δ is 1.0–1.8° more negative than the true offset, with no effect on f_{res} or Γ when a fold exists. The rounded fold under the narrow air peaks is what leaves the fit residual at 1–3 % of the range in air (Fig. S3) and the closed-form bias of the maximum 5–8 Hz short there (main text Fig. 5).

4 Closed-form biases of the simple estimators for a rotated Lorentzian

With $\Delta = f_{\text{res}} - f$ and $G - G_{\text{off}} = A(\Gamma \cos \varphi - \Delta \sin \varphi) / (\Delta^2 + \Gamma^2)$, $dG/d\Delta = 0 \iff \sin \varphi \Delta^2 - 2\Gamma \cos \varphi \Delta - \Gamma^2 \sin \varphi = 0$, whose maximum is $\Delta_{\text{max}} = \Gamma(\cos \varphi - 1) / \sin \varphi = -\Gamma \tan(\varphi/2)$, hence $f_{G_{\text{max}}} = f_{\text{res}} + \Gamma \tan(\varphi/2)$. The peak height above G_{off} is $(A/\Gamma) \cos^2(\varphi/2)$ and the curve has a negative lobe $-(A/\Gamma) \sin^2(\varphi/2)$ at $\Delta = \Gamma / \tan(\varphi/2)$. The half-height crossings (level $G_{\text{off}} + \text{half the peak height}$, $c = \cos^2(\varphi/2)$) solve $c\Delta^2 + 2\Gamma \sin \varphi \Delta + \Gamma^2(c - 2\cos \varphi) = 0$, $\Delta_{\pm} = \Gamma[-\sin \varphi \pm \sqrt{c(2-c)}] / c$, so $\Gamma_{\text{hh}} = (\Delta_+ - \Delta_-) / 2 = \Gamma \sqrt{(2-c)/c} = \Gamma \sqrt{1 + 2 \tan^2(\varphi/2)}$ and $f_{\text{mid}} = f_{\text{res}} + 2\Gamma \tan(\varphi/2)$. Checked on noise-free model curves on the 1 Hz grid (`results/closed_forms_check.csv`): argmax bias numerical/theory -3.0/-2.8 Hz ($\varphi = -5^\circ$, $\Gamma = 65$ Hz) ... -582/-582 Hz (-40°, 1600 Hz); $\Gamma_{\text{hh}}/\Gamma$ 1.0014/1.0019 ... 1.1198/1.1247; midpoint -5.7/-5.7 ... -1048/-1165 Hz (the midpoint deviates from its closed form at large $|\varphi|$ because the grid and the window truncate the far crossing). A symmetric Lorentzian with

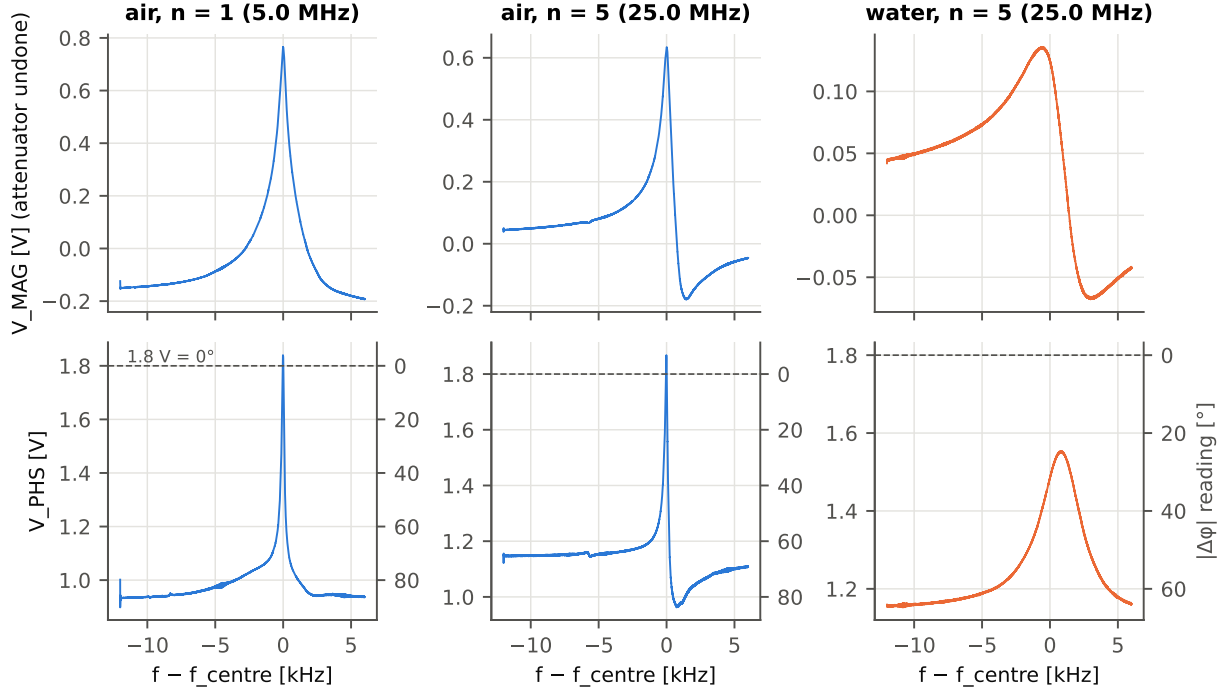


Figure 1: Raw detector voltages for the fundamental and the 5th overtone in air and for the 5th overtone in water (DS-2). Right axis: the unsigned phase reading. In air the reading folds at zero and overshoots it (the signature of δ); in water it does not reach zero.

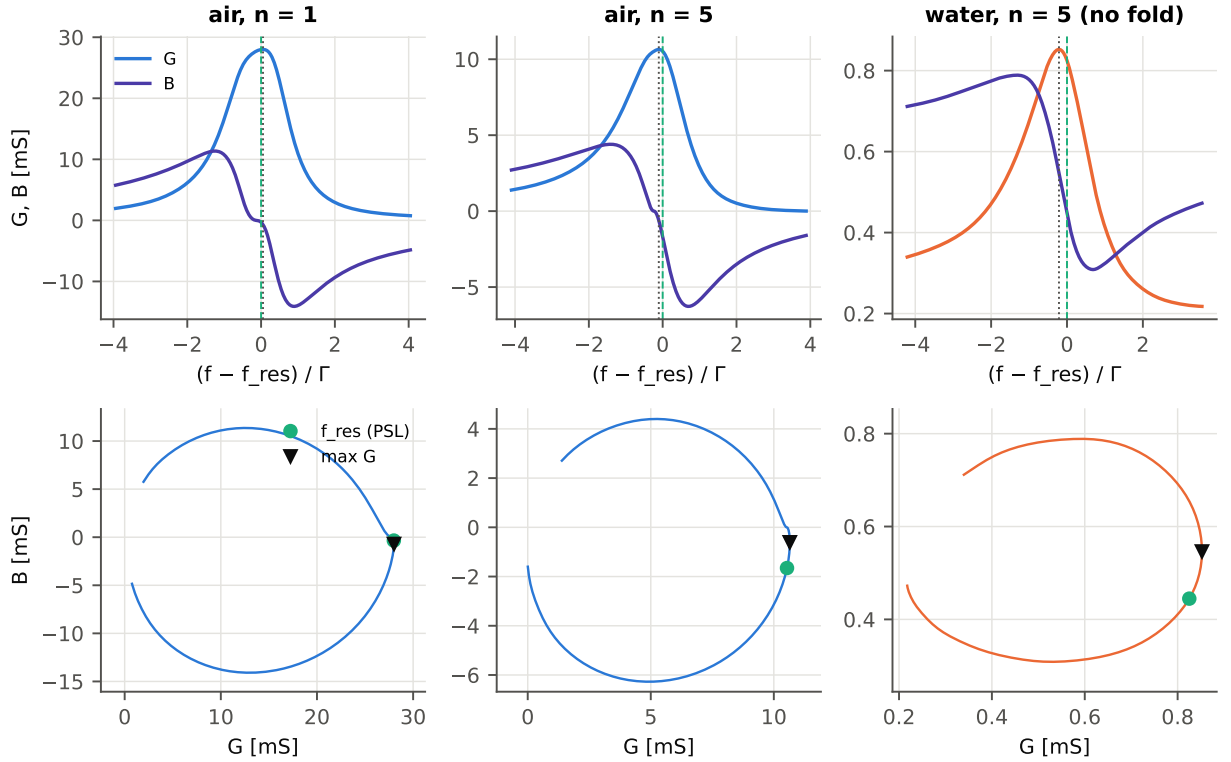


Figure 2: Reconstructed conductance and susceptance (top) and admittance locus (bottom) on $\pm 4 \Gamma$ for the sweeps of Fig. S1. Dotted: the maximum of G ; marker: f_{res} of the phase-shifted fit.

constant background fitted to a rotated one is biased by $1.9\text{--}2.1 \Gamma \tan(\varphi/2)$ in frequency and over-estimates Γ by 2–35 % between -8° and -28° ; with a linear background Γ is right to 0.2 % and the frequency bias is $\approx 1.25 \Gamma \tan(\varphi/2)$.

Sign convention. Johannsmann et al. print Eq. 13 with $+\Delta \sin \varphi$ in G and $+\Delta \cos \varphi$ in B ; with one φ in both lines that is not a single rotation (the lines correspond to φ and $-\varphi$). Fitting G alone, the two conventions are observationally identical and differ only in the sign quoted for φ ; the main text uses the rotation form, in which the fitted angle is negative on both boards and the maximum of G lies below f_{res} . On the data the measured $f_{G_{\text{max}}} - f_{\text{res}}$ is negative on every liquid sweep and on every air sweep with $n \geq 3$ (Table S8), as the convention requires.

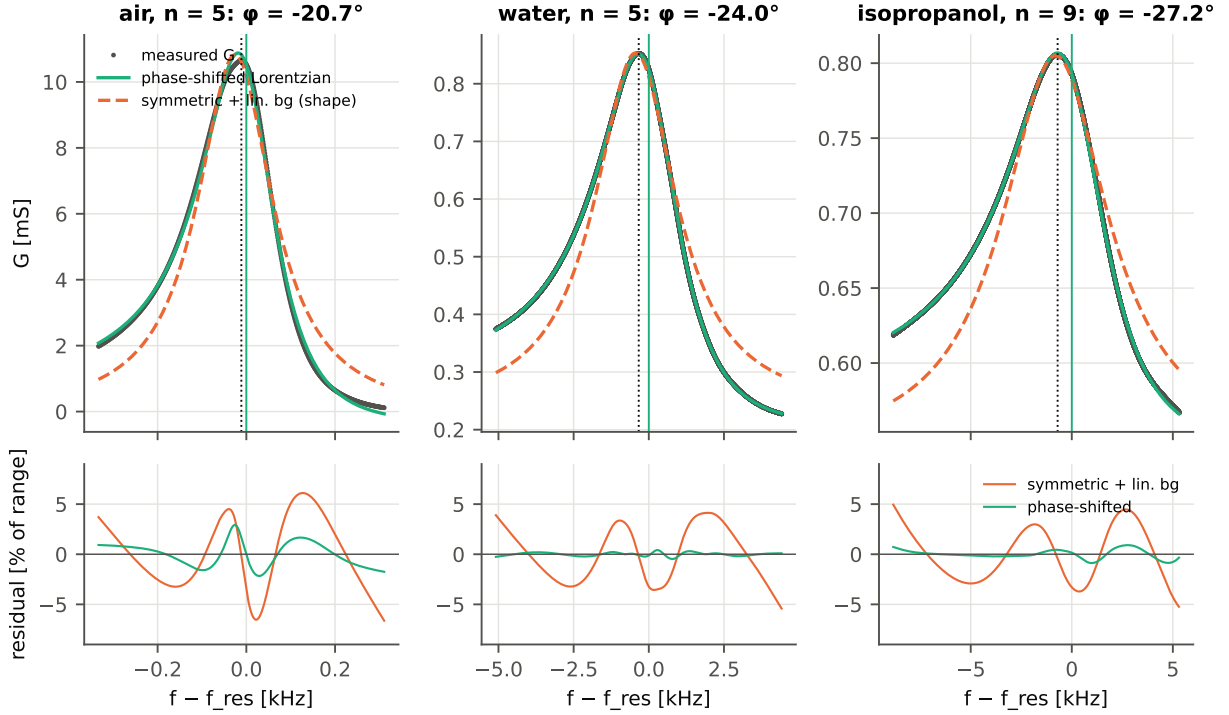


Figure 3: Conductance (dots) with the phase-shifted Lorentzian (solid) and the symmetric Lorentzian with linear background (dashed) on $\pm 3 \Gamma_{\text{hh}}$ for three sweeps of DS-2; below, the residuals in percent of the range of G .

5 Fitting: window, initialisation, acceptance gate, fallback rate, residuals, repeatability

Window $|f - f_{G_{\text{max}}}| \leq 3\Gamma_{\text{hh}}$ (clipped by the sweep edge on the right for $n \geq 5$ in isopropanol, 2.2–3.0 Γ available, and at $n = 9$ in DS-3, 2.8–2.9 Γ in water and 2.5–2.6 Γ in the glucose solutions); seeds $f_{G_{\text{max}}}$, Γ_{hh} , $\varphi = 0$, $G_{\text{off}} = \min G$, $G_{\text{max}} = \text{range of } G$; frequencies scaled to kHz about the seed and conductances to mS; Levenberg–Marquardt with tolerances 10^{-12} . Gate (instrument constants): convergence, f_{res} inside the window, $0.3 \leq \Gamma/\Gamma_{\text{hh}} \leq 3$, $|\varphi| \leq 60^\circ$, rms residual ≤ 5 % of the range; the limits were set at about ten times the observed values on DS-2 and never fired: 45/45 fits of DS-2 and 75/75 of DS-3 converged and were accepted (fallback rate 0 %). Residuals (rms, percent of the range of G): phase-shifted 1.0–2.7 % in air and 0.15–0.65 % in liquid on DS-2, 0.9–1.4 % and 0.2–0.8 % on DS-3; symmetric Lorentzian with linear background 3.0–4.2 % and 0.8–3.5 % (DS-2), 1.8–4.2 % and 0.7–3.8 % (DS-3), always S-shaped (Fig. S3). The fit’s covariance gives 0.1–0.8 Hz on f_{res} , an order of magnitude below the replica scatter, because the residual is structured; the replica scatter is the number quoted. Repeatability over the three sweeps of a plateau (Fig. S4): DS-2, f_{res} 1.5–23 Hz in air (the air baseline was still drifting at -0.3 to -2

Hz/min) and 0.3–29 Hz in liquid, $\Gamma \leq 2.3$ Hz in air and ≤ 38 Hz in liquid (the two-state sweep; ≤ 13 Hz otherwise); DS-3, $f_{\text{res}} \leq 2.4$ Hz in air and ≤ 7.6 Hz in liquid, $\Gamma \leq 0.7$ and ≤ 4.5 Hz. The magnitude estimator's -3 dB width is undefined inside the window on 15 of 45 (DS-2) and 33 of 75 (DS-3) sweeps; the half-height width of G is two-sided on all 120.

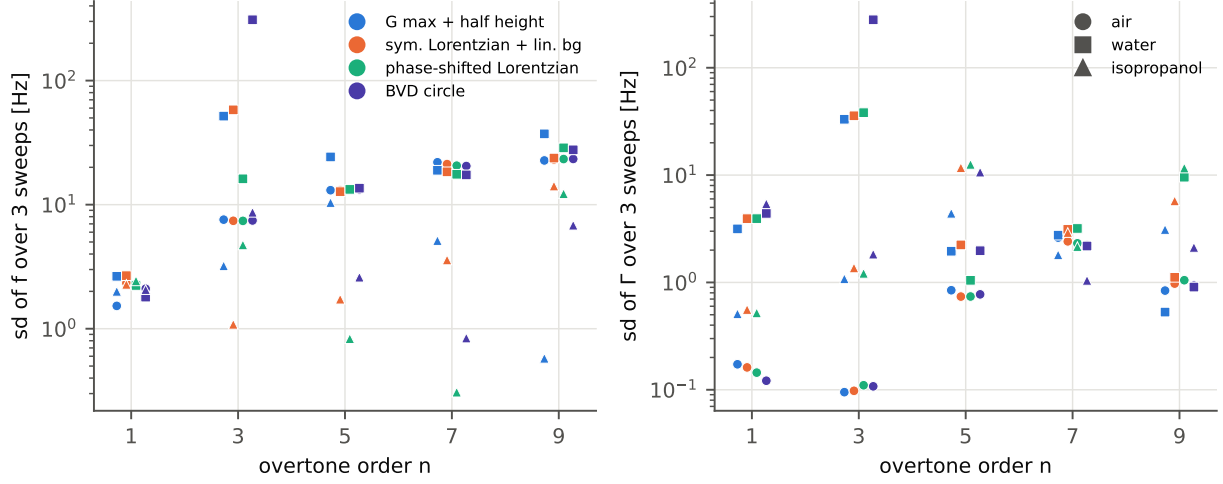


Figure 4: Standard deviation over the three plateau sweeps of f_{res} (left) and Γ (right) per estimator, overtone and load, DS-2.

6 Forward model, board phase, resistive standards

A board phase does not multiply the admittance; it multiplies the measured transfer function, $H_{\text{meas}} = H e^{j\phi_b}$. Inverting exactly with that phase gives $Y' = 1/[(Z_{\text{el}} + R_{17})e^{-j\phi_b} - R_{17}]$, a Möbius transformation of $Y_{\text{el}} = 1/Z_{\text{el}}$ that reduces to the rotation $Y_{\text{el}}e^{j\phi_b}$ only when $|Z_{\text{el}}| \gg R_{17}$. A Butterworth–Van Dyke crystal of known f_s , Γ , R_1 , C_0 was sent through the divider and the detector laws with a board phase on $\angle H$, an offset δ , the fold, the ADC quantisation and the firmware carry-over, and through the same chain and estimators (`run_forward_model.py`, `results/forward_model.md`). Findings: (i) the fitted angle equals the imposed board phase to 0.7° on the liquid-like cases and to 1° on the air-like ones, except the one case where the offset triggers a spurious fold; (ii) with $\phi_b = 0$ both estimators recover f_s to the grid; (iii) with $\phi_b = -8$ to -25° the maximum of G is off by -91 to -743 Hz on liquid-like cases, the phase-shifted fit by -9 to -59 Hz ($\leq 2\%$ of Γ), the symmetric fit by -96 to -833 Hz; (iv) the residual of the phase-shifted fit scales as $\approx -0.34 \Gamma (R_{17}/R_1)$ at $\phi_b = -20^\circ$: -344 Hz at $R_1 = R_{17}$ and -12 Hz at $1.6 \text{ k}\Omega$ for $\Gamma = 1 \text{ kHz}$, so for air-like cases ($\Gamma = 65\text{--}190$ Hz, $R_1 = 36\text{--}204 \Omega$) -12 to -39 Hz, a third to a half of the argmax bias for $R_1/R_{17} \geq 1.8$ and three quarters or more at $R_1/R_{17} = 0.7$; (v) with a fold, δ is removed and does not move f_{res} or Γ (≤ 0.5 Hz for $\delta = -3 \dots +7^\circ$); (vi) without a fold, $\pm 5^\circ$ of δ enters the fitted angle almost one to one and moves f_{res} by ≤ 11 Hz (15 Hz where a spurious fold is declared) and Γ by ≤ 7 Hz; (vii) $\pm 5\%$ on the magnitude slope moves f_{res} by ≤ 17 Hz and Γ by $\leq 1\%$, but $R_m = 1/G_{\text{max}}$ by 6–16 %, and even with an ideal magnitude channel R_m is 24–39 % low in liquid; (viii) the firmware carry-over moves f_{res} by ≈ 2 Hz; (ix) the smoothing widens a 65 Hz half-bandwidth by 6.5 Hz (+10 %) and a 190 Hz one by 3.5 Hz, negligible in liquid.

The repository's two-channel forward model, which fits a BVD crystal through the divider and the detector laws to V_{MAG} and V_{PHS} jointly with a board phase inside the modulus, gives $\phi_b = -7.6, -13.8, -19.9, -22.1, -20.4^\circ$ in air on board 1920, equal to the P angle within $0.4\text{--}0.8^\circ$ on $n = 1\text{--}7$. The short and 50Ω standards measured on the same front end (1–51 MHz) give phase slopes of $0.27\text{--}0.40^\circ \text{ MHz}^{-1}$ (0.74–1.10 ns), i.e. $1.4\text{--}2.0^\circ$ at 5 MHz and $12\text{--}18^\circ$ at 45 MHz, and read M 4–16 % low (8–14 % at 5 MHz); the fitted angle grows roughly as $f^{0.55}$ (Fig. S11). A

least-squares decomposition $\varphi = \varphi_0 - 360^\circ f \tau$ gives $\varphi_0 = -7.0^\circ$, $\tau = 1.28$ ns (rms 1.2°) for board 1920 in air and $\varphi_0 = -8.2^\circ$, $\tau = 1.31$ ns (rms 2.6°) for the second instrument, an approximation whose parameters move when $n = 1$ is excluded.

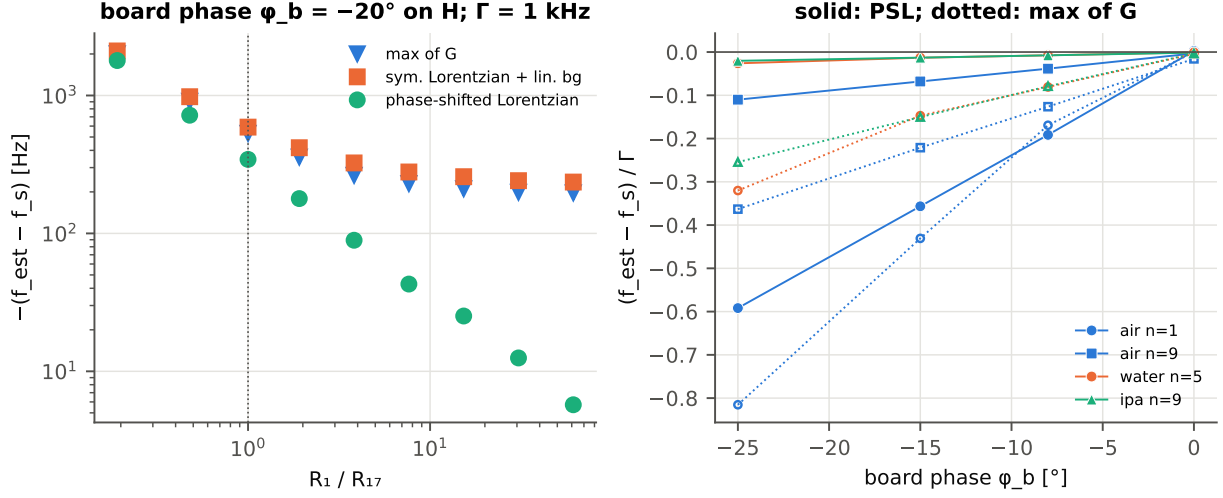


Figure 5: Forward model. Left: error of three estimators against R_1/R_{17} for a board phase of -20° on the transfer function ($\Gamma = 1$ kHz). Right: error in units of Γ against the board phase for four measured-like cases; solid: phase-shifted fit; dotted: maximum of G .

7 Firmware carry-over

Firmware versions up to 0.1.5c did not reset the per-point sums, so each printed point carried $1/500$ of the previous one ($+0.2\%$ on the counts). The recursion is exact and was undone offline on the counts ($m_i = v_i - v_{i-1}/500$). On DS-2 it changes f_{res} by ≤ 2.2 Hz and Γ by ≤ 1.7 Hz on 43 of 45 sweeps with P and φ by $\leq 0.2^\circ$; the exceptions are the threshold sweep of S3, whose fold decision flips ($f_{\text{res}} + 37$ Hz with P, $+111$ Hz with A; $\varphi + 4.3^\circ$), and one water sweep at $n = 9$ ($+10$ Hz on f_{res} , -18 Hz on Γ). With A the changes are larger (≤ 2 Hz on 21 of 45 sweeps, up to 111 Hz). On DS-3 it changes f_{res} by ≤ 2 Hz (P; ≤ 6 Hz with A), Γ by ≤ 2 Hz and φ by $\leq 0.2^\circ$. Over the 120 sweeps the fit moves by ≤ 2 Hz on 115 and by ≤ 4 Hz on 118. The A and P ranges of Table 2 move by ≤ 2 percentage points (the M rows by up to 3.4) (corrected variant: DS-2 P $\epsilon_f = -1.6 \dots +7.8\%$, $\epsilon_\Gamma = -4.3 \dots +7.3\%$; DS-3 P $+6.0 \dots +13.0\%$, $-4.4 \dots +4.6\%$); the bias law gives $+14 \pm 30$ Hz on 120 sweeps. Fig. S6 shows the differences on the shifts.

8 The raw-magnitude baseline and the production datalogs

Magnitude-only estimator from the sweeps (M). Maximum of the divider ratio in dB on the same grid and its -3 dB full width where it exists (Table S3 and Fig. S7): $\epsilon_f = +52 \dots +92\%$ (DS-2) and $+50 \dots +116\%$ (DS-3) on $n = 3-9$, growing with the overtone; the width is undefined inside the window for $n \geq 7$ in liquid and reaches 6 kHz at $n = 5$. **Production datalog of board 1920** (same instants as the impedance datalog, Fig. S8): maximum of the baseline-corrected magnitude and its -0.3 dB width; on the last 10 min of each plateau of 2026-09-11 (95 of 486 rows were exact duplicates written in bursts and were dropped) $\epsilon_f = +51, +69, +76, +89\%$ (water, $n = 3-9$) and $+57, +74, +85, +90\%$ (isopropanol), against $+23, +29, +22, +18\%$ and $+22, +27, +22, +22\%$ for the live A estimator; the -0.3 dB width changes by $0.8-3.7$ kHz (water) and $1.1-6.4$ kHz (isopropanol) where the theory's $\Delta\Gamma$ is $1.2-2.7$ kHz. The 2026-09-10 run (2.5 min plateaus, 36 of 175 rows duplicated) gives $+51 \dots +98\%$ and $+22 \dots +30\%$. The live A estimator reproduces the offline analysis of the dumped sweeps within the plateau drift (Table S11).

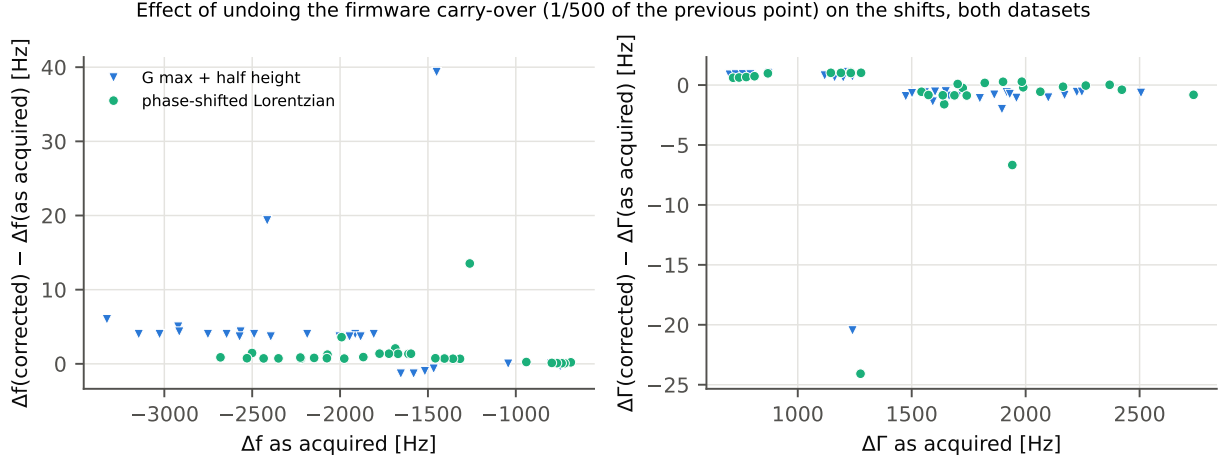


Figure 6: Difference of the air-to-liquid shifts between the firmware-corrected and the as-acquired variants, both datasets, estimators A and P.

Error metrics on overtones 3–9 for six estimators; M: magnitude maximum, A: max G + half height, MP: midpoint, S+: symmetric + linear bg, C: BVD circle, P: phase-shifted Lorentzian

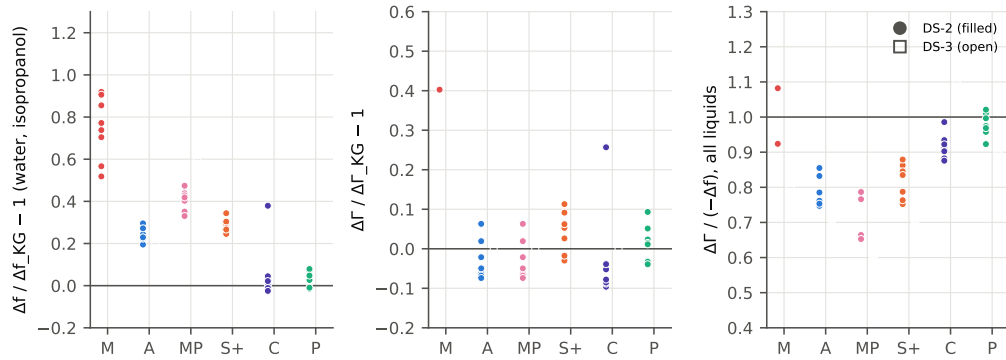


Figure 7: Error metrics on overtones 3–9 for six estimators on both datasets: ϵ_f , ϵ_Γ (water and isopropanol) and r_n (all liquids).

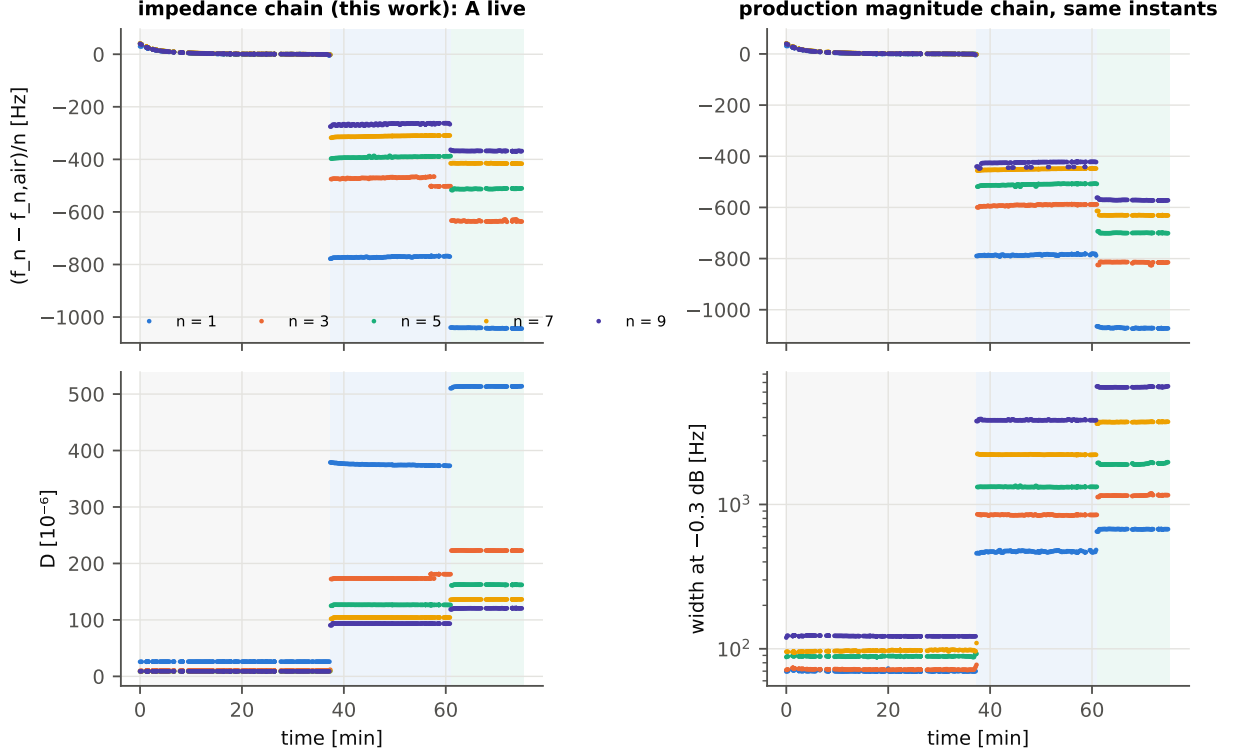


Figure 8: The run of 2026-09-11 as logged by the instrument: the impedance chain (left; A live) and the production magnitude chain at the same instants (right); overtone-normalised frequency relative to the air plateau, dissipation factor, and the production -0.3 dB width.

9 Glucose series: concentration lines, the 5 % offset, the fit window

Relative to water, the fitted resonance moves by -72 Hz (fundamental) to -307 Hz (9th) at 10 % w/v (-17 to -128 Hz at 5 %) and broadens by $+94$ to $+379$ Hz at 10 %; lines through the four concentrations have slopes -7.1 , -13.8 , -17.8 , -24.7 , -30.4 Hz per % w/v in Δf_n and $+9.2$, $+13.1$, $+16.6$, $+28.0$, $+37.8$ Hz per % in $\Delta \Gamma_n$ (Fig. S9). The 5 % plateau is less loaded than the line on every overtone: $+10$ to $+18$ Hz in Δf and -9 to -14 Hz in $\Delta \Gamma$, constant in hertz over n rather than $\propto \sqrt{n}$, so not an error of $\rho\eta$. Drift cannot explain it: the slope of f_{res} over the three replicas is ≤ 0.4 Hz/min inside the glucose plateaus and -0.2 to -1.0 Hz/min in water, the 5 % plateau is 4.3 min off the line of plateau times against concentration, so a time-linear drift maps into at most ≈ 4 Hz, and explaining the residual by drift alone would need -2 to -4 Hz/min, three to sixteen times what is measured (`results/glucose_tables_asis.md`). Without a return to water between concentrations the experiment cannot tell a property of the first solution from a step of the instrument. The ratio $\rho\eta/(\rho\eta)_w$ from the bandwidth exceeds that from the frequency on $n = 7$ and 9 (1.36 and 1.42 against 1.27 and 1.30 at 10 %); the $\pm 3\Gamma$ fit window is clipped by the sweep edge there (2.5–2.6 Γ on the right at $n = 9$), and refitting with a symmetric window limited by the edge moves the $n = 9$ ratio from 1.418 to 1.395, a fifth of the gap, and nothing at $n = 7$; the rest is unexplained. A roughness term, which in the Daikhin–Urbakh description adds to Δf without a counterpart in $\Delta \Gamma$ [6, 7], would act in the opposite direction and is not supported.

10 Tables

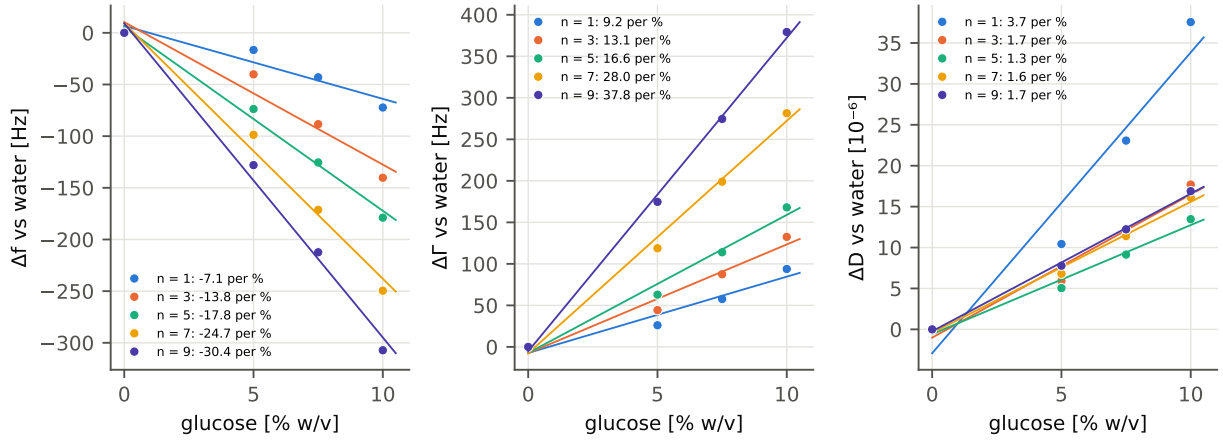


Figure 9: Shifts relative to water of the fitted resonance frequency, half-bandwidth and dissipation against glucose concentration, one line per overtone (least squares with intercept).

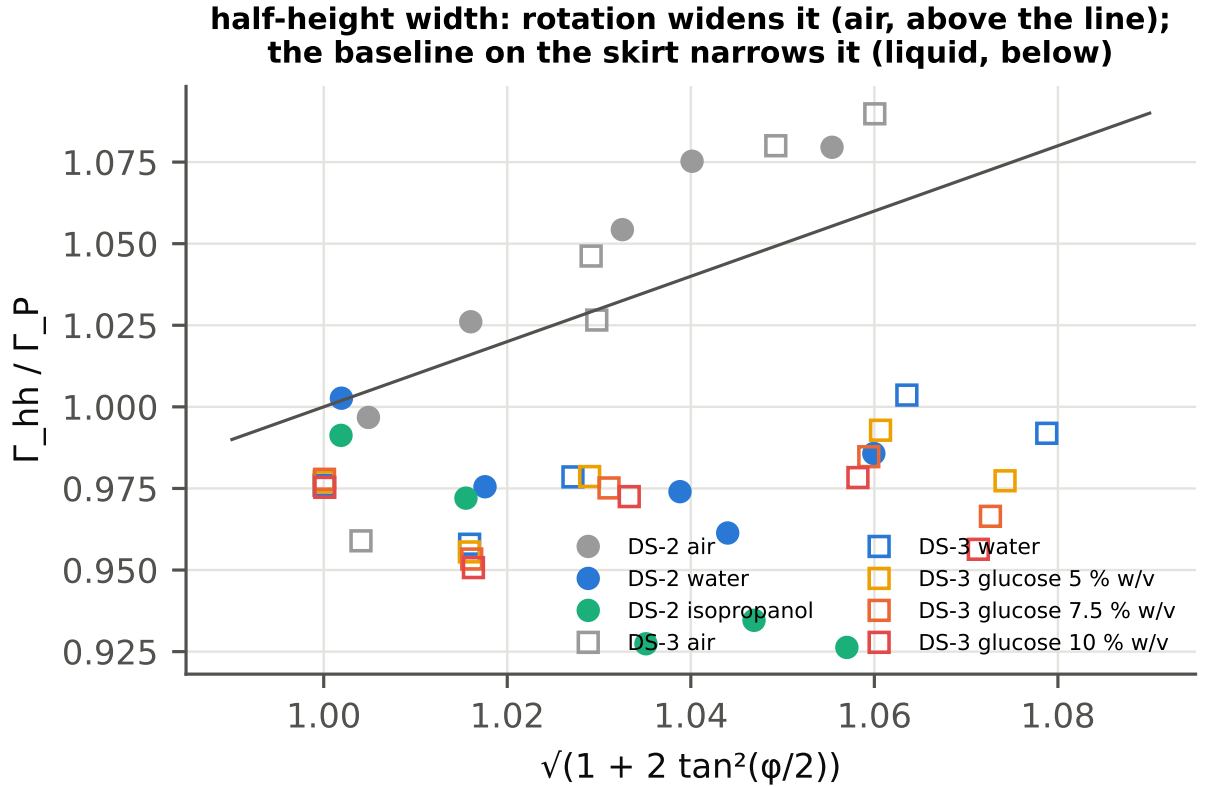


Figure 10: The half-height width against the fitted Γ : rotation widens it (air, above the identity), the baseline on the skirt narrows it (liquid, below).

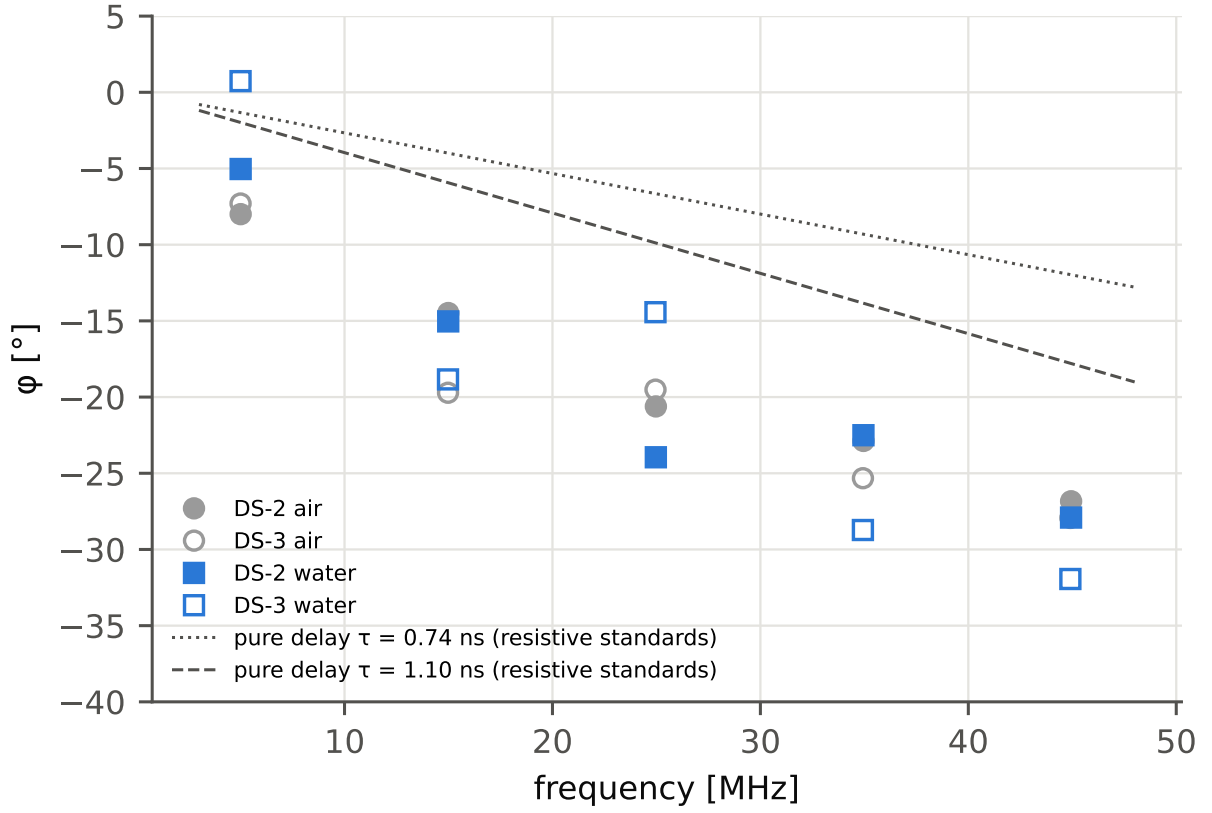


Figure 11: The rotation angle against frequency for air and water on both instruments, with the phase of a pure delay for the two delays measured on the resistive standards of board 1920.

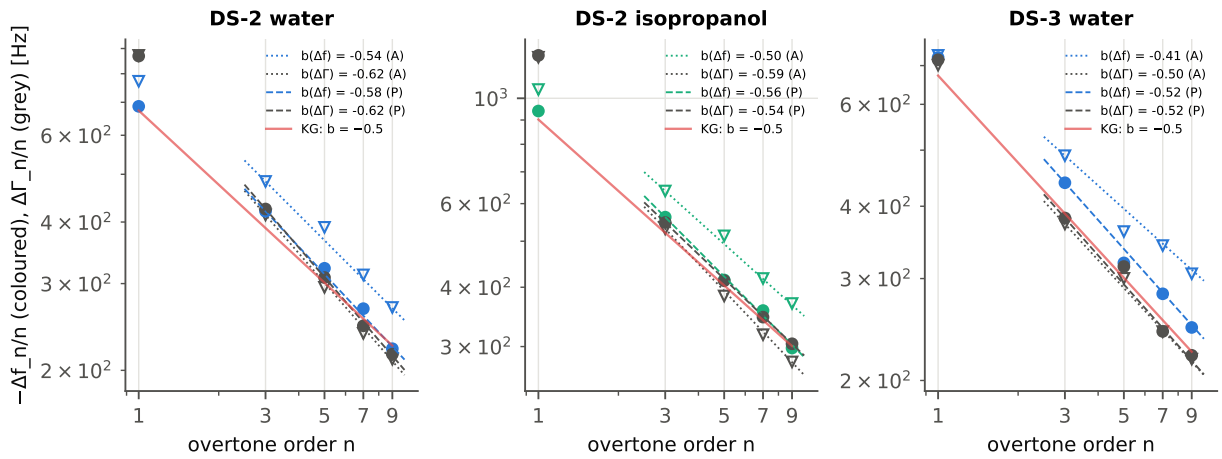


Figure 12: KG-2 on log-log axes: $-\Delta f_n/n$ and $\Delta \Gamma_n/n$ against n for A and P with the fitted slopes on $n = 3-9$ and the KG line of slope $-1/2$.

Table 1: Resonance frequency, half-bandwidth, dissipation and rotation angle per dataset, medium and overtone (mean $\pm$ sd of three sweeps). A = maximum of G + half height; P = phase-shifted Lorentzian; fold = number of sweeps on which the phase reading folds.

dataset	medium	n	f (A) [Hz]	f (P) [Hz]	Γ (A) [Hz]	Γ (P) [Hz]	D (A) [10^{-6}]	D (P) [10^{-6}]	φ (P) [$^\circ$]	fold
DS-2	air	1	5004598 $\pm$ 2	5004596 $\pm$ 2	65.4 $\pm$ 0.2	65.6 $\pm$ 0.1	26.1	26.2	-8.0 $\pm$ 0.05	3/3
DS-2	air	3	14988738 $\pm$ 8	14988740 $\pm$ 7	78.0 $\pm$ 0.1	76.0 $\pm$ 0.1	10.4	10.1	-14.5 $\pm$ 0.03	3/3
DS-2	air	5	24973688 $\pm$ 13	24973699 $\pm$ 13	108.0 $\pm$ 0.8	102.4 $\pm$ 0.7	8.6	8.2	-20.6 $\pm$ 0.06	3/3
DS-2	air	7	34957566 $\pm$ 22	34957593 $\pm$ 21	158.7 $\pm$ 2.6	147.6 $\pm$ 2.3	9.1	8.4	-22.9 $\pm$ 0.04	3/3
DS-2	air	9	44943110 $\pm$ 23	44943157 $\pm$ 23	203.7 $\pm$ 0.8	188.7 $\pm$ 1.0	9.1	8.4	-26.8 $\pm$ 0.00	3/3
DS-2	water	1	5003826 $\pm$ 3	5003909 $\pm$ 2	937.0 $\pm$ 3.2	934.5 $\pm$ 3.9	374.5	373.5	-5.0 $\pm$ 0.02	3/3
DS-2	water	3	14987288 $\pm$ 52	14987478 $\pm$ 16	1318.2 $\pm$ 33.1	1351.4 $\pm$ 38.2	175.9	180.3	-15.0 $\pm$ 2.45	1/3
DS-2	water	5	24971737 $\pm$ 24	24972088 $\pm$ 13	1582.0 $\pm$ 2.0	1645.6 $\pm$ 1.0	126.7	131.8	-24.0 $\pm$ 0.04	0/3
DS-2	water	7	34955379 $\pm$ 19	34955726 $\pm$ 18	1822.9 $\pm$ 2.8	1871.6 $\pm$ 3.2	104.3	107.1	-22.5 $\pm$ 0.05	0/3
DS-2	water	9	44940695 $\pm$ 37	44941165 $\pm$ 29	2099.7 $\pm$ 0.5	2130.1 $\pm$ 9.6	93.4	94.8	-27.9 $\pm$ 0.23	0/3
DS-2	isopropanol	1	5003555 $\pm$ 2	5003656 $\pm$ 2	1285.6 $\pm$ 0.5	1296.9 $\pm$ 0.5	513.9	518.4	-5.0 $\pm$ 0.02	3/3
DS-2	isopropanol	3	14986825 $\pm$ 3	14987054 $\pm$ 5	1670.5 $\pm$ 1.1	1718.6 $\pm$ 1.2	222.9	229.3	-14.2 $\pm$ 0.18	0/3
DS-2	isopropanol	5	24971122 $\pm$ 10	24971627 $\pm$ 1	2025.1 $\pm$ 4.4	2166.8 $\pm$ 12.6	162.2	173.5	-24.7 $\pm$ 0.17	0/3
DS-2	isopropanol	7	34954645 $\pm$ 5	34955093 $\pm$ 0	2383.2 $\pm$ 1.8	2569.8 $\pm$ 2.2	136.4	147.0	-21.4 $\pm$ 0.11	0/3
DS-2	isopropanol	9	44939783 $\pm$ 1	44940476 $\pm$ 12	2709.8 $\pm$ 3.1	2925.5 $\pm$ 11.6	120.6	130.2	-27.2 $\pm$ 0.04	0/3
DS-3	air	1	5000106 $\pm$ 1	5000107 $\pm$ 1	110.0 $\pm$ 0.7	114.7 $\pm$ 0.7	44.0	45.9	-7.3 $\pm$ 0.13	3/3
DS-3	air	3	14977476 $\pm$ 0	14977481 $\pm$ 0	52.6 $\pm$ 0.1	51.3 $\pm$ 0.1	7.0	6.8	-19.7 $\pm$ 0.02	3/3
DS-3	air	5	24955252 $\pm$ 1	24955258 $\pm$ 1	70.0 $\pm$ 0.1	66.9 $\pm$ 0.1	5.6	5.4	-19.5 $\pm$ 0.02	3/3
DS-3	air	7	34931726 $\pm$ 2	34931742 $\pm$ 2	106.2 $\pm$ 0.3	98.3 $\pm$ 0.2	6.1	5.6	-25.3 $\pm$ 0.05	3/3
DS-3	air	9	44909699 $\pm$ 3	44909726 $\pm$ 2	152.3 $\pm$ 0.1	139.8 $\pm$ 0.1	6.8	6.2	-27.9 $\pm$ 0.05	3/3
DS-3	water	1	4999377 $\pm$ 3	4999384 $\pm$ 1	811.1 $\pm$ 1.4	831.0 $\pm$ 1.5	324.5	332.5	0.7 $\pm$ 0.03	3/3
DS-3	water	3	14976009 $\pm$ 3	14976163 $\pm$ 3	1170.8 $\pm$ 1.3	1196.4 $\pm$ 1.9	156.4	159.8	-18.8 $\pm$ 0.03	3/3
DS-3	water	5	24953443 $\pm$ 5	24953662 $\pm$ 4	1571.3 $\pm$ 1.1	1640.4 $\pm$ 0.6	125.9	131.5	-14.4 $\pm$ 0.02	0/3
DS-3	water	7	34929332 $\pm$ 3	34929765 $\pm$ 5	1806.6 $\pm$ 2.3	1800.1 $\pm$ 0.1	103.4	103.1	-28.7 $\pm$ 0.01	0/3
DS-3	water	9	44906947 $\pm$ 36	44907503 $\pm$ 8	2111.9 $\pm$ 2.4	2129.1 $\pm$ 4.5	94.1	94.8	-31.9 $\pm$ 0.03	0/3
DS-3	glucose 5 %	1	4999359 $\pm$ 2	4999367 $\pm$ 0	837.5 $\pm$ 0.4	857.1 $\pm$ 0.8	335.0	342.9	0.9 $\pm$ 0.01	3/3
DS-3	glucose 5 %	3	14975959 $\pm$ 2	14976123 $\pm$ 0	1214.3 $\pm$ 0.2	1240.7 $\pm$ 0.2	162.2	165.7	-19.5 $\pm$ 0.01	3/3
DS-3	glucose 5 %	5	24953369 $\pm$ 3	24953588 $\pm$ 1	1627.6 $\pm$ 2.4	1703.3 $\pm$ 0.5	130.5	136.5	-14.4 $\pm$ 0.00	0/3
DS-3	glucose 5 %	7	34929237 $\pm$ 4	34929667 $\pm$ 1	1905.2 $\pm$ 0.8	1918.9 $\pm$ 0.3	109.1	109.9	-28.1 $\pm$ 0.01	0/3
DS-3	glucose 5 %	9	44906784 $\pm$ 7	44907375 $\pm$ 1	2251.6 $\pm$ 4.0	2303.8 $\pm$ 0.8	100.3	102.6	-31.0 $\pm$ 0.04	0/3
DS-3	glucose 7.5 %	1	4999332 $\pm$ 3	4999341 $\pm$ 0	869.0 $\pm$ 0.2	888.7 $\pm$ 0.9	347.6	355.5	1.1 $\pm$ 0.01	3/3
DS-3	glucose 7.5 %	3	14975895 $\pm$ 4	14976075 $\pm$ 1	1252.1 $\pm$ 0.3	1284.0 $\pm$ 0.5	167.2	171.5	-20.2 $\pm$ 0.01	3/3
DS-3	glucose 7.5 %	5	24953306 $\pm$ 5	24953536 $\pm$ 1	1672.6 $\pm$ 1.8	1754.4 $\pm$ 0.8	134.1	140.6	-14.5 $\pm$ 0.01	0/3
DS-3	glucose 7.5 %	7	34929154 $\pm$ 14	34929594 $\pm$ 1	1968.6 $\pm$ 1.1	1999.1 $\pm$ 0.2	112.7	114.5	-27.8 $\pm$ 0.00	0/3
DS-3	glucose 7.5 %	9	44906672 $\pm$ 3	44907291 $\pm$ 0	2323.1 $\pm$ 5.7	2403.7 $\pm$ 1.4	103.5	107.1	-30.7 $\pm$ 0.02	0/3
DS-3	glucose 10 %	1	4999304 $\pm$ 3	4999311 $\pm$ 0	902.1 $\pm$ 0.7	924.9 $\pm$ 0.9	360.9	370.0	1.2 $\pm$ 0.01	3/3
DS-3	glucose 10 %	3	14975822 $\pm$ 2	14976023 $\pm$ 0	1292.4 $\pm$ 0.9	1329.0 $\pm$ 0.8	172.6	177.5	-20.8 $\pm$ 0.03	3/3
DS-3	glucose 10 %	5	24953248 $\pm$ 3	24953483 $\pm$ 1	1719.4 $\pm$ 1.6	1808.4 $\pm$ 0.8	137.8	144.9	-14.6 $\pm$ 0.02	0/3
DS-3	glucose 10 %	7	34929080 $\pm$ 7	34929516 $\pm$ 1	2036.5 $\pm$ 0.9	2081.6 $\pm$ 2.2	116.6	119.2	-27.5 $\pm$ 0.02	0/3
DS-3	glucose 10 %	9	44906553 $\pm$ 2	44907196 $\pm$ 3	2398.9 $\pm$ 2.4	2508.4 $\pm$ 1.2	106.8	111.7	-30.4 $\pm$ 0.07	0/3

Table 2: Air-to-liquid shifts for A and P, all datasets and liquids, with the three tests. ϵ only where $\rho\eta$ is tabulated (water, isopropanol).

dataset	liquid	n	est.	Δf [Hz]	$\Delta f/n$	$\Delta\Gamma$ [Hz]	$\Delta\Gamma/n$	Δf_{KG}	ϵ_f [%]	ϵ_Γ [%]	$r = \Delta\Gamma/(-\Delta f)$	ΔD [10^{-6}]
DS-2	water	1	A	-772 ± 3	-772	872 ± 3	872	-674	+14.7	+29.4	1.129	348.4
DS-2	water	3	A	-1451 ± 52	-484	1240 ± 33	413	-1167	+24.3	+6.3	0.855	165.5
DS-2	water	5	A	-1951 ± 28	-390	1474 ± 2	295	-1506	+29.5	-2.1	0.756	118.1
DS-2	water	7	A	-2187 ± 29	-312	1664 ± 4	238	-1782	+22.7	-6.6	0.761	95.2
DS-2	water	9	A	-2415 ± 44	-268	1896 ± 1	211	-2021	+19.5	-6.2	0.785	84.4
DS-2	water	1	P	-687 ± 3	-687	869 ± 4	869	-674	+2.0	+29.0	1.265	347.3
DS-2	water	3	P	-1262 ± 18	-421	1275 ± 38	425	-1167	+8.2	+9.3	1.011	170.2
DS-2	water	5	P	-1611 ± 19	-322	1543 ± 1	309	-1506	+7.0	+2.5	0.958	123.6
DS-2	water	7	P	-1868 ± 27	-267	1724 ± 4	246	-1782	+4.8	-3.3	0.923	98.6
DS-2	water	9	P	-1991 ± 37	-221	1941 ± 10	216	-2021	-1.4	-3.9	0.975	86.4
DS-2	isopropanol	1	A	-1043 ± 3	-1043	1220 ± 1	1220	-902	+15.7	+35.3	1.169	487.7
DS-2	isopropanol	3	A	-1914 ± 8	-638	1593 ± 1	531	-1562	+22.5	+1.9	0.832	212.5
DS-2	isopropanol	5	A	-2566 ± 17	-513	1917 ± 4	383	-2017	+27.2	-5.0	0.747	153.5
DS-2	isopropanol	7	A	-2921 ± 23	-417	2224 ± 3	318	-2387	+22.4	-6.8	0.762	127.3
DS-2	isopropanol	9	A	-3327 ± 23	-370	2506 ± 3	278	-2706	+22.9	-7.4	0.753	111.5
DS-2	isopropanol	1	P	-940 ± 3	-940	1231 ± 1	1231	-902	+4.2	+36.5	1.310	492.2
DS-2	isopropanol	3	P	-1686 ± 9	-562	1643 ± 1	548	-1562	+7.9	+5.1	0.974	219.2
DS-2	isopropanol	5	P	-2072 ± 13	-414	2064 ± 13	413	-2017	+2.7	+2.3	0.996	165.3
DS-2	isopropanol	7	P	-2501 ± 21	-357	2422 ± 3	346	-2387	+4.8	+1.5	0.969	138.6
DS-2	isopropanol	9	P	-2681 ± 26	-298	2737 ± 12	304	-2706	-1.0	+1.1	1.021	121.8
DS-3	water	1	A	-729 ± 3	-729	701 ± 2	701	-673	+8.4	+4.2	0.962	280.5
DS-3	water	3	A	-1467 ± 3	-489	1118 ± 1	373	-1165	+25.9	-4.0	0.762	149.3
DS-3	water	5	A	-1808 ± 5	-362	1501 ± 1	300	-1504	+20.2	-0.2	0.830	120.3
DS-3	water	7	A	-2394 ± 4	-342	1700 ± 2	243	-1780	+34.5	-4.5	0.710	97.4
DS-3	water	9	A	-2752 ± 36	-306	1960 ± 2	218	-2018	+36.4	-2.9	0.712	87.3
DS-3	water	1	P	-723 ± 1	-723	716 ± 2	716	-673	+7.5	+6.5	0.991	286.6
DS-3	water	3	P	-1318 ± 3	-439	1145 ± 2	382	-1165	+13.1	-1.7	0.869	152.9
DS-3	water	5	P	-1596 ± 4	-319	1573 ± 1	315	-1504	+6.1	+4.6	0.986	126.1
DS-3	water	7	P	-1976 ± 6	-282	1702 ± 0	243	-1780	+11.0	-4.4	0.861	97.4
DS-3	water	9	P	-2223 ± 8	-247	1989 ± 5	221	-2018	+10.1	-1.4	0.895	88.6
DS-3	glucose 5 %	1	A	-747 ± 2	-747	727 ± 1	727	—	—	—	0.974	291.0
DS-3	glucose 5 %	3	A	-1517 ± 2	-506	1162 ± 0	387	—	—	—	0.766	155.1
DS-3	glucose 5 %	5	A	-1883 ± 3	-377	1558 ± 2	312	—	—	—	0.827	124.8
DS-3	glucose 5 %	7	A	-2489 ± 4	-356	1799 ± 1	257	—	—	—	0.723	103.0
DS-3	glucose 5 %	9	A	-2915 ± 8	-324	2099 ± 4	233	—	—	—	0.720	93.5
DS-3	glucose 5 %	1	P	-739 ± 1	-739	742 ± 1	742	—	—	—	1.004	297.0
DS-3	glucose 5 %	3	P	-1358 ± 1	-453	1189 ± 0	396	—	—	—	0.876	158.9
DS-3	glucose 5 %	5	P	-1670 ± 1	-334	1636 ± 1	327	—	—	—	0.980	131.2
DS-3	glucose 5 %	7	P	-2075 ± 2	-296	1821 ± 0	260	—	—	—	0.877	104.2
DS-3	glucose 5 %	9	P	-2351 ± 3	-261	2164 ± 1	240	—	—	—	0.921	96.4
DS-3	glucose 7.5 %	1	A	-775 ± 3	-775	759 ± 1	759	—	—	—	0.980	303.7
DS-3	glucose 7.5 %	3	A	-1581 ± 4	-527	1199 ± 0	400	—	—	—	0.759	160.2
DS-3	glucose 7.5 %	5	A	-1946 ± 5	-389	1603 ± 2	321	—	—	—	0.824	128.4
DS-3	glucose 7.5 %	7	A	-2572 ± 14	-367	1862 ± 1	266	—	—	—	0.724	106.6

Table 2: Air-to-liquid shifts for A and P, all datasets and liquids, with the three tests. ϵ only where $\rho\eta$ is tabulated (water, isopropanol).

dataset	liquid	n	est.	Δf [Hz]	$\Delta f/n$	$\Delta\Gamma$ [Hz]	$\Delta\Gamma/n$	Δf_KG	ϵ_f [%]	$\epsilon_f\Gamma$ [%]	$r = \Delta\Gamma/(-\Delta f)$	ΔD [10^{-6}]
DS-3	glucose 7.5 %	9	A	-3027 ± 5	-336	2171 ± 6	241	—	—	—	0.717	96.7
DS-3	glucose 7.5 %	1	P	-766 ± 1	-766	774 ± 1	774	—	—	—	1.011	309.7
DS-3	glucose 7.5 %	3	P	-1406 ± 1	-469	1233 ± 1	411	—	—	—	0.877	164.6
DS-3	glucose 7.5 %	5	P	-1722 ± 1	-344	1687 ± 1	337	—	—	—	0.980	135.2
DS-3	glucose 7.5 %	7	P	-2148 ± 2	-307	1901 ± 0	272	—	—	—	0.885	108.8
DS-3	glucose 7.5 %	9	P	-2435 ± 2	-271	2264 ± 1	252	—	—	—	0.930	100.8
DS-3	glucose 10 %	1	A	-802 ± 3	-802	792 ± 1	792	—	—	—	0.988	316.9
DS-3	glucose 10 %	3	A	-1654 ± 2	-551	1240 ± 1	413	—	—	—	0.749	165.6
DS-3	glucose 10 %	5	A	-2003 ± 3	-401	1649 ± 2	330	—	—	—	0.823	132.2
DS-3	glucose 10 %	7	A	-2646 ± 7	-378	1930 ± 1	276	—	—	—	0.730	110.5
DS-3	glucose 10 %	9	A	-3146 ± 3	-350	2247 ± 2	250	—	—	—	0.714	100.1
DS-3	glucose 10 %	1	P	-795 ± 1	-795	810 ± 1	810	—	—	—	1.019	324.1
DS-3	glucose 10 %	3	P	-1458 ± 1	-486	1278 ± 1	426	—	—	—	0.876	170.6
DS-3	glucose 10 %	5	P	-1775 ± 1	-355	1742 ± 1	348	—	—	—	0.981	139.6
DS-3	glucose 10 %	7	P	-2226 ± 2	-318	1983 ± 2	283	—	—	—	0.891	113.6
DS-3	glucose 10 %	9	P	-2530 ± 4	-281	2369 ± 1	263	—	—	—	0.936	105.5

Table 3: The same for the other estimators: M (magnitude maximum, Γ = half of the -3 dB width where defined), MP (midpoint of the half-height crossings), S (symmetric Lorentzian, constant background), S+ (symmetric + linear background), C (BVD admittance circle of the repository).

dataset	liquid	n	est.	Δf [Hz]	$\Delta f/n$	$\Delta \Gamma$ [Hz]	$\Delta \Gamma/n$	Δf_{KG}	ϵ_f [%]	ϵ_Γ [%]	$r = \Delta \Gamma / (-\Delta f)$	ΔD [10^{-6}]
DS-2	water	1	M	-788 ± 4	-788	779 ± 1	779	-674	+17.0	+15.6	0.988	311.2
DS-2	water	3	M	-1771 ± 10	-590	1636 ± 1	545	-1167	+51.8	+40.3	0.924	218.4
DS-2	water	5	M	-2567 ± 26	-513	6163 ± 71	1233	-1506	+70.4	+309.2	2.401	493.6
DS-2	water	7	M	-3158 ± 29	-451	—	—	-1782	+77.2	—	—	—
DS-2	water	9	M	-3879 ± 88	-431	—	—	-2021	+91.9	—	—	—
DS-2	water	1	MP	-755 ± 4	-755	872 ± 3	872	-674	+12.1	+29.4	1.155	348.4
DS-2	water	3	MP	-1577 ± 75	-526	1240 ± 33	413	-1167	+35.1	+6.3	0.787	165.5
DS-2	water	5	MP	-2220 ± 19	-444	1474 ± 2	295	-1506	+47.4	-2.1	0.664	118.1
DS-2	water	7	MP	-2516 ± 29	-359	1664 ± 4	238	-1782	+41.2	-6.6	0.661	95.2
DS-2	water	9	MP	-2907 ± 29	-323	1896 ± 1	211	-2021	+43.9	-6.2	0.652	84.4
DS-2	water	1	S	-756 ± 4	-756	869 ± 4	869	-674	+12.3	+29.0	1.149	347.3
DS-2	water	3	S	-1592 ± 86	-531	1362 ± 75	454	-1167	+36.4	+16.8	0.856	181.8
DS-2	water	5	S	-2287 ± 18	-457	1904 ± 7	381	-1506	+51.8	+26.4	0.832	152.5
DS-2	water	7	S	-2566 ± 29	-367	2090 ± 3	299	-1782	+44.0	+17.3	0.815	119.6
DS-2	water	9	S	-3019 ± 29	-335	2631 ± 20	292	-2021	+49.4	+30.2	0.872	117.1
DS-2	water	1	S+	-734 ± 4	-734	869 ± 4	869	-674	+8.9	+29.0	1.184	347.3
DS-2	water	3	S+	-1476 ± 59	-492	1273 ± 36	424	-1167	+26.5	+9.1	0.863	169.9
DS-2	water	5	S+	-2024 ± 18	-405	1545 ± 2	309	-1506	+34.4	+2.6	0.763	123.7
DS-2	water	7	S+	-2299 ± 28	-328	1729 ± 4	247	-1782	+29.0	-3.0	0.752	98.9
DS-2	water	9	S+	-2601 ± 33	-289	1985 ± 1	221	-2021	+28.7	-1.8	0.763	88.4
DS-2	water	1	C	-694 ± 3	-694	886 ± 4	886	-674	+3.1	+31.5	1.276	354.0
DS-2	water	3	C	-1609 ± 309	-536	1466 ± 280	489	-1167	+37.9	+25.7	0.911	195.7
DS-2	water	5	C	-1528 ± 19	-306	1428 ± 2	286	-1506	+1.5	-5.2	0.934	114.3
DS-2	water	7	C	-1829 ± 27	-261	1615 ± 3	231	-1782	+2.6	-9.4	0.883	92.4
DS-2	water	9	C	-2021 ± 36	-225	1827 ± 1	203	-2021	+0.0	-9.6	0.904	81.3
DS-2	isopropanol	1	M	-1072 ± 2	-1072	1083 ± 0	1083	-902	+18.8	+20.1	1.010	433.0
DS-2	isopropanol	3	M	-2448 ± 8	-816	2648 ± 13	883	-1562	+56.7	+69.5	1.082	353.5
DS-2	isopropanol	5	M	-3506 ± 14	-701	—	—	-2017	+73.8	—	—	—
DS-2	isopropanol	7	M	-4428 ± 23	-633	—	—	-2387	+85.5	—	—	—
DS-2	isopropanol	9	M	-5158 ± 23	-573	—	—	-2706	+90.6	—	—	—
DS-2	isopropanol	1	MP	-1034 ± 3	-1034	1220 ± 1	1220	-902	+14.6	+35.3	1.180	487.7
DS-2	isopropanol	3	MP	-2079 ± 8	-693	1593 ± 1	531	-1562	+33.0	+1.9	0.766	212.5
DS-2	isopropanol	5	MP	-2881 ± 15	-576	1917 ± 4	383	-2017	+42.8	-5.0	0.665	153.5
DS-2	isopropanol	7	MP	-3348 ± 22	-478	2224 ± 3	318	-2387	+40.3	-6.8	0.664	127.3
DS-2	isopropanol	9	MP	-3839 ± 24	-427	2506 ± 3	278	-2706	+41.9	-7.4	0.653	111.5
DS-2	isopropanol	1	S	-1039 ± 3	-1039	1235 ± 1	1235	-902	+15.2	+36.9	1.189	493.6
DS-2	isopropanol	3	S	-2084 ± 8	-695	1747 ± 5	582	-1562	+33.4	+11.8	0.838	233.1
DS-2	isopropanol	5	S	-2999 ± 14	-600	2557 ± 7	511	-2017	+48.7	+26.8	0.853	204.8
DS-2	isopropanol	7	S	-3379 ± 22	-483	2662 ± 5	380	-2387	+41.6	+11.5	0.788	152.3
DS-2	isopropanol	9	S	-3923 ± 31	-436	2925 ± 28	325	-2706	+45.0	+8.1	0.746	130.2
DS-2	isopropanol	1	S+	-1007 ± 3	-1007	1232 ± 1	1232	-902	+11.7	+36.6	1.223	492.5
DS-2	isopropanol	3	S+	-1946 ± 7	-649	1645 ± 1	548	-1562	+24.5	+5.3	0.845	219.5

Table 3: The same for the other estimators: M (magnitude maximum, Γ = half of the -3 dB width where defined), MP (midpoint of the half-height crossings), S (symmetric Lorentzian, constant background), S+ (symmetric + linear background), C (BVD admittance circle of the repository).

dataset	liquid	n	est.	Δf [Hz]	$\Delta f/n$	$\Delta \Gamma$ [Hz]	$\Delta \Gamma/n$	Δf_{KG}	ϵ_f [%]	ϵ_Γ [%]	$r = \Delta \Gamma / (-\Delta f)$	ΔD [10^{-6}]
DS-2	isopropanol	5	S+	-2630 ± 13	-526	2070 ± 12	414	-2017	+30.4	+2.6	0.787	165.8
DS-2	isopropanol	7	S+	-3037 ± 22	-434	2535 ± 4	362	-2387	+27.2	+6.2	0.835	145.1
DS-2	isopropanol	9	S+	-3427 ± 27	-381	3012 ± 6	335	-2706	+26.6	+11.3	0.879	134.1
DS-2	isopropanol	1	C	-941 ± 3	-941	1332 ± 5	1332	-902	+4.3	+47.7	1.416	532.4
DS-2	isopropanol	3	C	-1545 ± 11	-515	1425 ± 2	475	-1562	-1.1	-8.8	0.922	190.2
DS-2	isopropanol	5	C	-1967 ± 14	-393	1939 ± 11	388	-2017	-2.5	-3.9	0.986	155.3
DS-2	isopropanol	7	C	-2493 ± 20	-356	2183 ± 2	312	-2387	+4.4	-8.5	0.876	124.9
DS-2	isopropanol	9	C	-2765 ± 24	-307	2496 ± 2	277	-2706	+2.2	-7.8	0.903	111.1
DS-3	water	1	M	-769 ± 3	-769	733 ± 1	733	-673	+14.3	+9.0	0.954	293.3
DS-3	water	3	M	-1741 ± 3	-580	1356 ± 2	452	-1165	+49.5	+16.4	0.779	181.1
DS-3	water	5	M	-2523 ± 6	-505	6012 ± 9	1202	-1504	+67.7	+299.7	2.383	481.9
DS-3	water	7	M	-3387 ± 9	-484	—	—	-1780	+90.3	—	—	—
DS-3	water	9	M	-4354 ± 14	-484	—	—	-2018	+115.8	—	—	—
DS-3	water	1	MP	-700 ± 1	-700	701 ± 2	701	-673	+4.0	+4.2	1.002	280.5
DS-3	water	3	MP	-1698 ± 4	-566	1118 ± 1	373	-1165	+45.8	-4.0	0.658	149.3
DS-3	water	5	MP	-1961 ± 4	-392	1501 ± 1	300	-1504	+30.4	-0.2	0.766	120.3
DS-3	water	7	MP	-2825 ± 8	-404	1700 ± 2	243	-1780	+58.7	-4.5	0.602	97.4
DS-3	water	9	MP	-3300 ± 5	-367	1960 ± 2	218	-2018	+63.5	-2.9	0.594	87.3
DS-3	water	1	S	-699 ± 1	-699	713 ± 2	713	-673	+3.8	+6.0	1.021	285.3
DS-3	water	3	S	-1694 ± 4	-565	1306 ± 3	435	-1165	+45.4	+12.1	0.771	174.4
DS-3	water	5	S	-1975 ± 4	-395	1666 ± 1	333	-1504	+31.3	+10.7	0.843	133.5
DS-3	water	7	S	-2927 ± 6	-418	2392 ± 1	342	-1780	+64.5	+34.4	0.817	137.0
DS-3	water	9	S	-3492 ± 7	-388	3048 ± 9	339	-2018	+73.0	+51.0	0.873	135.8
DS-3	water	1	S+	-707 ± 1	-707	716 ± 2	716	-673	+5.2	+6.4	1.012	286.3
DS-3	water	3	S+	-1554 ± 4	-518	1138 ± 2	379	-1165	+33.4	-2.4	0.732	151.9
DS-3	water	5	S+	-1840 ± 4	-368	1569 ± 1	314	-1504	+22.4	+4.3	0.852	125.7
DS-3	water	7	S+	-2541 ± 6	-363	1730 ± 0	247	-1780	+42.8	-2.8	0.681	99.0
DS-3	water	9	S+	-2943 ± 8	-327	2070 ± 1	230	-2018	+45.8	+2.6	0.703	92.2
DS-3	water	1	C	-733 ± 1	-733	734 ± 2	734	-673	+9.0	+9.1	1.001	293.6
DS-3	water	3	C	-1284 ± 3	-428	1376 ± 3	459	-1165	+10.2	+18.1	1.072	183.8
DS-3	water	5	C	-1696 ± 5	-339	1463 ± 0	293	-1504	+12.8	-2.7	0.862	117.2
DS-3	water	7	C	-1887 ± 6	-270	1743 ± 0	249	-1780	+6.0	-2.1	0.924	99.8
DS-3	water	9	C	-2202 ± 8	-245	2022 ± 1	225	-2018	+9.1	+0.2	0.918	90.1
DS-3	glucose 5 %	1	M	-789 ± 2	-789	759 ± 1	759	—	—	—	0.962	303.7
DS-3	glucose 5 %	3	M	-1802 ± 1	-601	1430 ± 1	477	—	—	—	0.794	191.0
DS-3	glucose 5 %	5	M	-2697 ± 4	-539	—	—	—	—	—	—	—
DS-3	glucose 5 %	7	M	-3568 ± 3	-510	—	—	—	—	—	—	—
DS-3	glucose 5 %	9	M	-4579 ± 5	-509	—	—	—	—	—	—	—
DS-3	glucose 5 %	1	MP	-713 ± 1	-713	727 ± 1	727	—	—	—	1.020	291.0
DS-3	glucose 5 %	3	MP	-1767 ± 1	-589	1162 ± 0	387	—	—	—	0.657	155.1
DS-3	glucose 5 %	5	MP	-2047 ± 1	-409	1558 ± 2	312	—	—	—	0.761	124.8
DS-3	glucose 5 %	7	MP	-2954 ± 3	-422	1799 ± 1	257	—	—	—	0.609	103.0

Table 3: The same for the other estimators: M (magnitude maximum, Γ = half of the -3 dB width where defined), MP (midpoint of the half-height crossings), S (symmetric Lorentzian, constant background), S+ (symmetric + linear background), C (BVD admittance circle of the repository).

dataset	liquid	n	est.	Δf [Hz]	$\Delta f/n$	$\Delta \Gamma$ [Hz]	$\Delta \Gamma/n$	Δf_KG	ϵ_f [%]	$\epsilon_ \Gamma$ [%]	$r = \Delta \Gamma / (-\Delta f)$	ΔD [10^{-6}]
DS-3	glucose 5 %	9	MP	-3462 ± 5	-385	2099 ± 4	233	—	—	—	0.606	93.5
DS-3	glucose 5 %	1	S	-713 ± 1	-713	739 ± 1	739	—	—	—	1.038	295.7
DS-3	glucose 5 %	3	S	-1764 ± 1	-588	1371 ± 1	457	—	—	—	0.777	183.1
DS-3	glucose 5 %	5	S	-2064 ± 1	-413	1736 ± 1	347	—	—	—	0.841	139.1
DS-3	glucose 5 %	7	S	-3059 ± 2	-437	2529 ± 1	361	—	—	—	0.827	144.8
DS-3	glucose 5 %	9	S	-3652 ± 3	-406	3112 ± 9	346	—	—	—	0.852	138.6
DS-3	glucose 5 %	1	S+	-722 ± 1	-722	742 ± 1	742	—	—	—	1.027	296.7
DS-3	glucose 5 %	3	S+	-1612 ± 1	-537	1181 ± 0	394	—	—	—	0.733	157.8
DS-3	glucose 5 %	5	S+	-1924 ± 1	-385	1632 ± 0	326	—	—	—	0.848	130.8
DS-3	glucose 5 %	7	S+	-2660 ± 2	-380	1845 ± 1	264	—	—	—	0.693	105.6
DS-3	glucose 5 %	9	S+	-3093 ± 2	-344	2296 ± 2	255	—	—	—	0.742	102.3
DS-3	glucose 5 %	1	C	-751 ± 1	-751	762 ± 0	762	—	—	—	1.015	304.8
DS-3	glucose 5 %	3	C	-1325 ± 1	-442	1448 ± 1	483	—	—	—	1.093	193.4
DS-3	glucose 5 %	5	C	-1771 ± 1	-354	1529 ± 1	306	—	—	—	0.863	122.5
DS-3	glucose 5 %	7	C	-1976 ± 2	-282	1853 ± 1	265	—	—	—	0.938	106.1
DS-3	glucose 5 %	9	C	-2301 ± 2	-256	2182 ± 1	242	—	—	—	0.948	97.2
DS-3	glucose 7.5 %	1	M	-818 ± 6	-818	791 ± 1	791	—	—	—	0.966	316.3
DS-3	glucose 7.5 %	3	M	-1868 ± 1	-623	1506 ± 1	502	—	—	—	0.806	201.1
DS-3	glucose 7.5 %	5	M	-2821 ± 3	-564	—	—	—	—	—	—	—
DS-3	glucose 7.5 %	7	M	-3701 ± 3	-529	—	—	—	—	—	—	—
DS-3	glucose 7.5 %	9	M	-4720 ± 4	-524	—	—	—	—	—	—	—
DS-3	glucose 7.5 %	1	MP	-737 ± 1	-737	759 ± 1	759	—	—	—	1.030	303.7
DS-3	glucose 7.5 %	3	MP	-1841 ± 1	-614	1199 ± 0	400	—	—	—	0.651	160.2
DS-3	glucose 7.5 %	5	MP	-2113 ± 1	-423	1603 ± 2	321	—	—	—	0.758	128.4
DS-3	glucose 7.5 %	7	MP	-3049 ± 2	-436	1862 ± 1	266	—	—	—	0.611	106.6
DS-3	glucose 7.5 %	9	MP	-3568 ± 5	-396	2171 ± 6	241	—	—	—	0.608	96.7
DS-3	glucose 7.5 %	1	S	-736 ± 1	-736	771 ± 1	771	—	—	—	1.048	308.4
DS-3	glucose 7.5 %	3	S	-1845 ± 1	-615	1438 ± 1	479	—	—	—	0.779	192.0
DS-3	glucose 7.5 %	5	S	-2132 ± 1	-426	1793 ± 2	359	—	—	—	0.841	143.7
DS-3	glucose 7.5 %	7	S	-3159 ± 2	-451	2627 ± 5	375	—	—	—	0.832	150.4
DS-3	glucose 7.5 %	9	S	-3756 ± 3	-417	3132 ± 14	348	—	—	—	0.834	139.5
DS-3	glucose 7.5 %	1	S+	-747 ± 1	-747	773 ± 1	773	—	—	—	1.036	309.3
DS-3	glucose 7.5 %	3	S+	-1679 ± 1	-560	1225 ± 1	408	—	—	—	0.729	163.6
DS-3	glucose 7.5 %	5	S+	-1986 ± 1	-397	1684 ± 0	337	—	—	—	0.848	135.0
DS-3	glucose 7.5 %	7	S+	-2749 ± 2	-393	1925 ± 2	275	—	—	—	0.700	110.2
DS-3	glucose 7.5 %	9	S+	-3191 ± 2	-355	2422 ± 2	269	—	—	—	0.759	107.9
DS-3	glucose 7.5 %	1	C	-779 ± 1	-779	795 ± 1	795	—	—	—	1.021	318.2
DS-3	glucose 7.5 %	3	C	-1373 ± 1	-458	1517 ± 1	506	—	—	—	1.105	202.6
DS-3	glucose 7.5 %	5	C	-1825 ± 1	-365	1580 ± 0	316	—	—	—	0.866	126.7
DS-3	glucose 7.5 %	7	C	-2041 ± 2	-292	1925 ± 1	275	—	—	—	0.943	110.2
DS-3	glucose 7.5 %	9	C	-2373 ± 2	-264	2276 ± 1	253	—	—	—	0.959	101.4
DS-3	glucose 10 %	1	M	-839 ± 8	-839	822 ± 0	822	—	—	—	0.981	329.0

Table 3: The same for the other estimators: M (magnitude maximum, Γ = half of the -3 dB width where defined), MP (midpoint of the half-height crossings), S (symmetric Lorentzian, constant background), S+ (symmetric + linear background), C (BVD admittance circle of the repository).

dataset	liquid	n	est.	Δf [Hz]	$\Delta f/n$	$\Delta \Gamma$ [Hz]	$\Delta \Gamma/n$	Δf_KG	ϵ_f [%]	ϵ_f [%]	$r = \Delta \Gamma / (-\Delta f)$	ΔD [10^{-6}]
DS-3	glucose 10 %	3	M	-1937 ± 1	-646	1586 ± 2	529	—	—	—	0.819	211.8
DS-3	glucose 10 %	5	M	-2929 ± 2	-586	—	—	—	—	—	—	—
DS-3	glucose 10 %	7	M	-3828 ± 5	-547	—	—	—	—	—	—	—
DS-3	glucose 10 %	9	M	-4875 ± 4	-542	—	—	—	—	—	—	—
DS-3	glucose 10 %	1	MP	-765 ± 1	-765	792 ± 1	792	—	—	—	1.036	316.9
DS-3	glucose 10 %	3	MP	-1921 ± 1	-640	1240 ± 1	413	—	—	—	0.645	165.6
DS-3	glucose 10 %	5	MP	-2179 ± 1	-436	1649 ± 2	330	—	—	—	0.757	132.2
DS-3	glucose 10 %	7	MP	-3148 ± 3	-450	1930 ± 1	276	—	—	—	0.613	110.5
DS-3	glucose 10 %	9	MP	-3688 ± 3	-410	2247 ± 2	250	—	—	—	0.609	100.1
DS-3	glucose 10 %	1	S	-762 ± 0	-762	807 ± 1	807	—	—	—	1.059	323.0
DS-3	glucose 10 %	3	S	-1932 ± 1	-644	1507 ± 2	502	—	—	—	0.780	201.2
DS-3	glucose 10 %	5	S	-2202 ± 1	-440	1854 ± 2	371	—	—	—	0.842	148.6
DS-3	glucose 10 %	7	S	-3263 ± 2	-466	2710 ± 4	387	—	—	—	0.831	155.2
DS-3	glucose 10 %	9	S	-3872 ± 4	-430	3148 ± 8	350	—	—	—	0.813	140.2
DS-3	glucose 10 %	1	S+	-774 ± 0	-774	809 ± 1	809	—	—	—	1.046	323.8
DS-3	glucose 10 %	3	S+	-1751 ± 1	-584	1270 ± 1	423	—	—	—	0.726	169.7
DS-3	glucose 10 %	5	S+	-2050 ± 1	-410	1738 ± 1	348	—	—	—	0.848	139.3
DS-3	glucose 10 %	7	S+	-2840 ± 2	-406	2017 ± 2	288	—	—	—	0.710	115.5
DS-3	glucose 10 %	9	S+	-3301 ± 3	-367	2561 ± 1	285	—	—	—	0.776	114.0
DS-3	glucose 10 %	1	C	-810 ± 1	-810	832 ± 1	832	—	—	—	1.028	333.0
DS-3	glucose 10 %	3	C	-1423 ± 1	-474	1589 ± 1	530	—	—	—	1.117	212.2
DS-3	glucose 10 %	5	C	-1879 ± 1	-376	1635 ± 1	327	—	—	—	0.870	131.0
DS-3	glucose 10 %	7	C	-2110 ± 2	-301	1998 ± 1	285	—	—	—	0.947	114.4
DS-3	glucose 10 %	9	C	-2460 ± 3	-273	2368 ± 1	263	—	—	—	0.963	105.5

Table 4: Summary on overtones 3–9 (range over n ; over water and isopropanol for ϵ ; over all liquids for r_n), every estimator and dataset.

dataset	estimator	ϵ_f [%]		ϵ_Γ [%]		r_n (water)		r_n (all liquids)		max	ϵ_f [%]
DS-2	M	+51.8 ...	+91.9	+40.3 ...	+309.2	0.92 ...	2.40	0.92 ...	2.40	91.9	
DS-2	A	+19.5 ...	+29.5	-7.4 ...	+6.3	0.76 ...	0.85	0.75 ...	0.85	29.5	
DS-2	MP	+33.0 ...	+47.4	-7.4 ...	+6.3	0.65 ...	0.79	0.65 ...	0.79	47.4	
DS-2	S	+33.4 ...	+51.8	+8.1 ...	+30.2	0.81 ...	0.87	0.75 ...	0.87	51.8	
DS-2	S+	+24.5 ...	+34.4	-3.0 ...	+11.3	0.75 ...	0.86	0.75 ...	0.88	34.4	
DS-2	C	-2.5 ...	+37.9	-9.6 ...	+25.7	0.88 ...	0.93	0.88 ...	0.99	37.9	
DS-2	P	-1.4 ...	+8.2	-3.9 ...	+9.3	0.92 ...	1.01	0.92 ...	1.02	8.2	
DS-3	M	+49.5 ...	+115.8	+16.4 ...	+299.7	0.78 ...	2.38	0.78 ...	2.38	115.8	
DS-3	A	+20.2 ...	+36.4	-4.5 ...	-0.2	0.71 ...	0.83	0.71 ...	0.83	36.4	
DS-3	MP	+30.4 ...	+63.5	-4.5 ...	-0.2	0.59 ...	0.77	0.59 ...	0.77	63.5	
DS-3	S	+31.3 ...	+73.0	+10.7 ...	+51.0	0.77 ...	0.87	0.77 ...	0.87	73.0	
DS-3	S+	+22.4 ...	+45.8	-2.8 ...	+4.3	0.68 ...	0.85	0.68 ...	0.85	45.8	
DS-3	C	+6.0 ...	+12.8	-2.7 ...	+18.1	0.86 ...	1.07	0.86 ...	1.12	12.8	
DS-3	P	+6.1 ...	+13.1	-4.4 ...	+4.6	0.86 ...	0.99	0.86 ...	0.99	13.1	

Table 5: KG-2: log-log slopes, $\sqrt{n}$ slopes through the origin and coefficients of variation of the $\sqrt{n}$ -normalised shifts, A and P, fits on $n = 1-9$ and $3-9$.

dataset	liquid	est.	fit	$b(\Delta f)$	$b(\Delta \Gamma)$	$k(-\Delta f)$ [Hz/ $\sqrt{n}$]	$k(\Delta \Gamma)$	k_KG	$CV(-\Delta f/\sqrt{n})$ [%]	$CV(\Delta \Gamma/\sqrt{n})$ [%]
DS-2	isopropanol	A	n=1-9	-0.470	-0.677	1112	867	902	3.4	17.5
DS-2	isopropanol	A	n=3-9	-0.503	-0.589	1115	852	902	1.9	4.5
DS-2	isopropanol	P	n=1-9	-0.517	-0.638	926	932	902	3.1	14.0
DS-2	isopropanol	P	n=3-9	-0.564	-0.536	925	920	902	3.6	1.8
DS-2	water	A	n=1-9	-0.473	-0.654	827	656	674	4.5	14.4
DS-2	water	A	n=3-9	-0.539	-0.621	829	647	674	3.4	6.1
DS-2	water	P	n=1-9	-0.506	-0.639	696	677	674	3.7	12.7
DS-2	water	P	n=3-9	-0.576	-0.625	696	669	674	4.1	6.1
DS-3	glucose 5 %	A	n=1-9	-0.389	-0.520	917	691	—	10.1	3.1
DS-3	glucose 5 %	A	n=3-9	-0.395	-0.471	924	690	—	6.5	2.0
DS-3	glucose 5 %	P	n=1-9	-0.477	-0.516	775	711	—	2.9	3.6
DS-3	glucose 5 %	P	n=3-9	-0.493	-0.474	776	710	—	2.4	3.3
DS-3	glucose 7.5 %	A	n=1-9	-0.390	-0.524	950	714	—	10.1	3.5
DS-3	glucose 7.5 %	A	n=3-9	-0.400	-0.468	957	713	—	6.5	1.9
DS-3	glucose 7.5 %	P	n=1-9	-0.478	-0.516	802	740	—	3.0	3.6
DS-3	glucose 7.5 %	P	n=3-9	-0.492	-0.464	803	739	—	2.6	3.1
DS-3	glucose 10 %	A	n=1-9	-0.392	-0.528	983	739	—	10.2	3.9
DS-3	glucose 10 %	A	n=3-9	-0.408	-0.466	991	737	—	6.7	1.9
DS-3	glucose 10 %	P	n=1-9	-0.478	-0.517	831	771	—	3.2	3.8
DS-3	glucose 10 %	P	n=3-9	-0.490	-0.454	832	769	—	2.9	3.2
DS-3	water	A	n=1-9	-0.401	-0.532	876	655	673	9.1	3.6
DS-3	water	A	n=3-9	-0.413	-0.499	882	653	673	5.8	2.0
DS-3	water	P	n=1-9	-0.493	-0.536	739	668	673	2.5	4.6
DS-3	water	P	n=3-9	-0.515	-0.517	740	666	673	2.6	3.8

Table 6: Experiment 1 reproducibility: the air $\rightarrow$ water step of DS-2 and DS-3 (A and P) and the live A estimator of board 1920 on two days.

n	$\Delta f/n$	A	DS-2	DS-3	$\Delta f/n$	P	DS-2	DS-3	$\Delta \Gamma/n$	A	DS-2	DS-3	$\Delta \Gamma/n$	P	DS-2	DS-3	ϵ_f	P	DS-2 [%]	DS-3	ϵ_{Γ}	P	DS-2 [%]	DS-3	r	P	DS-2	DS-3	φ_{water}	DS-2 [°]	DS-3	ϵ_f	A live 09-11 [%]	09-10
1	-772			-729	-687			-723	872		701	869		716	+2.0		+7.5	+29.0		+6.5	1.26	0.99	-5.0		0.7	+14.2						+12.1		
3	-484			-489	-421			-439	413		373	425		382	+8.2		+13.1	+9.3		-1.7	1.01	0.87	-15.0		-18.8	+23.1						+30.4		
5	-390			-362	-322			-319	295		300	309		315	+7.0		+6.1	+2.5		+4.6	0.96	0.99	-24.0		-14.4	+29.3						+30.2		
7	-312			-342	-267			-282	238		243	246		243	+4.8		+11.0	-3.3		-4.4	0.92	0.86	-22.5		-28.7	+21.7						+25.1		
9	-268			-306	-221			-247	211		218	216		221	-1.4		+10.1	-3.9		-1.4	0.97	0.90	-27.9		-31.9	+17.5						+26.1		

Table 7: The '8 %' claim per overtone: P and A against KG.

dataset	liquid	n	$\epsilon_{\text{f P}}$ [%]	$\epsilon_{\text{f P}}$ [%]	$\epsilon_{\text{f A}}$ [%]	$\epsilon_{\text{f A}}$ [%]	P within 8 % (f / Γ)	A within 8 % (f / Γ)
DS-2	water	1	+2.0	+29.0	+14.7	+29.4	yes / no	no / no
DS-2	water	3	+8.2	+9.3	+24.3	+6.3	no / no	no / yes
DS-2	water	5	+7.0	+2.5	+29.5	-2.1	yes / yes	no / yes
DS-2	water	7	+4.8	-3.3	+22.7	-6.6	yes / yes	no / yes
DS-2	water	9	-1.4	-3.9	+19.5	-6.2	yes / yes	no / yes
DS-2	isopropanol	1	+4.2	+36.5	+15.7	+35.3	yes / no	no / no
DS-2	isopropanol	3	+7.9	+5.1	+22.5	+1.9	yes / yes	no / yes
DS-2	isopropanol	5	+2.7	+2.3	+27.2	-5.0	yes / yes	no / yes
DS-2	isopropanol	7	+4.8	+1.5	+22.4	-6.8	yes / yes	no / yes
DS-2	isopropanol	9	-1.0	+1.1	+22.9	-7.4	yes / yes	no / yes
DS-3	water	1	+7.5	+6.5	+8.4	+4.2	yes / yes	no / yes
DS-3	water	3	+13.1	-1.7	+25.9	-4.0	no / yes	no / yes
DS-3	water	5	+6.1	+4.6	+20.2	-0.2	yes / yes	no / yes
DS-3	water	7	+11.0	-4.4	+34.5	-4.5	no / yes	no / yes
DS-3	water	9	+10.1	-1.4	+36.4	-2.9	no / yes	no / yes

Table 8: Bias of the conductance maximum and of the half-height width per dataset, medium and overtone (mean of three sweeps).

dataset	medium	n	Γ_P [Hz]	φ [°]	$f_Gmax - f_res$ [Hz]	$\Gamma \tan(\varphi/2)$ [Hz]	meas - pred [Hz]	(meas - pred)/ Γ	Γ_hh/Γ_P	$\sqrt{(1+2\tan^2(\varphi/2))}$
DS-2	air	1	66	-8.0	$+3 \pm 1$	-5	+7	+0.110	0.997	1.005
DS-2	air	3	76	-14.5	-2 ± 0	-10	+8	+0.103	1.026	1.016
DS-2	air	5	102	-20.6	-11 ± 0	-19	+7	+0.073	1.054	1.033
DS-2	air	7	148	-22.9	-28 ± 2	-30	+2	+0.014	1.075	1.040
DS-2	air	9	189	-26.8	-47 ± 1	-45	-2	-0.009	1.080	1.055
DS-2	isopropanol	1	1297	-5.0	-101 ± 0	-56	-44	-0.034	0.991	1.002
DS-2	isopropanol	3	1719	-14.2	-230 ± 2	-215	-15	-0.009	0.972	1.015
DS-2	isopropanol	5	2167	-24.7	-505 ± 10	-475	-31	-0.014	0.935	1.047
DS-2	isopropanol	7	2570	-21.4	-448 ± 5	-486	+38	+0.015	0.927	1.035
DS-2	isopropanol	9	2925	-27.2	-693 ± 12	-708	+16	+0.005	0.926	1.057
DS-2	water	1	934	-5.0	-83 ± 2	-41	-42	-0.045	1.003	1.002
DS-2	water	3	1351	-15.0	-191 ± 37	-179	-12	-0.009	0.976	1.018
DS-2	water	5	1646	-24.0	-351 ± 14	-349	-2	-0.001	0.961	1.044
DS-2	water	7	1872	-22.5	-347 ± 2	-372	+25	+0.014	0.974	1.039
DS-2	water	9	2130	-27.9	-470 ± 15	-529	+59	+0.028	0.986	1.060
DS-3	air	1	115	-7.3	-0 ± 0	-7	+7	+0.062	0.959	1.004
DS-3	air	3	51	-19.7	-5 ± 0	-9	+4	+0.085	1.027	1.030
DS-3	air	5	67	-19.5	-6 ± 0	-12	+5	+0.077	1.046	1.029
DS-3	air	7	98	-25.3	-16 ± 0	-22	+6	+0.064	1.080	1.049
DS-3	air	9	140	-27.9	-27 ± 1	-35	+8	+0.055	1.090	1.060
DS-3	glucose 5 %	1	857	0.9	-8 ± 2	+7	-14	-0.017	0.977	1.000
DS-3	glucose 5 %	3	1241	-19.5	-164 ± 2	-213	+49	+0.039	0.979	1.029
DS-3	glucose 5 %	5	1703	-14.4	-219 ± 2	-215	-4	-0.002	0.956	1.016
DS-3	glucose 5 %	7	1919	-28.1	-430 ± 3	-480	+50	+0.026	0.993	1.061
DS-3	glucose 5 %	9	2304	-31.0	-591 ± 7	-639	+48	+0.021	0.977	1.074
DS-3	glucose 7.5 %	1	889	1.1	-9 ± 3	+8	-17	-0.019	0.978	1.000
DS-3	glucose 7.5 %	3	1284	-20.2	-180 ± 3	-228	+48	+0.038	0.975	1.031
DS-3	glucose 7.5 %	5	1754	-14.5	-230 ± 4	-224	-7	-0.004	0.953	1.016
DS-3	glucose 7.5 %	7	1999	-27.8	-440 ± 13	-494	+55	+0.027	0.985	1.059
DS-3	glucose 7.5 %	9	2404	-30.7	-619 ± 3	-660	+40	+0.017	0.966	1.073
DS-3	glucose 10 %	1	925	1.2	-7 ± 3	+10	-17	-0.018	0.975	1.000
DS-3	glucose 10 %	3	1329	-20.8	-201 ± 2	-244	+43	+0.033	0.973	1.033
DS-3	glucose 10 %	5	1808	-14.6	-234 ± 2	-232	-2	-0.001	0.951	1.016
DS-3	glucose 10 %	7	2082	-27.5	-436 ± 6	-509	+74	+0.036	0.978	1.058
DS-3	glucose 10 %	9	2508	-30.4	-643 ± 2	-682	+39	+0.015	0.956	1.071
DS-3	water	1	831	0.7	-6 ± 1	+5	-12	-0.014	0.976	1.000
DS-3	water	3	1196	-18.8	-154 ± 1	-198	+44	+0.037	0.979	1.027
DS-3	water	5	1640	-14.4	-218 ± 1	-208	-11	-0.006	0.958	1.016
DS-3	water	7	1800	-28.7	-434 ± 2	-461	+27	+0.015	1.004	1.064
DS-3	water	9	2129	-31.9	-556 ± 29	-609	+53	+0.025	0.992	1.079

(a) every dataset and medium

Table 9: The rotation angle: every dataset and medium; stability per overtone; between boards and days; monotonicity.

dataset	medium	n	f [MHz]	φ [°]	sd	min	max	sweeps
DS-2	air	1	5.005	-8.0	0.05	-8.0	-7.9	3
DS-2	air	3	14.989	-14.5	0.03	-14.5	-14.5	3
DS-2	air	5	24.974	-20.6	0.06	-20.7	-20.5	3
DS-2	air	7	34.958	-22.9	0.04	-22.9	-22.8	3
DS-2	air	9	44.943	-26.8	0.00	-26.8	-26.8	3
DS-2	isopropanol	1	5.004	-5.0	0.02	-5.0	-5.0	3
DS-2	isopropanol	3	14.987	-14.2	0.18	-14.4	-14.0	3
DS-2	isopropanol	5	24.972	-24.7	0.17	-24.9	-24.6	3
DS-2	isopropanol	7	34.955	-21.4	0.11	-21.5	-21.3	3
DS-2	isopropanol	9	44.940	-27.2	0.04	-27.3	-27.2	3
DS-2	water	1	5.004	-5.0	0.02	-5.1	-5.0	3
DS-2	water	3	14.987	-15.0	2.45	-17.9	-13.6	3
DS-2	water	5	24.972	-24.0	0.04	-24.0	-23.9	3
DS-2	water	7	34.956	-22.5	0.05	-22.5	-22.5	3
DS-2	water	9	44.941	-27.9	0.23	-28.1	-27.7	3
DS-3	air	1	5.000	-7.3	0.13	-7.4	-7.2	3
DS-3	air	3	14.977	-19.7	0.02	-19.7	-19.7	3
DS-3	air	5	24.955	-19.5	0.02	-19.5	-19.5	3
DS-3	air	7	34.932	-25.3	0.05	-25.4	-25.3	3
DS-3	air	9	44.910	-27.9	0.05	-28.0	-27.9	3
DS-3	glucose 5 %	1	4.999	0.9	0.01	0.9	0.9	3
DS-3	glucose 5 %	3	14.976	-19.5	0.01	-19.5	-19.5	3
DS-3	glucose 5 %	5	24.954	-14.4	0.00	-14.4	-14.4	3
DS-3	glucose 5 %	7	34.930	-28.1	0.01	-28.1	-28.1	3
DS-3	glucose 5 %	9	44.907	-31.0	0.04	-31.0	-31.0	3
DS-3	glucose 7.5 %	1	4.999	1.1	0.01	1.1	1.1	3
DS-3	glucose 7.5 %	3	14.976	-20.2	0.01	-20.2	-20.1	3
DS-3	glucose 7.5 %	5	24.954	-14.5	0.01	-14.5	-14.5	3
DS-3	glucose 7.5 %	7	34.930	-27.8	0.00	-27.8	-27.8	3
DS-3	glucose 7.5 %	9	44.907	-30.7	0.02	-30.7	-30.7	3
DS-3	glucose 10 %	1	4.999	1.2	0.01	1.2	1.2	3
DS-3	glucose 10 %	3	14.976	-20.8	0.03	-20.9	-20.8	3
DS-3	glucose 10 %	5	24.953	-14.6	0.02	-14.6	-14.6	3
DS-3	glucose 10 %	7	34.930	-27.5	0.02	-27.5	-27.5	3
DS-3	glucose 10 %	9	44.907	-30.4	0.07	-30.5	-30.4	3
DS-3	water	1	4.999	0.7	0.03	0.7	0.8	3
DS-3	water	3	14.976	-18.8	0.03	-18.9	-18.8	3
DS-3	water	5	24.954	-14.4	0.02	-14.5	-14.4	3
DS-3	water	7	34.930	-28.7	0.01	-28.7	-28.7	3
DS-3	water	9	44.908	-31.9	0.03	-32.0	-31.9	3
air 2026-09-03 (board 1920 class)	air	1	4.999	-7.8	—	-7.8	-7.8	1
air 2026-09-03 (board 1920 class)	air	3	14.974	-17.5	—	-17.5	-17.5	1
air 2026-09-03 (board 1920 class)	air	5	24.951	-22.6	—	-22.6	-22.6	1
air 2026-09-03 (board 1920 class)	air	7	34.926	-25.7	—	-25.7	-25.7	1

Table 9: The rotation angle: every dataset and medium; stability per overtone; between boards and days; monotonicity.

dataset	medium	n	f [MHz]	φ [°]	sd	min	max	sweeps
air 2026-09-03 (board 1920 class)	air	9	44.903	-28.9	—	-28.9	-28.9	1
water 2026-07-28 (board not recorded)	water	1	4.998	2.2	—	2.2	2.2	1

(b) stability per overtone

dataset	n	φ air	φ liquids	(min ... max)	range over liquids	air – mean(liquids)	range over all media	max replica sd
DS-2	1	-8.0	-5.0	... -5.0	0.1	-3.0	3.0	0.05
DS-2	3	-14.5	-15.0	... -14.2	0.8	+0.2	0.8	2.45
DS-2	5	-20.6	-24.7	... -24.0	0.8	+3.7	4.1	0.17
DS-2	7	-22.9	-22.5	... -21.4	1.1	-0.9	1.5	0.11
DS-2	9	-26.8	-27.9	... -27.2	0.7	+0.7	1.1	0.23
DS-3	1	-7.3	0.7	... 1.2	0.5	-8.3	8.5	0.13
DS-3	3	-19.7	-20.8	... -18.8	2.0	+0.1	2.0	0.03
DS-3	5	-19.5	-14.6	... -14.4	0.2	-5.0	5.1	0.02
DS-3	7	-25.3	-28.7	... -27.5	1.2	+2.7	3.4	0.05
DS-3	9	-27.9	-31.9	... -30.4	1.5	+3.1	4.0	0.07

(c) between boards and days, air

n	φ air DS-2 (board 1920, 09-11)	air 2026-09-03	φ air DS-3 (2024)	09-03 – DS-2	DS-3 – DS-2
1	-8.0	-7.8	-7.3	+0.2	+0.7
3	-14.5	-17.5	-19.7	-3.0	-5.2
5	-20.6	-22.6	-19.5	-2.0	+1.1
7	-22.9	-25.7	-25.3	-2.8	-2.4
9	-26.8	-28.9	-27.9	-2.0	-1.1

(d) monotonicity

dataset	medium	$\varphi(n = 1 \dots 9)$ [°]	monotonic in n	largest step in the wrong direction [°]
DS-2	air	-8.0 / -14.5 / -20.6 / -22.9 / -26.8	yes	0.0
DS-2	isopropanol	-5.0 / -14.2 / -24.7 / -21.4 / -27.2	no	3.3
DS-2	water	-5.0 / -15.0 / -24.0 / -22.5 / -27.9	no	1.4
DS-3	air	-7.3 / -19.7 / -19.5 / -25.3 / -27.9	no	0.2
DS-3	glucose 5 %	0.9 / -19.5 / -14.4 / -28.1 / -31.0	no	5.0
DS-3	glucose 7.5 %	1.1 / -20.2 / -14.5 / -27.8 / -30.7	no	5.6
DS-3	glucose 10 %	1.2 / -20.8 / -14.6 / -27.5 / -30.4	no	6.2
DS-3	water	0.7 / -18.8 / -14.4 / -28.7 / -31.9	no	4.4
air 2026-09-03 (board 1920 class)	air	-7.8 / -17.5 / -22.6 / -25.7 / -28.9	yes	0.0

(a) relative $\sqrt{(\rho\eta)}$ from the data, $x = \sqrt{(\rho\eta)}/\sqrt{(\rho\eta)}_{\text{water}}$

Table 11: Glucose: data-derived relative $\sqrt{\rho\eta}$, its dependence on concentration, steps between concentrations in units of the replica scatter, and the resolution.

est. liquid	% w/v	x from Δf , $n = 1 \dots 9$	mean $3-9 \pm \text{sd_n}$ x from $\Delta \Gamma$	mean $\pm \text{sd_n}$ x from both	mean $\pm \text{sd_n}$
A water	0.0	1.000 / 1.000 / 1.000 / 1.000 / 1.000	1.000 $\pm$ 0.000	1.000 / 1.000 / 1.000 / 1.000 / 1.000	1.000 $\pm$ 0.000
A glucose 5 %	5.0	1.025 / 1.034 / 1.041 / 1.040 / 1.059	1.044 $\pm$ 0.011	1.038 / 1.039 / 1.037 / 1.058 / 1.071	1.051 $\pm$ 0.016
A glucose 7.5 %	7.5	1.063 / 1.078 / 1.076 / 1.074 / 1.100	1.082 $\pm$ 0.012	1.083 / 1.073 / 1.067 / 1.095 / 1.108	1.086 $\pm$ 0.019
A glucose 10 %	10.0	1.100 / 1.127 / 1.108 / 1.105 / 1.143	1.121 $\pm$ 0.018	1.130 / 1.109 / 1.099 / 1.135 / 1.146	1.122 $\pm$ 0.022
P water	0.0	1.000 / 1.000 / 1.000 / 1.000 / 1.000	1.000 $\pm$ 0.000	1.000 / 1.000 / 1.000 / 1.000 / 1.000	1.000 $\pm$ 0.000
P glucose 5 %	5.0	1.023 / 1.030 / 1.046 / 1.050 / 1.058	1.046 $\pm$ 0.011	1.036 / 1.039 / 1.040 / 1.070 / 1.088	1.059 $\pm$ 0.024
P glucose 7.5 %	7.5	1.060 / 1.067 / 1.079 / 1.087 / 1.096	1.082 $\pm$ 0.012	1.081 / 1.076 / 1.072 / 1.117 / 1.138	1.101 $\pm$ 0.032
P glucose 10 %	10.0	1.100 / 1.106 / 1.112 / 1.126 / 1.138	1.121 $\pm$ 0.014	1.131 / 1.116 / 1.107 / 1.165 / 1.191	1.145 $\pm$ 0.040

(b) x against concentration (least squares with intercept on 0, 5, 7.5, 10 % w/v)

est.	x_rel	slope [per % w/v]	intercept	residual of the 5 % point	rms
A	from Δf , n = 3-9	0.01198	0.9942	-0.0106	0.0070
A	from $\Delta \Gamma$, n = 3-9	0.01214	0.9966	-0.0059	0.0041
A	from both, n = 3-9	0.01203	0.9952	-0.0086	0.0058
P	from Δf , n = 3-9	0.01194	0.9950	-0.0087	0.0061
P	from $\Delta \Gamma$, n = 3-9	0.01436	0.9954	-0.0081	0.0056
P	from both, n = 3-9	0.01307	0.9952	-0.0084	0.0058

(c) steps and resolution; σ_x = replica sd / slope, slope = the water shift of the same overtone

est.	n	sd f [Hz]	sd Γ [Hz]	slope f [Hz per x]	slope Γ	σ_{x} from f	σ_{x} from Γ	water→5 %: $\Delta\text{x_f}$ (σ)	$\Delta\text{x_}\Gamma$ (σ)	5→7.5 %: $\Delta\text{x_f}$ (σ)	$\Delta\text{x_}\Gamma$ (σ)	7.5→10 %: $\Delta\text{x_f}$ (σ)	$\Delta\text{x_}\Gamma$ (σ)
A	1	2.7	0.6	729	701	0.0037	0.0008	0.025 (6)	0.038 (18)	0.038 (8)	0.045 (63)	0.037 (7)	0.047 (47)
A	3	2.3	0.6	1467	1118	0.0016	0.0005	0.034 (15)	0.039 (32)	0.044 (16)	0.034 (106)	0.050 (18)	0.036 (44)
A	5	3.6	1.7	1808	1501	0.0020	0.0011	0.041 (13)	0.037 (21)	0.035 (12)	0.030 (15)	0.032 (11)	0.031 (19)
A	7	5.3	1.0	2394	1700	0.0022	0.0006	0.040 (20)	0.058 (41)	0.035 (6)	0.037 (47)	0.031 (5)	0.040 (48)
A	9	5.2	3.2	2752	1960	0.0019	0.0016	0.059 (4)	0.071 (30)	0.041 (14)	0.036 (10)	0.043 (31)	0.039 (12)
P	1	0.3	0.9	723	716	0.0004	0.0012	0.023 (14)	0.036 (15)	0.037 (58)	0.044 (26)	0.040 (79)	0.051 (29)
P	3	0.5	0.7	1318	1145	0.0004	0.0006	0.030 (14)	0.039 (23)	0.037 (65)	0.038 (77)	0.039 (66)	0.039 (46)
P	5	0.9	0.7	1596	1573	0.0006	0.0004	0.046 (17)	0.040 (81)	0.032 (59)	0.032 (52)	0.033 (41)	0.034 (46)
P	7	0.8	0.2	1976	1702	0.0004	0.0001	0.050 (19)	0.070 (427)	0.037 (67)	0.047 (232)	0.040 (70)	0.048 (38)
P	9	1.7	1.3	2223	1989	0.0008	0.0006	0.058 (17)	0.088 (38)	0.038 (105)	0.050 (64)	0.043 (34)	0.053 (58)

Table 13: Live datalogs of board 1920 (A as published by the instrument):
plateau shifts against KG.

run	liquid	n	Δf [Hz]	ϵ_f [%]	$\Delta\Gamma$ [Hz]	ϵ_Γ [%]	r_n
DS-2 datalog 2026-09-11	water	1	-769 ± 2	+14.2	870 ± 1	+29.2	1.13
DS-2 datalog 2026-09-11	water	3	-1436 ± 48	+23.1	1239 ± 27	+6.2	0.86
DS-2 datalog 2026-09-11	water	5	-1948 ± 5	+29.3	1473 ± 1	-2.2	0.76
DS-2 datalog 2026-09-11	water	7	-2169 ± 6	+21.7	1663 ± 2	-6.7	0.77
DS-2 datalog 2026-09-11	water	9	-2373 ± 17	+17.5	1898 ± 2	-6.1	0.80
DS-2 datalog 2026-09-11	isopropanol	1	-1042 ± 1	+15.5	1220 ± 0	+35.2	1.17
DS-2 datalog 2026-09-11	isopropanol	3	-1904 ± 7	+21.9	1592 ± 1	+1.9	0.84
DS-2 datalog 2026-09-11	isopropanol	5	-2560 ± 4	+26.9	1919 ± 3	-4.9	0.75
DS-2 datalog 2026-09-11	isopropanol	7	-2908 ± 6	+21.8	2223 ± 2	-6.9	0.76
DS-2 datalog 2026-09-11	isopropanol	9	-3312 ± 8	+22.4	2507 ± 3	-7.4	0.76
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	water	1	-755 ± 1	+12.1	794 ± 0	+17.9	1.05
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	water	3	-1521 ± 1	+30.4	1254 ± 0	+7.4	0.82
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	water	5	-1961 ± 2	+30.2	1451 ± 0	-3.7	0.74
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	water	7	-2230 ± 3	+25.1	1660 ± 1	-6.8	0.74
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	water	9	-2549 ± 5	+26.1	1931 ± 5	-4.4	0.76
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	isopropanol	1	-1016 ± 29	+12.6	1093 ± 47	+21.2	1.08
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	isopropanol	3	-1913 ± 8	+22.4	1545 ± 4	-1.1	0.81
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	isopropanol	5	-2603 ± 14	+29.0	1862 ± 9	-7.7	0.72
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	isopropanol	7	-2950 ± 18	+23.6	2186 ± 6	-8.4	0.74
datalog 2026-09-10 (air $\rightarrow$ ipa $\rightarrow$ water)	isopropanol	9	-3374 ± 47	+24.7	2515 ± 23	-7.1	0.75

11 Remaining experiments before submission

1. Reference impedance analyser on the same crystal, same day, air and water (thru configuration): absolute f_{res} , Γ , R_m , and the reference's own φ (expected ≈ 0).
2. A dedicated air $\rightarrow$ water acquisition with raw sweeps on both instruments, with the liquid temperature logged at the interface, repeated on two days: the reproducibility of Experiment 1 without the confounding of a board and crystal change.
3. Two boards $\times$ two sensors in air and water, overtones 1–9: is $\varphi(n)$ a board constant, and does the fundamental excess follow the sensor or the board.
4. Liquid temperature measured, or a water–glycerol series at controlled temperature with tabulated $\rho\eta$: the absolute KG-3 test over a range, and the absolute $\rho\eta$ of the glucose solutions (literature values at 25 °C to be adopted and cited).
5. Bench calibration of the phase channel: a known phase ramp through 0° (δ and the fold rounding) and an RLC standard in the operating range (0.5–5 k Ω) for $\phi_b(f)$.
6. Long plateau (≥ 1 h) in water with the fit running live beside the conductance maximum: drift, noise, fallback rate, and the two-state behaviour of the 3rd overtone.
7. Larger or switchable divider resistor (0.5–1 k Ω) for liquids: the out-of-roundness and the residual frequency excess against the AD8302 operating point.
8. Sweep window scaled with Γ ($\pm 6 \Gamma$): removes the clipping of the fit window and the baseline-on-skirt bias.
9. Re-acquisition with firmware 0.1.5d (no carry-over) and, for the concentration series, a return to water between solutions and a repeated 5 % point.
10. A third liquid (20–40 % glycerol) and a viscoelastic film: the estimator where $r_n \neq 1$ is expected.

References

- [1] Diethelm Johannsmann. Viscoelastic, mechanical, and dielectric measurements on complex samples with the quartz crystal microbalance. *Physical Chemistry Chemical Physics*, 10(31):4516–4534, 2008. doi: 10.1039/b803960g.
- [2] Diethelm Johannsmann, Arne Langhoff, and Christian Leppin. Studying soft interfaces with shear waves: principles and applications of the quartz crystal microbalance (QCM). *Sensors*, 21(10):3490, 2021. doi: 10.3390/s21103490.
- [3] K. Keiji Kanazawa and Joseph G. Gordon. Frequency of a quartz microbalance in contact with liquid. *Analytical Chemistry*, 57(8):1770–1771, 1985. doi: 10.1021/ac00285a062.
- [4] National Institute of Standards and Technology. Thermophysical properties of fluid systems: water (density from the IAPWS-95 formulation of wagner and pruß, viscosity from the IAPWS 2008 formulation of huber et al.). NIST Chemistry WebBook, SRD 69, <https://webbook.nist.gov/chemistry/fluid/>, 2026. Accessed 2026-10-08; values at 25.000 °C and 0.101325 MPa: 997.048 kg m⁻³, 0.890022 mPa s.
- [5] Manuel Kerscher, Lena M. Braun, Julius H. Jander, Michael H. Rausch, Thomas M. Koller, Peter Wasserscheid, and Andreas P. Fröba. Viscosity, interfacial tension, and density of 2-propanol and acetone up to 423 K by surface light scattering and conventional methods. *International Journal of Thermophysics*, 45(1):8, 2024. doi: 10.1007/s10765-023-03294-z. Open

access (CC BY). Pure 2-propanol and acetone: viscosity and interfacial tension 273–403 K, density 278–423 K at ambient pressure. Title and author list corrected 2026-10-08 to match the DOI (OpenAlex/Springer record); the entry in references_additions_2026-10-08.bib carried the title of a different, unlocated paper on 2-propanol–water mixtures.

- [6] Leonid Daikhin and Michael Urbakh. Effect of surface film structure on the quartz crystal microbalance response in liquids. *Langmuir*, 12(26):6354–6360, 1996. doi: 10.1021/la950763d.
- [7] Leonid Daikhin and Michael Urbakh. Influence of surface roughness on the quartz crystal microbalance response in a solution: new configuration for QCM studies. *Faraday Discussions*, 107:27–38, 1997. doi: 10.1039/a703124f.