


DeepSeek-V3 third scored run: attenuated prefill PASS (max 4.52%)
Unattenuated REFUTED (13.98%); decode calibration 59.83% low

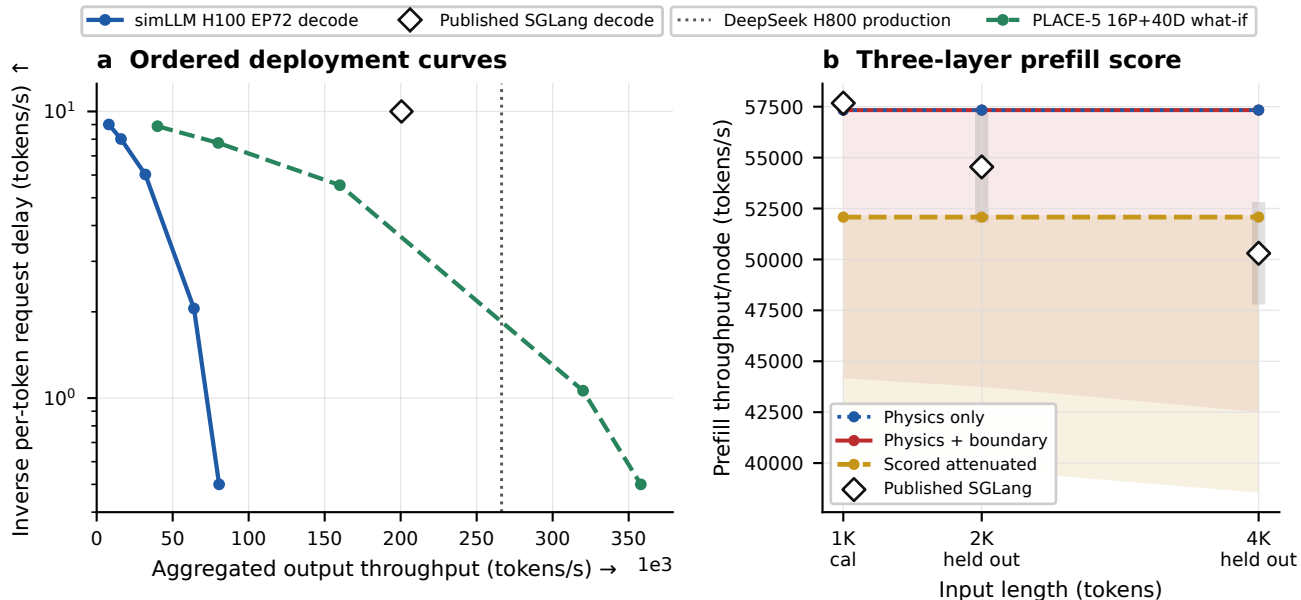

Scored scope: 2K and 4K prefill under the declared benchmark-bias model. expert-balance correction $a=0.90835$, two-SE uncertainty.

MTP BLOCKED on COMP-72, numeric anchor unread. Decode remains unattenuated (28.6 ms declared vs 11.5 ms implied).

Prefill and decode are separate experiments. Bands propagate record, constant, overlap-boundary, attenuation, and registered distribution terms.