



User	Daniel	Cartridge	SNAP KP-Sil 25g
Sample Name	RGS249_CHLOR_MERack Type		16x150 mm
	OH_1%ET3N		
Date	2022-Apr-07 12:57	Max Fraction Volume	22 ml
Method	Chloroform-MeOH-1%Et3N	Solvent A	n-Hexane
Detection Mode	Lambda-all	Solvent C	Chloroform
UV1 (Monitor)	254 nm (Red)	Solvent D	Methanol
UV2 (Monitor)	280 nm (Black)		
Lambda-all (Collect)	(Brown)		



1 A

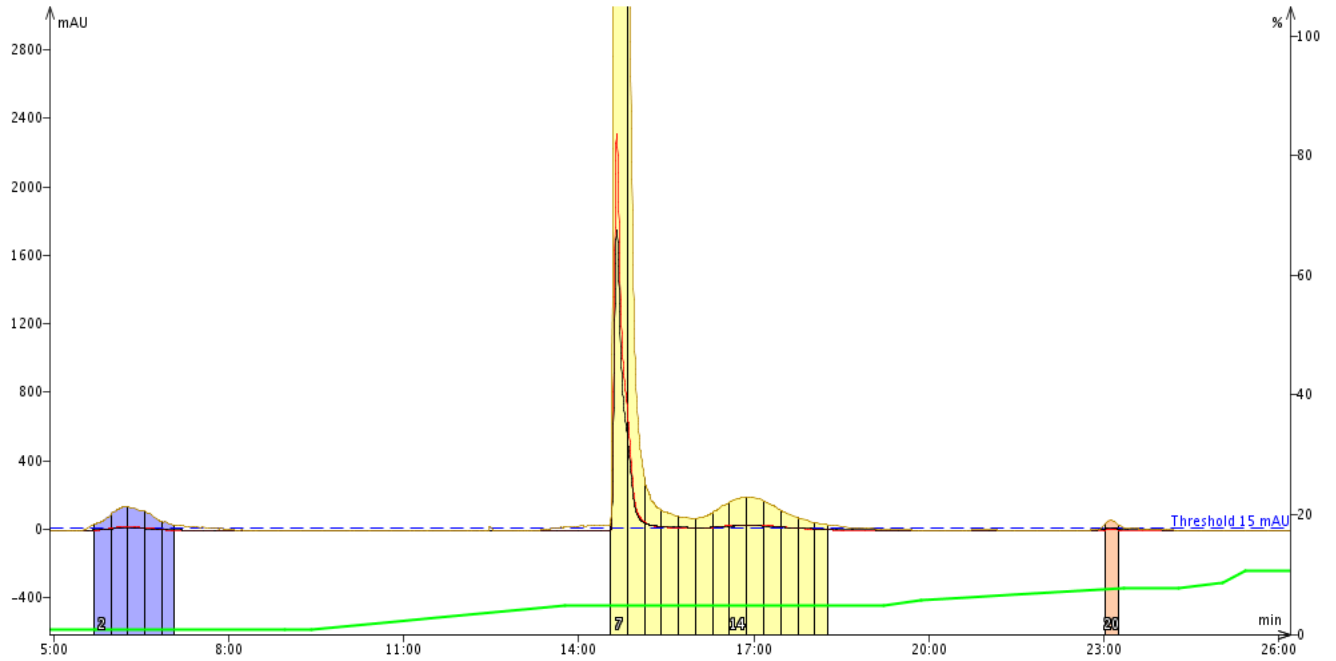