

JM O'Toole*, GB Boylan, EM Dempsey

Neonatal Brain Research Group, INFANT, University College Cork, Ireland

*contact: JOToole@ucc.ie

Background and Aims

Challenges in brain monitoring for preterm infants:

- Up to 30% of preterm infants <32 weeks of gestation develop intra-ventricular haemorrhages (IVH)
- Cranial ultrasound will detect IVH, but 1) required handling can compromise stability of infant and 2) serial measurements only



NIRS device



NIRS probe

Near Infrared Spectroscopy (NIRS):

- Measures regional cerebral oxygenation (rcSO₂)
- Continuous, long-duration (days) measurements of rcSO₂ possible
- Minimal handling required (initial application of probe only)
- Can automated (computer) analysis of rcSO₂ detect IVH?

AIM 1: Remove noise: develop automated method to extract transients and baseline shifts from rcSO₂ signal

AIM 2: Extract features from signal to detect IVH


Methods

Patients rcSO₂ Data

- Recorded continuously for up to 48 hours of life (INVOS 5100c NIRS device with neonatal probe)
- Adverse outcome: any grade of IVH or PVL
- Good outcome: absence of IVH/PVL

SSA Decomposition Method

- Rotate signal 90° in time–frequency domain (use discrete cosine transform, DCT)
- Decompose signal using singular spectrum analysis (SSA); remove noise [1]
- Rotate back in time–frequency domain (inverse DCT)

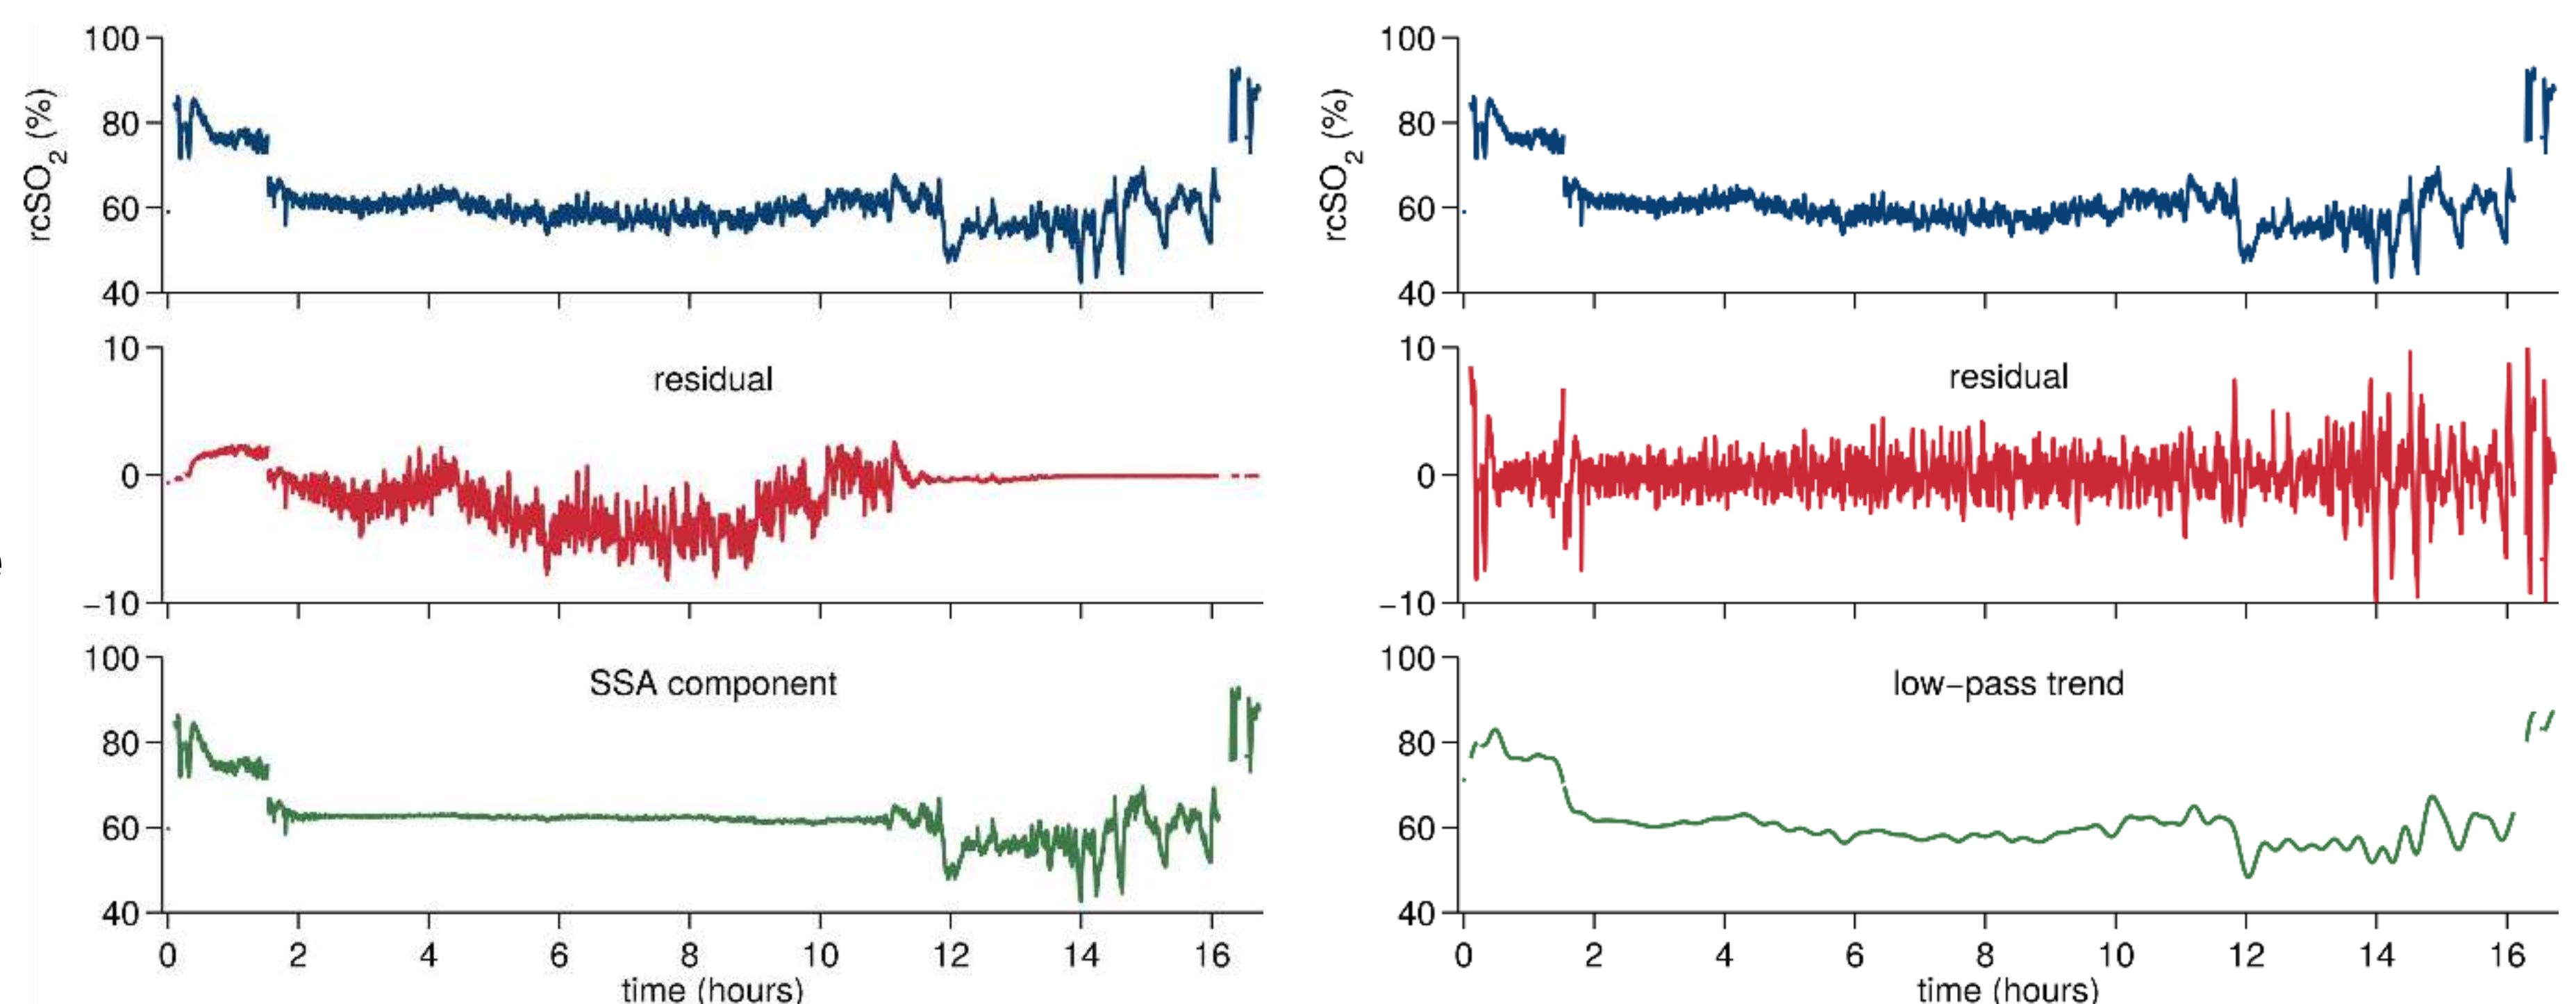


SSA decomposition method (left) differs to low-pass filtering approach (right)


Feature Set

- Filter with dyadic filter bank
- Amplitude modulated (AM) features; frequency modulated (FM) features; and fractal dimension (FD); see [2] for details.

Results and Conclusions

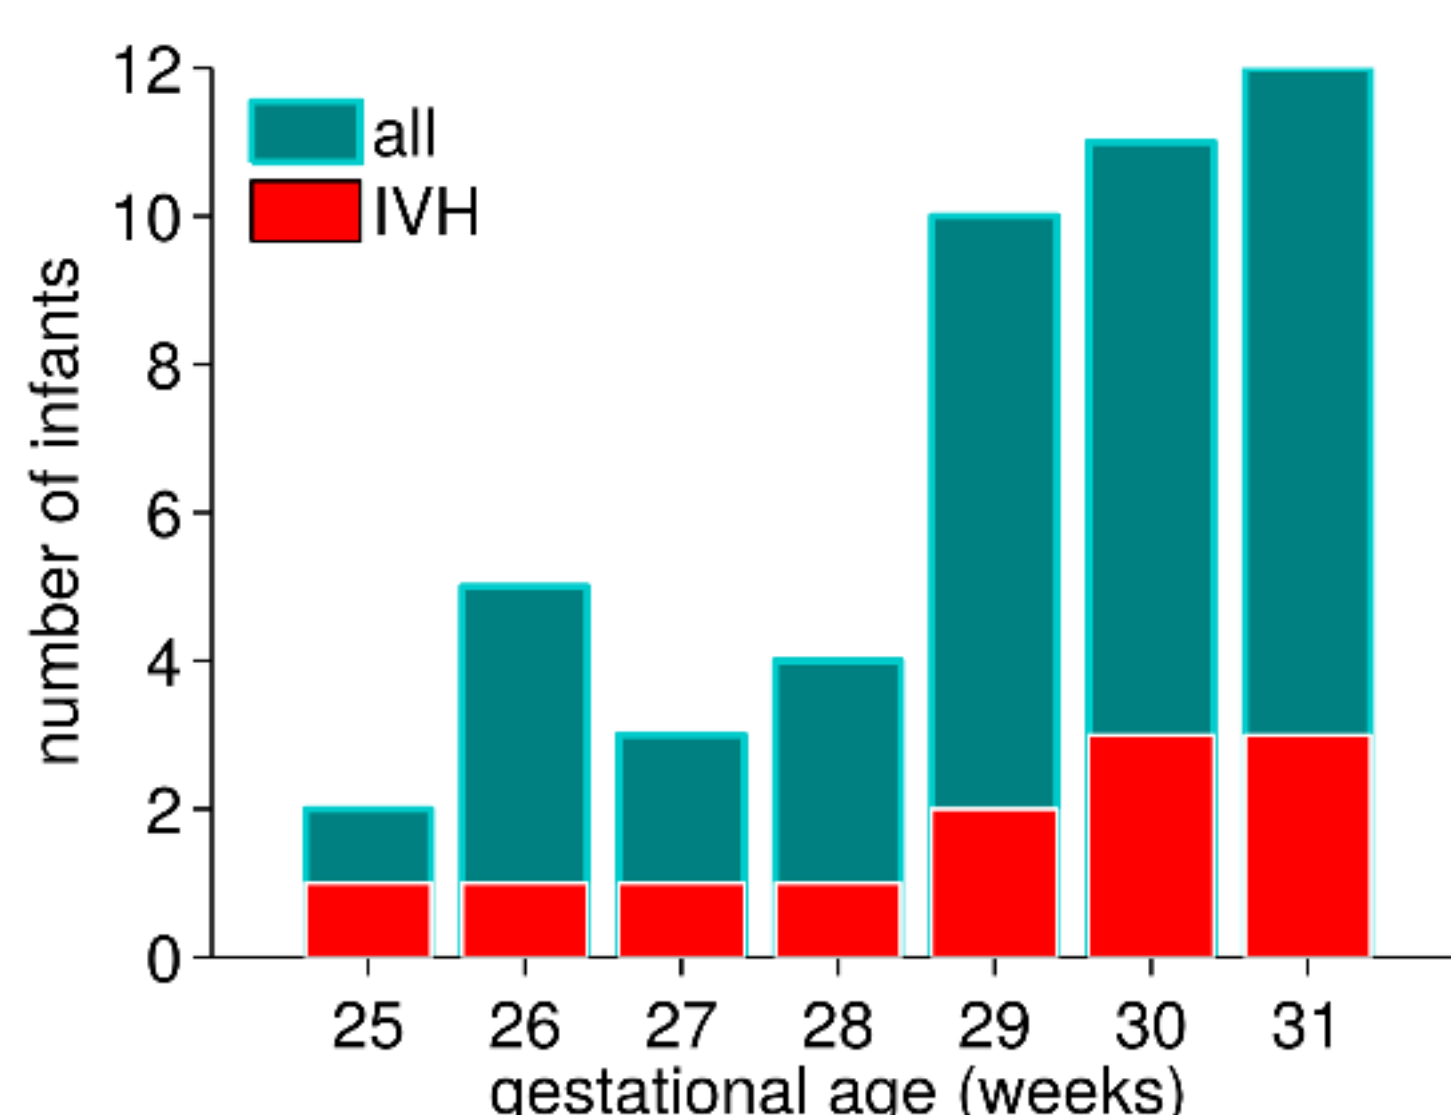

47 preterm infants; 12 with IVH

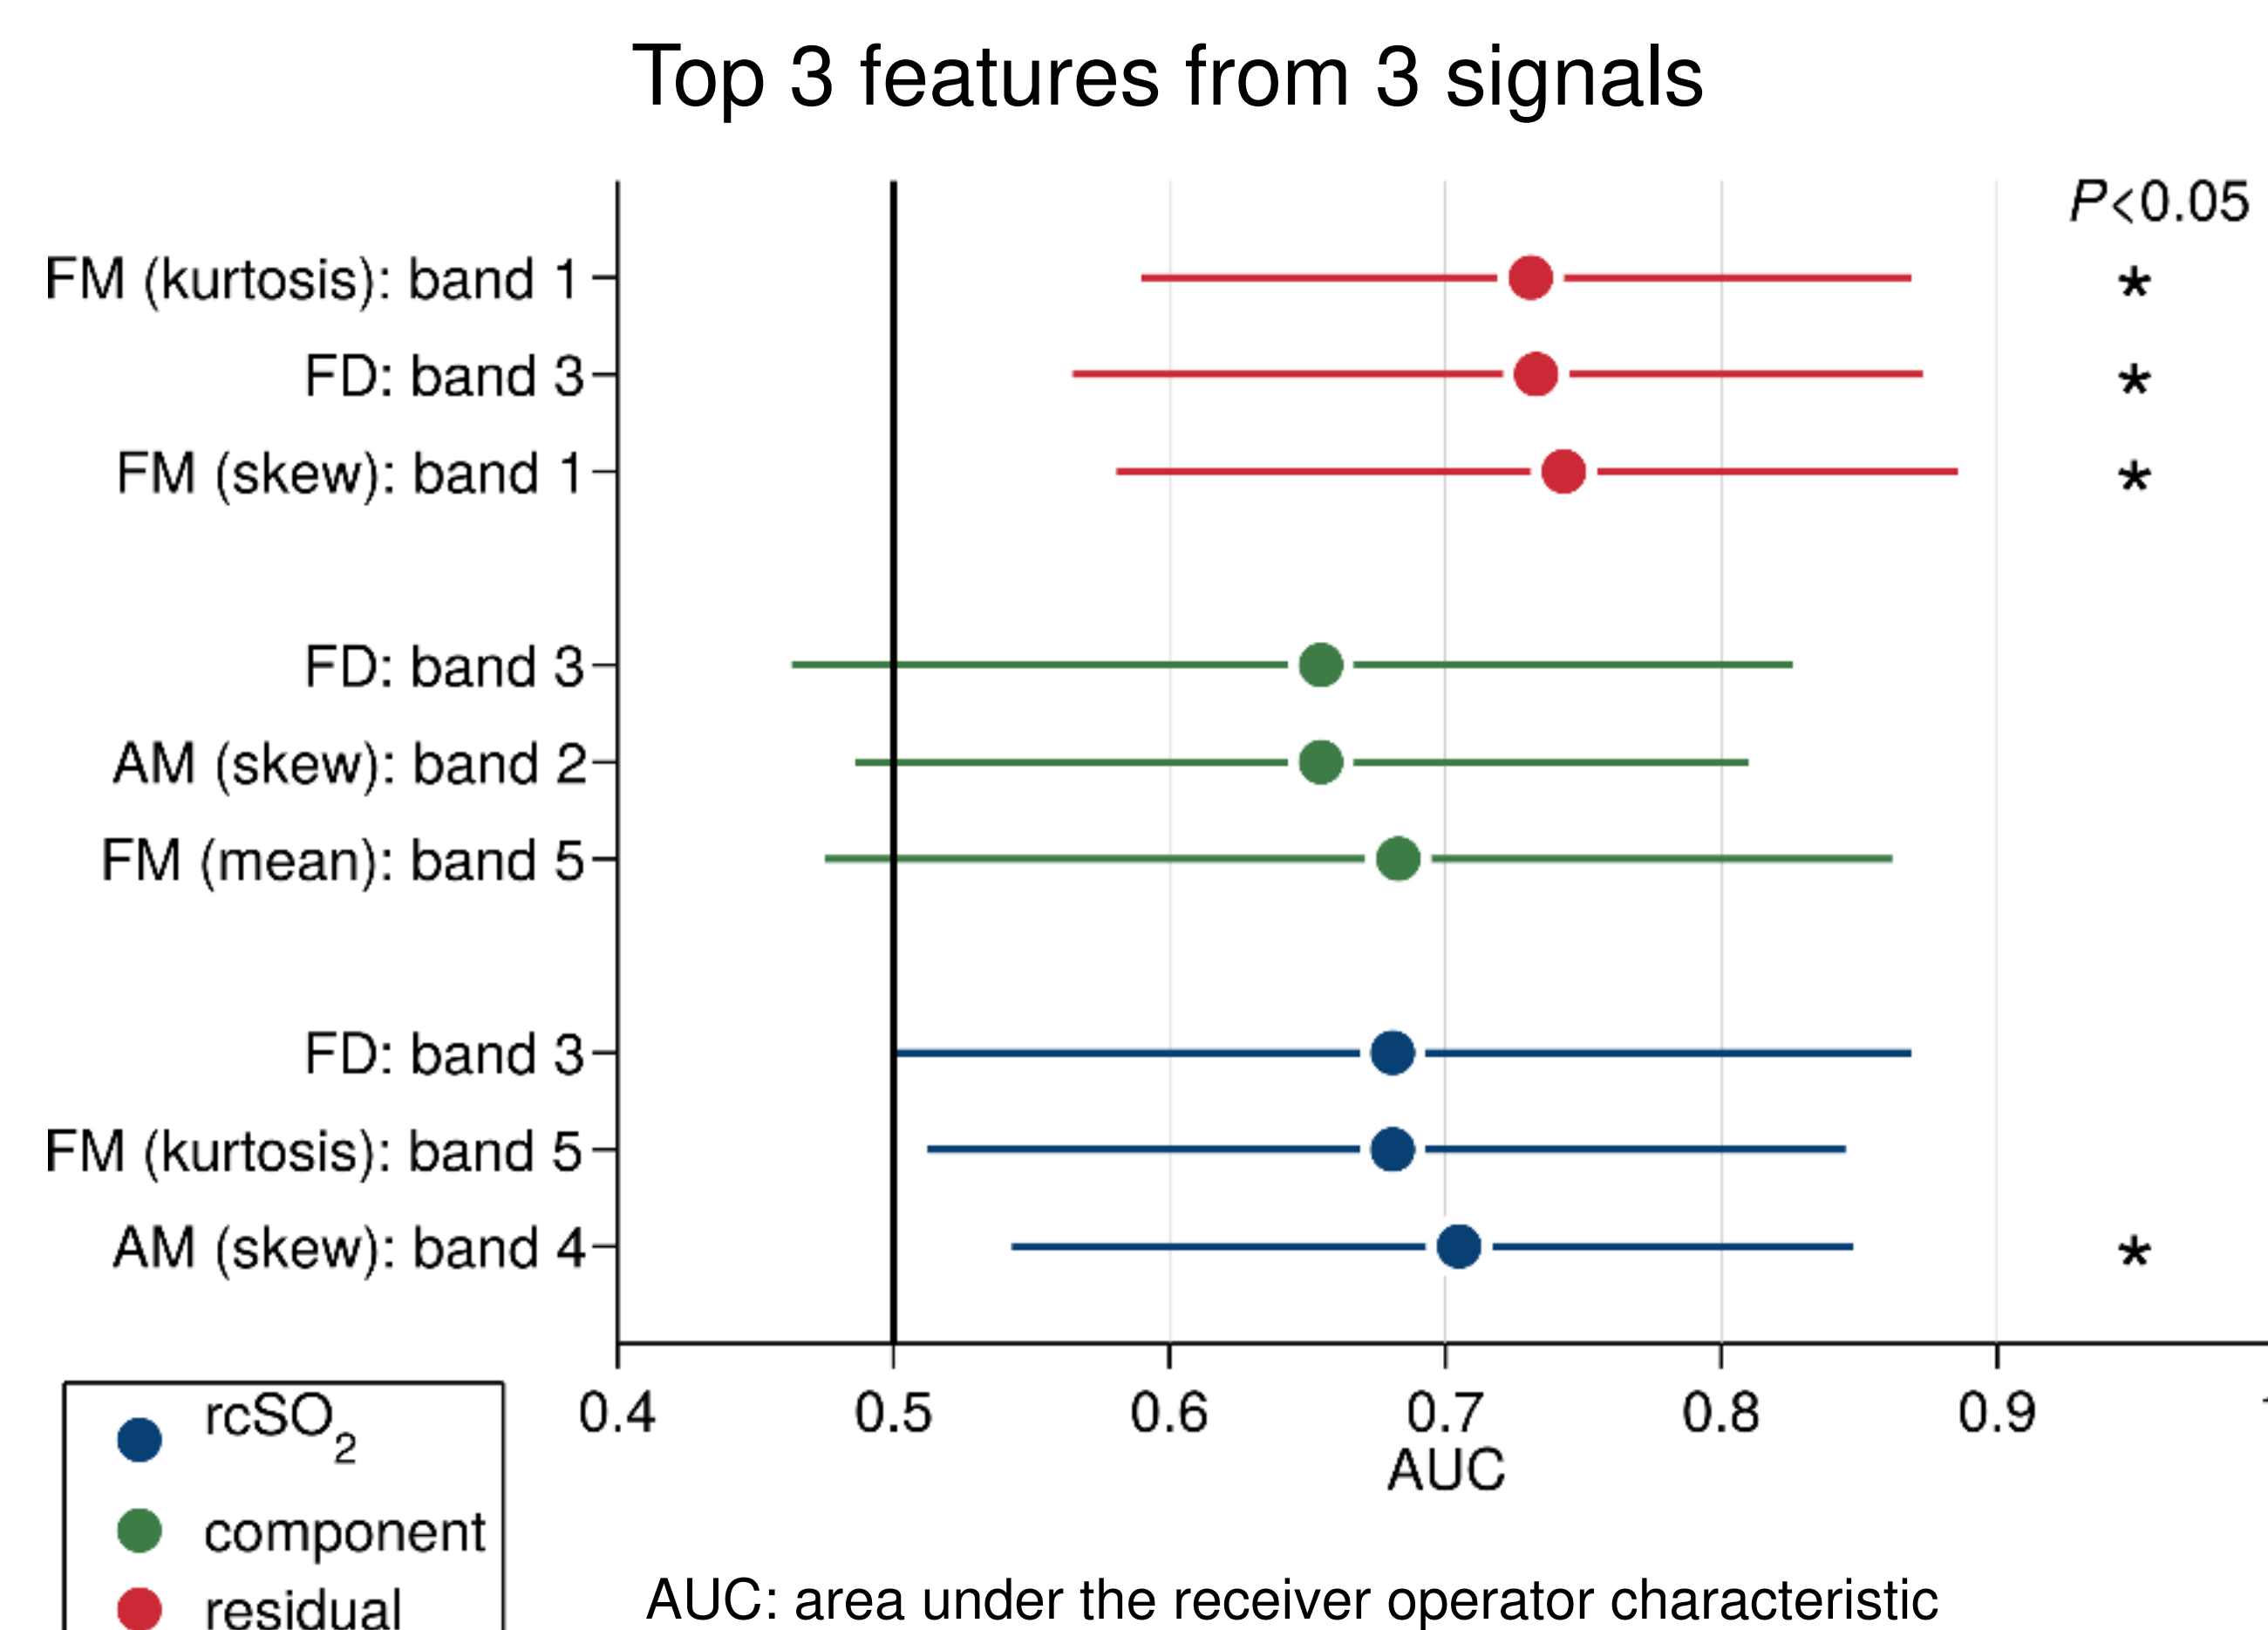

AUC: area under the receiver operator characteristic

Conclusions:

- New decomposition method able to extract components from rcSO₂ with transients and baseline shifts.
- Features from residual signal discriminates between those infants with and without IVH
- Automated analysis of cerebral oxygenation could aid early detection of IVH and help improve outcomes for preterm infants

REFERENCES:

- [1] Vautard R, Yiu P, & Ghil M (1992). Singular-spectrum analysis: A toolkit for short, noisy chaotic signals. Physica D: Nonlinear Phenomena, 58(1–4), 95–126.
- [2] O'Toole JM, Kenosi M, Finn D, Boylan GB, & Dempsey EM. (2016). Features of cerebral oxygenation detects brain injury in premature infants. In IEEE 38th Int Conf EMBC, Aug. (pp. 3614–3617).