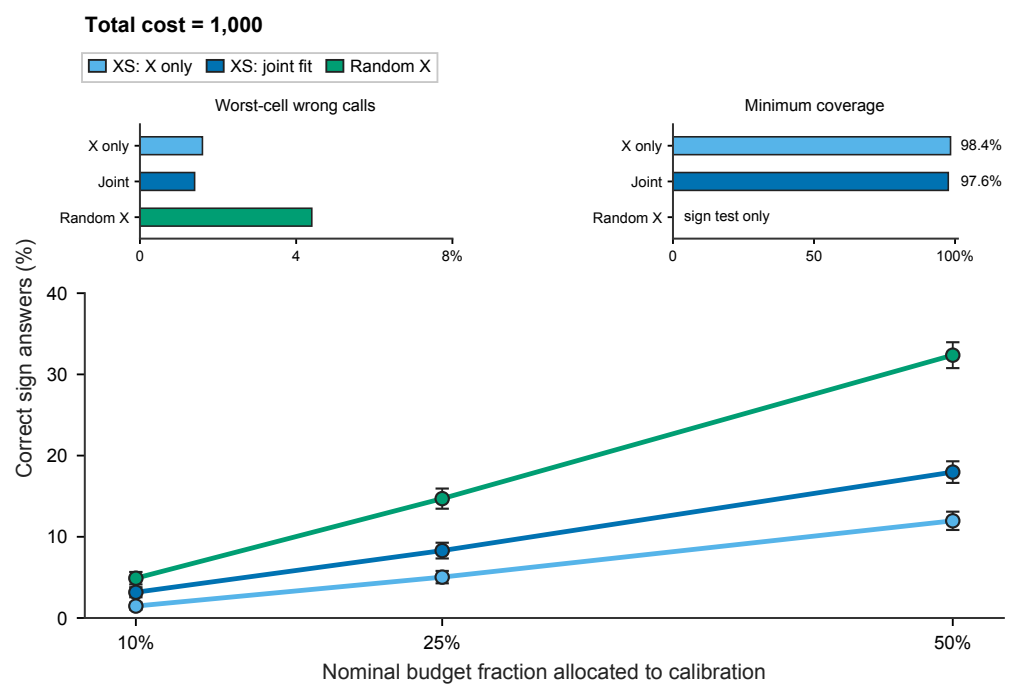

Total cost = 1,000
XS: X only
XS: joint fit
Random X
Worst-cell wrong calls
X only
Joint
Random X
0
4
8%
Minimum coverage
X only
Joint
Random X
98.4%
97.6%
sign test only
0
50
100%
Correct sign answers (%)
0
10
20
30
40
10%
25%
50%
Nominal budget fraction allocated to calibration