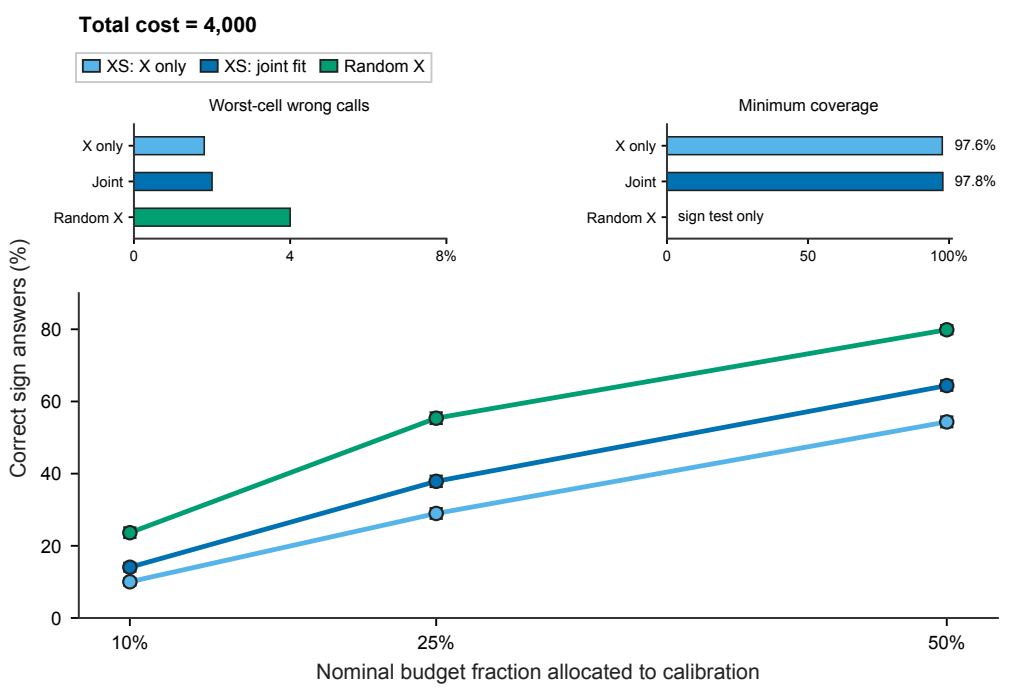

Total cost = 4,000
XS: X only
XS: joint fit
Random X
Worst-cell wrong calls
X only
Joint
Random X
0
4
8%
Minimum coverage
X only
Joint
Random X
97.6%
97.8%
sign test only
0
50
100%
Correct sign answers (%)
0
20
40
60
80
10%
25%
50%
Nominal budget fraction allocated to calibration