

A systematic evaluation of machine learning classifiers for event-by-event background rejection in LAFOV PET scanners

Konrad Klimaszewski^{1,*} ([ORCID: 0000-0003-0741-5922](#)), Michał Obara¹ ([ORCID: 0009-0006-4779-6757](#)), Mateusz Bala¹ ([ORCID: 0000-0002-2505-7949](#)), Beatrix C. Hiesmayr^{2,3} ([ORCID: 0000-0001-9062-6039](#)), Lech Raczyński¹ ([ORCID: 0000-0002-7039-2084](#)), Roman Y. Shopa¹ ([ORCID: 0000-0002-1089-5050](#)), Wojciech Zdeb¹ ([ORCID: 0009-0000-1485-251X](#)), Wojciech Krzemien^{4,*} ([ORCID: 0000-0002-9546-358X](#))

¹*National Centre for Nuclear Research, Department of Complex Systems, 05-400 Otwock, Poland*

²*IT:U Interdisciplinary Transformation University, Freistädter Strasse 400, 4040 Linz, Austria*

³*University of Vienna, Faculty of Physics, Währingerstrasse 17, 1090 Vienna, Austria and*

⁴*National Centre for Nuclear Research, Department of High Energy Physics, 05-400 Otwock, Poland**

Abstract

The introduction of Long Axial Field-of-View PET scanners brings significant sensitivity gains but also a substantial increase in the background rate from accidental coincidences, phantom-scattered and detector-scattered photons. While machine learning methods have been applied to background reduction in PET imaging, existing approaches target specific background components in post-processing rather than performing event-by-event classification on the raw data. In this work, we formulate coincidence classification as a supervised multi-class problem and evaluate Boosted Decision Tree (XGBoost, AdaBoost) and Artificial Neural Network classifiers as pre-reconstruction filters, using Monte Carlo simulations of the Siemens Biograph Vision Quadra scanner with NEMA IEC and anthropomorphic XCAT phantoms. We investigate two feature sets: a 4-feature representation based on the Attenuation Factor (AF), photon time difference (dt), energy sum, and energy difference, and an extended 6-feature set that additionally incorporates topology-based variables. A systematic robustness study via cross-phantom inference reveals that the 4-feature models generalise significantly better across different phantom geometries, with XGBoost suffering an accuracy loss of only 0.04 compared to 0.13 for the 6-feature variant. The Attenuation Factor and time difference are identified as the most discriminating features across all models and phantoms. Our best models achieve accuracies of up to 0.74 and 0.69 for the NEMA IEC and XCAT phantoms, respectively, outperforming traditional geometry-based cuts. However, we show that this compact feature set not only provides limited suppression of in-phantom scattered coincidences, but it also can lead to non-trivial spatial patterns in classifier performance characteristics. With scattered coincidences being the dominant background component in clinical conditions, this suggests that while the method serves as an effective and geometry-agnostic replacement for traditional cut-based selection, meaningful further gains in image quality will require either larger input representations or dedicated treatment of the phantom-scattered component.

I. INTRODUCTION

Positron Emission Tomography (PET) is a widely used medical imaging modality that enables quantitative measurements of metabolic processes *in vivo*. One of the current trends

* konrad.klimaszewski@ncbj.gov.pl and wojciech.krziemien@ncbj.gov.pl

in PET scanner development is the introduction of Long Axial Field of View (LAFOV) systems with improved time-of-flight (TOF) capabilities, which cover a considerably larger portion of the patient’s body than conventional scanners. The principal advantage of such systems is their significantly higher sensitivity, which can improve image resolution, enable dynamic whole-body imaging, shorten scan duration, or reduce the radiation dose delivered to the patients [Esquinas *et al.* \(2026\)](#), [Karakatsanis \(2026\)](#), [Slart *et al.* \(2021\)](#), [Surti, Pantel, and Karp \(2020\)](#). Indeed, several such systems are already in clinical operation [Badawi *et al.* \(2019\)](#), [Pantel *et al.* \(2020\)](#), [Prenosil *et al.* \(2022\)](#), [Yamagishi *et al.* \(2023\)](#), while additional concepts continue to be proposed and developed [Baran *et al.* \(2025\)](#), [Vandenberghe *et al.* \(2023\)](#).

However, the increased axial coverage of LAFOV scanners operating in a fully 3D mode comes at a cost: a higher background level that degrades image quality.

In PET, a radiopharmaceutical is administered to the patient. Depending on the tracer, it accumulates in regions characterised by a particular biological process – for example, elevated glucose metabolism in the case of fluorodeoxyglucose. The radioactive isotope undergoes β^+ decay, producing a positron that annihilates with an electron from the patient’s body, resulting in the emission of a pair of nearly back-to-back 511 keV photons. These photons are detected in coincidence by the scanner, with each detected event characterised by its deposited energy, interaction time, and spatial position within the detector. Each pair defines an Line of Response (LOR), and is passed to the image reconstruction algorithm. The spatial density of reconstructed annihilation points forms an image that can be subsequently analysed by a physician, for example, to identify cancerous lesions.

Ideally, each coincidence corresponds to an unperturbed pair of photons originating from a single annihilation point (*true* event). In practice, however, due to finite detector resolution and physical interaction processes, the coincidence set contains not only *true* events but also a fraction of background pairs. This background consists of three principal components. First, accidental coincidences are formed from photons originating from different annihilation events, whose rates are of a combinatorial nature and increase approximately quadratically with the activity and axial length of the scanner. Second, phantom-scattered coincidences arise when one or both photons undergo Compton scattering within the patient’s body before reaching the detector, thereby altering their direction and energy. In the case of LAFOV scanners, the contribution of multiply scattered photons becomes increasingly important. Finally,

photons that undergo more than one interaction within the scanner detection system can be incorrectly assigned as a genuine photon pair, giving rise to so-called *detector-scatter* events. The occurrence and spatial distribution of these background coincidences depend on multiple factors, including scanner geometry, detector properties, and activity distribution within the patient. For LAFOV scanners, the acceptance of more oblique LORs increases the sensitivity but can lead to an increase in terms of the scatter and random fractions [Daube-Witherspoon *et al.* \(2022\)](#).

Conventional approaches to background suppression rely primarily on energy thresholds and geometrical constraints applied to the line of response. However, such methods are inherently limited in their ability to distinguish between signal and background events that share similar kinematic properties [Brasse *et al.* \(2005\)](#). Moreover, background reduction inevitably entails a partial loss of *true* events, thereby reducing the overall system sensitivity. Consequently, background suppression in PET represents a trade-off between maximising sensitivity and minimising background contamination.

The application of machine learning techniques to PET data processing has grown considerably in recent years [Arabi *et al.* \(2021\)](#), with Machine Learning algorithms being used at various stages of the reconstruction pipeline, ranging from raw data filtering to enhancement of the reconstructed image [Reader *et al.* \(2021\)](#).

In the case of scattered and accidental coincidences, most of the recent works focus on corrections in image or sinogram space [Laurent *et al.* \(2023\)](#). There are only a few existing approaches that target background reduction on an event-by-event basis at the raw coincidence level, prior to image reconstruction. Operating at this level is advantageous, as it allows individual photon properties to be taken into account, and the resulting method is not tied to a specific reconstruction method – it can be naturally extended to multiphoton imaging, as well as to other imaging modalities such as Positron Emission Particle Tracking. [Oliver *et al.* \(2013\)](#) considered the application of an Artificial Neural Network (ANN) for accidental coincidence reduction in small animal PET, a significantly simpler setting than clinical LAFOV imaging. As this work focused on accidental coincidences, neither scatter nor attenuation in the phantom was simulated. The authors did not consider factors such as the spatial uniformity of the classifier response. Instead, they used overall image quality metrics, such as the Contrast Recovery Coefficient (CRC) or the spillover ratio (SOR). An interesting approach to recover, usually discarded, Inter-Crystal Scatter (ICS) triple coincidences was

proposed by [Michaud *et al.* \(2015\)](#). An ANN is used to classify the true photon pair within the three detected photons. The model does not classify phantom-scattered and accidental coincidences, and only standard accidental compensation is applied during image reconstruction. While the authors verify their method using a Derenzo phantom, the model’s performance is confounded by the reconstruction quality in this setting. As the spatial uniformity of the classifier response is not discussed, it is hard to judge if any dependence is observed. A detailed study of various classifiers for background reduction from ^{176}Lu radiation was presented by [Wang *et al.* \(2020\)](#). In particular, the performance of eXtreme Gradient Boosting (XGBoost) and ANN classifiers is compared; the focus is on reducing the ^{176}Lu background, with classification of accidental and scattered coincidences left for further studies. As in [Michaud *et al.* \(2015\)](#), the authors validate their method using volumetric phantoms, including Derenzo and planar bars. Also, in this case, the spatial uniformity of the classifier response is not discussed. In a recent study by [Debus *et al.* \(2024\)](#), the use of Spiking Neural Networks was proposed as a replacement for traditional coincidence sorters. As this work focuses on what constitutes a coincidence, it does not address the problem of scattered coincidences. Moreover, the authors consider only a centrally positioned point source, without accounting for possible dependence of the method’s performance on the source position within the scanner. While all of those works verify the performance of the classifier on out-of-distribution data, they are limited to training the machine learning model on a phantom that covers all or most of the scanner FOV and to application to other phantoms. To our knowledge, no study has examined the impact of training data selection on the model performance for PET background reduction on an event-by-event basis.

In this contribution, we formulate coincidence classification as a supervised multi-class learning problem, applied event-by-event at the raw-data level, prior to image reconstruction, and evaluate its applicability to LAFOV PET background reduction. We compare two classifier families: Boosted Decision Tree (BDT)s and ANN networks trained on Monte Carlo (MC) simulations of the Siemens Biograph Vision Quadra scanner using two phantoms: the standard NEMA IEC PET (NEMA IEC) phantom and the anthropomorphic 4D eXtended CArdiac-Torso (XCAT) phantom. We perform a systematic study of feature selection, model generalisation across phantom geometries, and the impact of classifier hyperparameter selection. In addition to standard classification metrics, we evaluate the classifier’s impact on the reconstructed spatial distribution of the radio-tracer, which is crucial for image quality.

For this purpose, we propose an activity-agnostic method to visualise the model performance metrics, such as accuracy, as a three-dimensional map. Such an approach enhances the model evaluation beyond reliance on global performance metrics. We show that a modest difference in a global metric, such as accuracy, can result from severe performance degradation in a particular image region, with no change in most of the volume.

Our findings establish the performance level of this approach with a minimal feature set and identify the conditions under which it can serve as a practical, geometry-agnostic replacement for traditional cut-based coincidence rejection.

The rest of the article is structured into five sections. The Materials and Methods section [II](#) begins with the formulation of the background reduction problem in terms of supervised classification with a description of the considered models. Next, we briefly define the evaluation metrics and discuss the input data generation and its characteristics. The section concludes with a discussion of model hyperparameter selection, followed by an overview of the feature selection. The results section [III](#) presents the obtained classifier performance in terms of global performance metrics. A discussion of the impact of feature selection on the model performance and robustness to out-of-distribution data is provided in section [IV](#). Finally, section [V](#) provides the results summary and discusses the prospects and possible future extensions of the methods.

II. MATERIALS AND METHODS

A. Machine Learning approach

The problem of background reduction due to scatter and accidental coincidences can be formulated as a classification problem. We consider a P -dimensional feature space $\mathcal{X} \in \mathbb{R}^P$. The vector $\vec{x} \in \mathcal{X}$ describes an event corresponding to a registered photon pair. The goal is to find a classifier function $f : \mathcal{X} \rightarrow \mathcal{Y}$ that maps the vector of features to a class type $\vec{y} \in \mathcal{Y}$. In our case, the categorical output space $\mathcal{Y}$ consists of four classes corresponding to the physical coincidence types defined in section [III E](#). The optimal classifier f^* is defined with respect to an objective function $O(f(\vec{x}_i), y_i)$, which typically consists of two parts: loss function $L(f(\vec{x}_i), y_i)$ and the regularization term $\Omega(f(\vec{x}_i))$. The loss function quantifies the quality of the prediction $f(\vec{x}_i)$ for the given event described by the feature vector $\vec{x}_i$,

compared to the expected class y_i . The role of the regularisation term is to limit the model's complexity. This helps to mitigate the problem of overfitting, the situation in which the model learns perfectly the characteristics of the sample on which it was trained; however, it performs poorly when classifying events not seen before. This optimisation task is solved by minimising the objective function, calculated based on the training sample composed of the N events with the assigned labels: $T = [[\vec{x}_1, y_1], \dots, [\vec{x}_N, y_N]]$. Hence, the problem can be treated as an example of supervised learning.

Our classification models are based on two classes of machine learning algorithms: BDT and ANN networks. Both model classes are well established, with their properties thoroughly studied. Moreover, compared to newer architectures, they are extremely fast. Both properties make them good candidates for background reduction in a medical setting.

Our BDT classifiers are constructed based on libraries: XGBoost [Chen and Guestrin \(2016\)](#), which is a current state-of-the-art BDT implementation, and Adaptive Boosting (AdaBoost) [Freund and Schapire \(1997\)](#), one of the first robust BDT algorithms. In the following paragraph, the main ideas of decision tree-based classifiers and the boosting method are briefly discussed. A decision tree – Classification and Regression tree (CART) – is a simple predictive model that can be used for classification or regression. It consists of a chain of rules represented by nodes and branches. Each node represents a test based on a single feature that splits the set of classified objects into subsets and assigns scores to the subsets. The choice of a feature and the value at which the split is performed are determined by splitting rules. The splitting process is repeated recursively until the subsets contain objects belonging to only one class, or until further splitting no longer improves the prediction score. The terminal leaves are associated with the output classes. The classification based on the trained decision tree can be seen as a chain of 'yes-no' questions. Since a single split corresponds to a linear division of the feature space along a given feature dimension, the final decision boundary, corresponding to the given tree model, divides the feature space into a hyperrectangle.

Decision trees are weak predictive models due to the high tendency to overfit. Therefore, instead of using a single tree, the better approach is to use a set of decision trees and combine their predictions. There are several methods of combining the set of trees. Boosting is a general method of generating many simple classification rules (weak classifiers) and combining them into a single, highly accurate classifier [Freund and Schapire \(1997\)](#).

This strategy is not limited to decision trees; rather, it is a general scheme and can be applied to other classification models, e.g., logistic regression or even deep neural networks.

The key idea of boosting consists of forming a cumulative predictor by adding subsequent weak classifiers sequentially, where each new classifier is trained to correct the mistakes of its predecessor. Formally, the prediction at boosting iteration t is given by the additive model:

$$\hat{y}_i^{(t)} = \sum_{k=1}^t f_k(\vec{x}_i) \quad (1)$$

where each f_k denotes the k -th decision tree added to the ensemble and the sum runs over t trees in the current iteration. The final ensemble prediction runs over all T trees. To control model complexity and reduce overfitting, a regularisation term is added to the objective function for each tree f :

$$\Omega(f) = \gamma L + \frac{1}{2} \lambda \sum_{j=1}^L w_j^2 \quad (2)$$

where the sum runs over all leaves L of the tree, w_j is the score assigned to the j -th leaf, γ is a penalty on the number of leaves that controls tree depth, and λ is an L2 regularisation coefficient that penalises large leaf weights. Both γ and λ are hyperparameters, whose values are determined during the optimisation procedure described in section II B.

The trees are added greedily, one per iteration. At iteration t , the new tree f_t is chosen to minimise the regularised objective

$$\mathcal{L}^{(t)} = \sum_i l(y_i, \hat{y}_i^{(t-1)} + f_t(\vec{x}_i)) + \Omega(f_t), \quad (3)$$

where l is the per-sample loss (here the multiclass cross-entropy, i.e. the `multi:softprob` objective). Since the loss cannot in general be optimised directly over tree structures, XGBoost approximates it by a second-order Taylor expansion around the current prediction $\hat{y}_i^{(t-1)}$, so each point contributes a gradient $g_i = \partial_{\hat{y}} l$ and a second derivative $h_i = \partial_{\hat{y}}^2 l$. For a fixed tree structure the objective is then minimised analytically. Because the space of structures cannot be searched exhaustively, each tree is grown by recursively splitting nodes, retaining at every step the split that maximises the *gain* defined as:

$$gain = \frac{1}{2} \left[\frac{G_L^2}{H_L + \lambda} + \frac{G_R^2}{H_R + \lambda} - \frac{(G_L + G_R)^2}{H_L + H_R + \lambda} \right] - \gamma \quad (4)$$

with $G_{L(R)} = \sum_i g_i$ and $H_{L(R)} = \sum_i h_i$ the sums of the gradients g_i and second derivatives h_i over the data points assigned to the left (right) child after the split, and λ , γ the regularisation terms.

AdaBoost grows its CART trees analogously, but selects at each node the split maximising the Gini-impurity decrease, where impurity is defined in Eq. (5), and trains successive trees on reweighted samples so that each focuses on its predecessor’s errors. The impurity decrease is the difference between a node’s impurity and the Gini index — a weighted sum of the impurity measures of the two child nodes. The impurity of a node n is defined as:

$$\widehat{\Gamma}(n) = \sum_{j=1}^J \widehat{\phi}_j(n)(1 - \widehat{\phi}_j(n)) \quad (5)$$

where $\widehat{\phi}_j(n)$ denotes the frequency of class j in node n .

For our ANN model, we use the Multi-Layer Perceptron (MLP) architecture. An MLP is a foundational class of artificial neural networks. Structurally, an MLP comprises at least three sequential layers of interconnected nodes: an input layer to receive the initial data, one or more hidden layers to extract underlying patterns, and an output layer to yield the final prediction. Information propagates unidirectionally from input to output, with each node in the hidden and output layers serving as a computational unit with a non-linear activation function, such as a rectified linear unit (ReLU) or a sigmoid. This non-linearity, combined with a hidden layer, enables the network to map high-dimensional feature spaces to target variables. The network optimises its internal parameters through supervised learning with the backpropagation algorithm, which iteratively updates inter-node connection weights and node biases via gradient descent to minimise a predefined loss function.

Our MLP implementation, built with the Keras library [Chollet *et al.* \(2015\)](#), comprises a variable number M of hidden layers, each containing a variable number N of neurons. Both N and M are treated as hyperparameters of the model, and their selection is described in section [II B](#). Each hidden layer utilises the ReLU activation function and is followed by a Dropout layer. The output layer is composed of several neurons equal to the number of considered coincidence classes, with Softmax as the activation function. The model is optimised using the Adam algorithm [Kingma and Ba \(2014\)](#) with a sparse categorical cross-entropy loss function.

It should be noted that there exist additional, domain-specific requirements that a candidate classifier must fulfil. For example, the classifier should be generic, in the sense

that it cannot depend on the details of the phantom geometry. Also, since the final objective is the patient’s body image, the classification procedure cannot introduce any artefacts into the reconstructed image.

B. Hyperparameter selection

The model hyperparameters are selected using Bayesian Optimisation [Brochu, Cora, and de Freitas \(2010\)](#). It is a powerful optimisation technique for functions that are costly to evaluate, especially when derivatives are not available. It is particularly well suited to hyperparameter optimisation of machine learning models. The goal of this approach is to minimise the number of function evaluations by making informed decisions about which point in the hyperparameter space to evaluate next. It is done by replacing the function with a surrogate model that is easy to evaluate and update with results of previous evaluations. A common selection for the surrogate model is the Gaussian Process [Mockus \(1994\)](#). The selection of the next evaluation point is based on an acquisition function that balances exploration and exploitation. Exploration is understood as probing areas with high variance in the surrogate model; hence, the probable gain is high but uncertain. Exploitation involves probing regions where the optimised function is already known to be large. A common selection for the acquisition function is the Expected Improvement [Jones, Schonlau, and Welch \(1998\)](#). For the presented results, an open-source implementation of Bayesian Optimisation from the scikit-optimize package [Head *et al.* \(2021\)](#) was used, with a Gaussian Process for the surrogate function and Expected Improvement as the acquisition function. At each function evaluation by the procedure, a three-fold stratified cross-validation was performed, preserving the class ratios in each fold. The mean accuracy from the three folds was used to update the surrogate model. The best model was refit on the full training sample.

In Table [IV](#), a list of considered hyperparameters for each model is presented along with the range of allowed values and the type of prior used for sampling the next point to evaluate, along with the results of the optimisation. An example of the obtained accuracy distribution as a function of parameter values is presented in Fig. [1](#). Distributions for all considered models and hyperparameters are provided in Appendix [A](#).

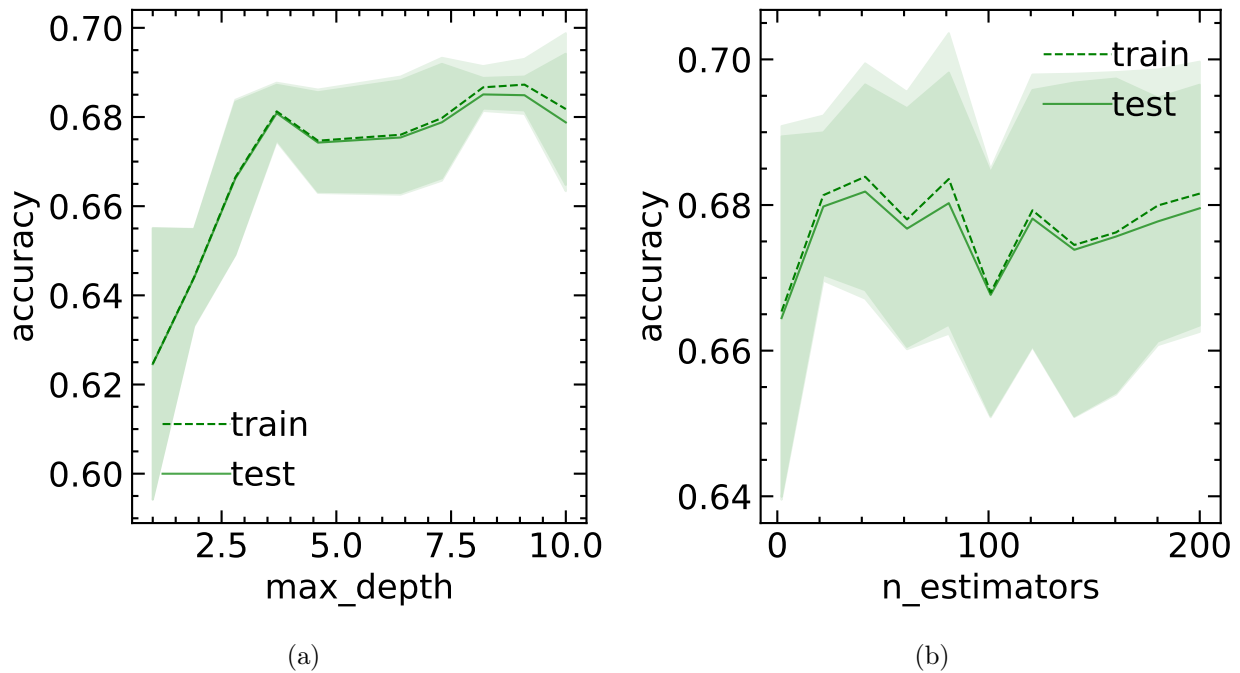


Figure 1. Example of observed dependence of the accuracy on model hyperparameters for the 6-feature XGBoost model trained on the XCAT sample.

C. Detector simulation

The studies were performed based on MC simulations that modelled PET measurements, carried out with the Siemens Biograph Vision Quadra, a LAFOV PET/CT system [Prenosil *et al.* \(2022\)](#). The Geant4 Application for Tomographic Emission (GATE) v9.4.1 [Sarrut *et al.* \(2022, 2021\)](#) simulation library, based on Geant v4.11.3.0 [Agostinelli *et al.* \(2003\)](#), has been used to model the data taking by the PET scanner. The interaction of particles with matter was simulated by using the `em_livermore_polar` physics list. Tracking of optical photons was switched off to reduce computation time. The simulation starts with isotropic emission of back-to-back photon pairs, with the initial energy set to 511 keV.

The GATE geometry of the scanner consists of 38 detection element arrays (rsectors) repeated in a ring with a radius of 420 mm, replicated 4 times along the axial direction for a total axial field of view of 1060 mm. Each rsector contains 8 detector modules arranged axially, each comprising 4×2 miniblocks of 5×5 lutetium oxyorthosilicate (LSO) crystals with individual dimensions of $3.2 \times 3.2 \times 20 \text{ mm}^3$, giving 243,200 crystals in total arranged in 320 crystal rings.


The front-end electronic response was modelled by the GATE digitiser, which converts photon interactions in the scintillator crystals into deposited energy and detection time. Energy depositions within the same crystal were summed, and a readout grouping at the crystal level was applied. The energy resolution was parametrised as 9% full width at half maximum at 511 keV. Only single events with deposited energy within the 435–585 keV window were accepted. Coincidences were formed from pairs of singles detected within a 4.7 ns timing window, requiring a minimum sector difference of 1. The timing resolution was applied in post-processing by smearing the detection times with a Gaussian of $\sigma_t = 93$ ps, corresponding to a Coincidence Resolving Time of 219 ps. Additionally, the position of each photon interaction was discretised to the centre of the crystal in which the energy was deposited.

D. Phantoms


Two experimental setups were chosen for the simulations: NEMA IEC [NEMA \(2018\)](#) and XCAT [Segars *et al.* \(2010\)](#) phantoms. The 22 cm long NEMA IEC phantom is built out of four high-activity (denoted as *hot*) and two low-activity (denoted as *cold*) spheres. The phantom is positioned isocentrically within the scanner. Hot spheres of 10 mm, 13 mm, 17 mm and 22 mm diameters and cold spheres of 28 mm and 37 mm diameters were simulated. The ratio between the hot spheres and the background was set to 4:1. The total activity of 50 MBq was simulated, and the acquisition time was set to 100 seconds.

The activity of the male XCAT phantom was prepared [Silva-Rodríguez *et al.* \(2015\)](#), [Zincirkeser *et al.* \(2007\)](#) to mimic the ^{18}F -FDG distribution within the human body. Additionally, two hot spheres (diameter = 1.2 cm) positioned in the lung and liver were incorporated into the phantom simulations. The contrast between the hot region and the background activity was set to 16:1 and 3:1 for the lungs and liver, respectively. The phantom’s overall activity was 50 MBq, and the acquisition time was set to 1000 seconds. The XCAT phantom activity map is depicted in Fig. 2a, while the NEMA IEC phantom activity map is depicted in Fig. 2b.

For each dataset, we extract randomly two subsamples: a training sample of $2.4 \cdot 10^6$ coincidences and an independent testing sample of $0.6 \cdot 10^6$ coincidences. As described in section II B, the models are trained using a three-fold stratified cross-validation; hence, each

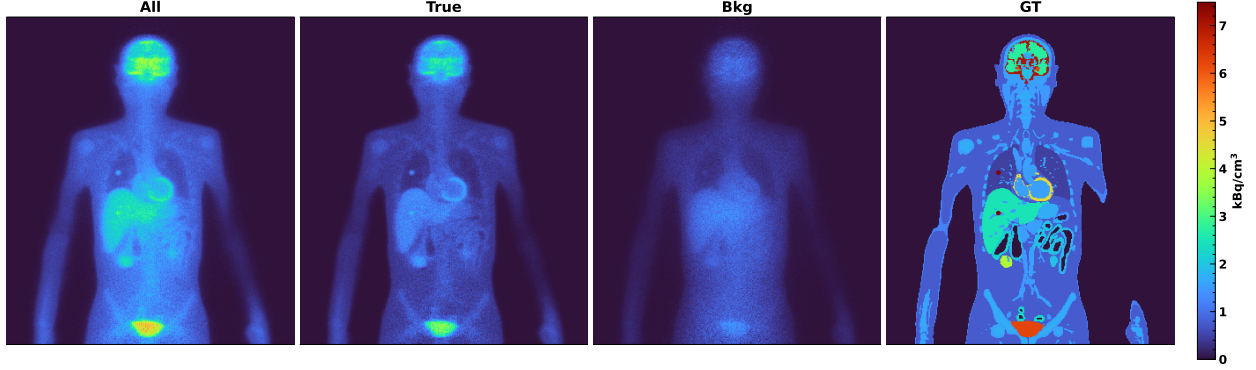

(a)

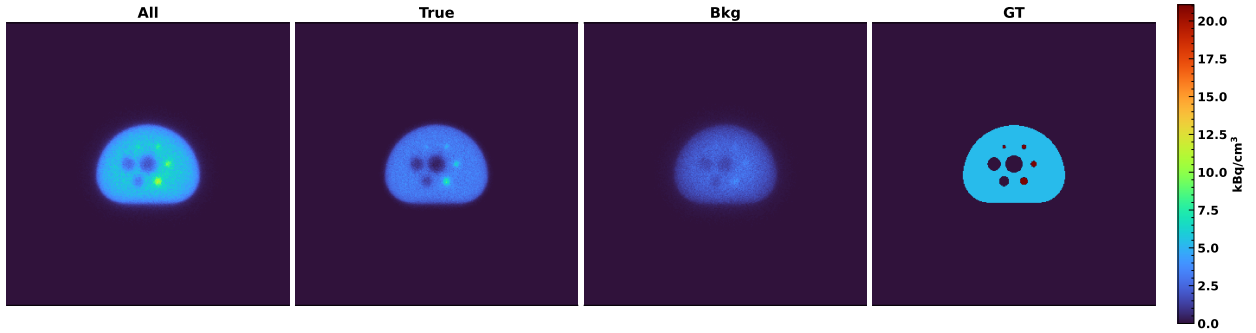

(b)

Figure 2. Reconstructed activity for *ALL*, *TRUE*, background (*PHT*, *DET* and *ACC*) coincidences as well as the Ground Truth activity map for XCAT (a) and NEMA IEC (b) phantoms.

cross-validation iteration is trained on $1.6 \cdot 10^6$ coincidences. Remaining coincidences are used for image reconstruction and generation of quality maps as described in sections II F and II H. In addition, the best model is evaluated on out-of-distribution data via cross-inference: the NEMA IEC trained model is evaluated on the XCAT data sample, and the XCAT model on the NEMA IEC dataset.

E. Data representation

We now define the output space $\mathcal{Y}$ and the input feature space $\mathcal{X}$ in terms of the physical properties of the detected coincidences.

Each event is assigned a class label from the following four categories, corresponding to the coincidence types illustrated in Fig. 3:

- genuine, undisturbed photon pairs (denoted as *TRUE*),
- photon pairs with at least one scatter in the patient's body (denoted as *PHT*),
- photon pairs with at least one additional interaction in the detector system (denoted as *DET*),
- accidental coincidences from uncorrelated annihilation events (denoted as *ACC*).

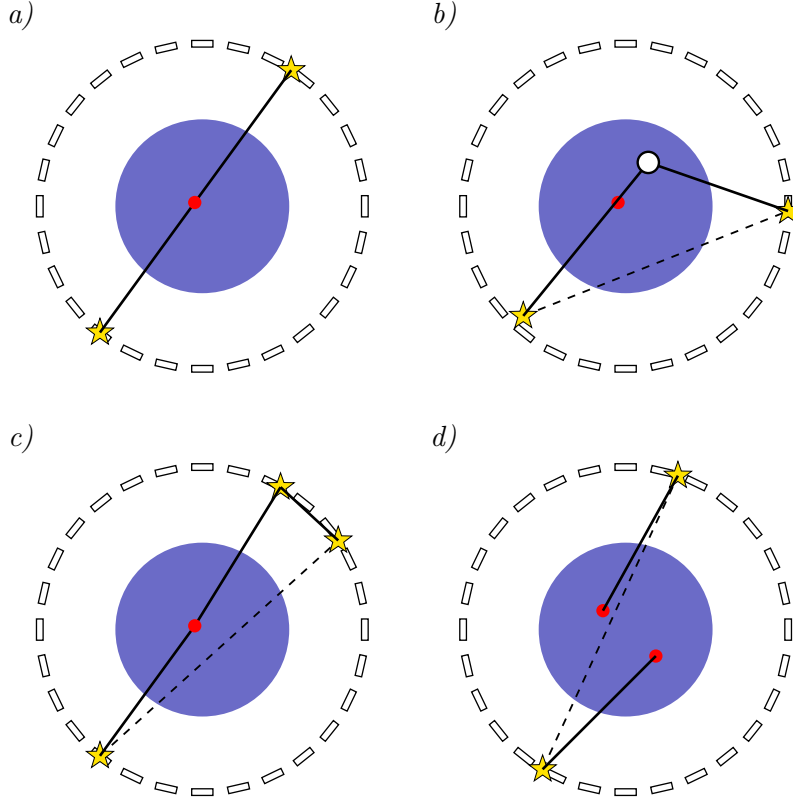


Figure 3. Classes of the coincidences $\mathcal{Y}$. The blue circle represents the patient's body, and the small rectangles positioned circularly denote the scanner. The red point is the emission vertex. The yellow stars represent the registered photon position. The dotted line represents the incorrectly reconstructed LOR. a) *TRUE*: genuine photon pair. b) *PHT*: one of the photons is scattered in the patient's body (void circle) before reaching the scanner. c) *DET*: one of the photons scatters twice in the scanner. d) *ACC*: two photons originating from different emission vertices are classified as a coincidence.

Class labels are assigned based on the MC truth information available from the simulation (see Fig. 4(a)). The decomposition of $\mathcal{Y}$ into these four classes is not unique, but it is

governed by the order of the selection rules. Because the rules are evaluated sequentially (Fig. 4), an event labelled as *ACC* may also involve a photon that scattered in the phantom or detector; had the labelling order been different, such an event would have been assigned to *PHT* or *DET* instead. Independently of the labelling order, some events within one class are indistinguishable from another class in the observable feature space – for instance, an accidental coincidence composed of two unscattered photons has the same measured characteristics as a *TRUE* event. Both types of admixtures are illustrated in Fig. 4: the dotted subsets represent events that, due to labelling priority, share characteristics with the enclosed class.

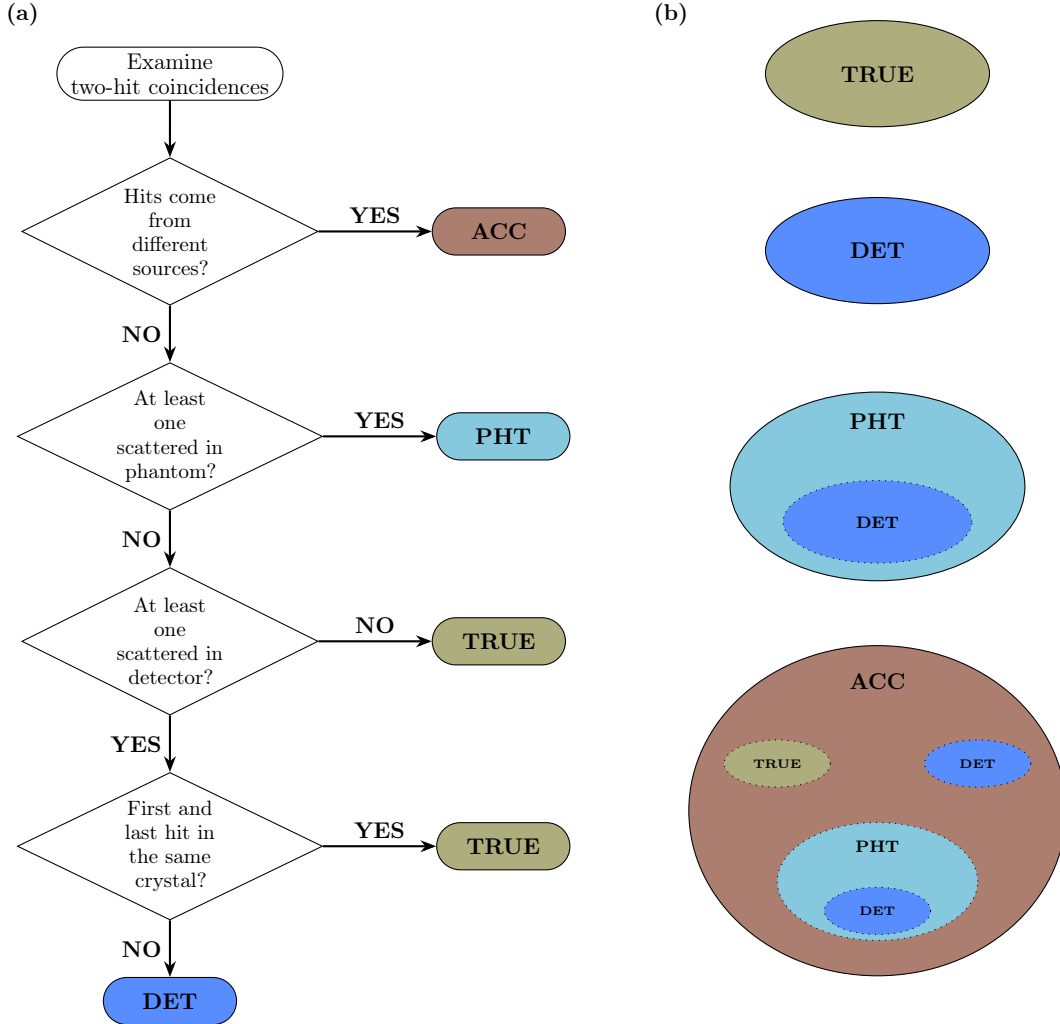


Figure 4. (a) Scheme of the algorithm assigning class labels to the coincidences based on the information from MC simulations. (b) Representation of the four main event classes together with the potential subsets of events that originate from the assumed classification hierarchy.

The resulting class distributions for both simulated phantoms are presented in Table I.

Class	NEMA IEC	XCAT
<i>TRUE</i>	46.8 %	49.0 %
<i>PHT</i>	25.2 %	24.5 %
<i>DET</i>	9.8 %	10.2 %
<i>ACC</i>	18.2 %	16.3 %

Table I. Class fractions for the NEMA IEC and XCAT simulation samples after geometry cuts.

For selected tests, we consider a 3-class scenario (3C), in which we merge the *TRUE* and *DET* classes. We observe that both classes exhibit similar photon characteristics, making it difficult for the classifier to distinguish between them.

Each *event* is described by ten scalar features corresponding to the following parameters: the reconstructed spatial positions x_1, y_1, z_1 , and x_2, y_2, z_2 , of the two registered photons, their deposited energies E_1, E_2 , and their registration times t_1, t_2 . These raw quantities are not directly suitable as classification features for two reasons. First, certain raw measurements carry no discriminating information on their own. For example, the absolute photon registration times t_1 and t_2 are meaningless without a common time reference. Moreover, coincidences are typically formed by sorting photons by time or energy, which introduces an artificial skewness in the feature distributions of the two photons. Since we always consider each coincidence as an unordered photon pair without distinguishing their identities, the constructed features should be symmetric with respect to the operation of photon swap: $x^p(1, 2) = x^p(2, 1)$, where 1 and 2 denote the first and second photon in the pair. The second important point to consider is that the distributions of the x-, y-, and z-positions of the registered hit directly encode the detector and phantom geometries; thus, this choice is not ideal for maintaining the model’s generality. We therefore construct the following set of derived features (Fig. 5), all of which satisfy the photon swap symmetry condition by construction:

- absolute time difference between the registered hits:

$$dt = |t_1 - t_2|; \tag{6}$$

- absolute value of the deposited energy difference:

$$eDiff = |E_1 - E_2|; \quad (7)$$

- sum of deposited energies:

$$eSum = E_1 + E_2; \quad (8)$$

- Attenuation Factor computed by ray-tracing through a map of linear 511 keV attenuation coefficients μ - which is normally obtained from the Computed Tomography scan

$$AF = \exp \left(- \int_0^{lorL} \mu(x) dx \right). \quad (9)$$

In addition, two topology-dependent features are defined:

- 2D opening angle with respect to the geometrical centre of the detector

$$deg2D = \arccos \left(\frac{x_1 \times x_2 + y_1 \times y_2}{\sqrt{x_1^2 + y_1^2} \times \sqrt{x_2^2 + y_2^2}} \right); \quad (10)$$

- length of the line of response spanned between two registered hits

$$lorL = \sqrt{(x_1 - x_2)^2 + (y_1 - y_2)^2 + (z_1 - z_2)^2}. \quad (11)$$

We consider two scenarios: 4-features (4F) and 6-features (6F). In the former, only the first group of previously described variables is used, and the final feature space becomes four-dimensional $\mathcal{X} \in \mathbb{R}^4$. For the latter, all six variables are considered, leading to a six-dimensional $\mathcal{X} \in \mathbb{R}^6$ feature space. Such a distinction is made to assess the impact of topological features on the model's generality. In both scenarios, the output space $\mathcal{Y}$ is defined as a categorical one with four possible outcomes $Y = [TRUE, PHT, DET, ACC]$, as defined above.

All features are preprocessed using the min-max normalisation:

$$x_i^{(p)} \rightarrow \frac{x_i^{(p)} - \min_{1 \leq j \leq N} x_j^{(p)}}{\max_{1 \leq j \leq N} x_j^{(p)} - \min_{1 \leq j \leq N} x_j^{(p)}}, \quad i \in [1, \dots, N], p \in [1, \dots, P] \quad (12)$$

The minimum and the maximum values for each (p) of P features are computed over the training sample containing N events. The normalisation parameters are determined during the training procedure and subsequently reused for validation and inference.

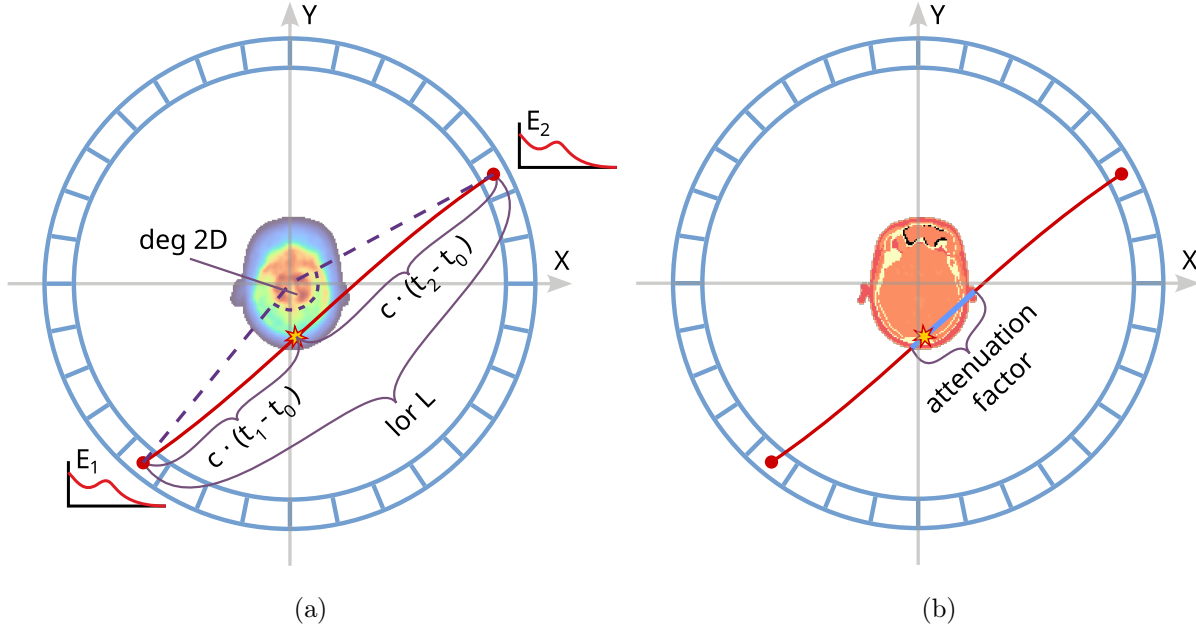


Figure 5. Graphical representation of observables used to create the final feature set. Panel (a) presents the *deg2D* opening angle, *lorL*, photon detection t_1 , t_2 and emission t_0 times together with photon deposited energies E_1 and E_2 . Panel (b) presents the way the attenuation factor is extracted for a given coincidence.

F. PET image reconstruction

A direct TOF positioning algorithm is used for image reconstruction. Each coincidence defines a LOR from two photon detection points. Based on the time difference dt between the photon registrations, the most likely annihilation position is estimated along the LOR and the event is deposited into the corresponding voxel of a 3D grid with 2.5 mm isotropic spacing ($424 \times 280 \times 280$ voxels). The intensity in each voxel is thus defined by the number of coincidences whose estimated emission point falls within that voxel volume.

The reconstructed image is corrected for attenuation and detector sensitivity using a combined attenuation-sensitivity map derived using the CASToR [Merlin et al. \(2018\)](#) reconstruction package from a dedicated GATE simulation. The corrected image is then normalised to the assumed phantom activity.

This reconstruction approach is chosen deliberately for two reasons. First, it is parameter-free, unlike iterative algorithms such as Maximum-Likelihood Expectation-Maximization, it introduces no tunable hyperparameters that could interact with or obscure the classifier's effect

on image quality. Second, and crucially for the present study, the direct TOF positioning preserves an explicit one-to-one correspondence between each coincidence event and its deposited voxel. This property allows mapping the spatial distribution of classifier metrics, such as accuracy, TPR, and PPV, directly onto the reconstructed image volume, as described in section III H. In contrast, iterative algorithms redistribute event contributions across the image through repeated forward and backwards projection steps, which would destroy event-to-event traceability and introduce additional systematic effects into the spatial quality maps.

The reconstructed images for both phantoms are presented in Fig. 2, showing separate reconstructions for *ALL*, *TRUE*, and background (*PHT*, *DET* and *ACC*) coincidence classes, with class association based on the true label of each event from the MC simulation.

G. Evaluation metrics

We evaluated the performance of the classifiers based on several metrics commonly used in ML, expressing the dependence between the genuine, positive (P) and spurious, false (F) classification:

True Positive Rate (sensitivity) ¹

$$TPR = \frac{TP}{TP + FN}; \quad (13)$$

Positive Predictive Value (precision):

$$PPV = \frac{TP}{TP + FP}; \quad (14)$$

accuracy

$$accuracy = \frac{TP + TN}{TP + TN + FP + FN}; \quad (15)$$

F1 Score

$$F1 = \frac{2TP}{2TP + FP + FN}; \quad (16)$$

Matthews correlation coefficient (MCC)

$$MCC = \frac{TP \cdot TN - FP \cdot FN}{\sqrt{(TP + FP)(TP + FN)(TN + FP)(TN + FN)}}; \quad (17)$$

¹ There are several names for the same metric depending on the scientific community. The True Positive Rate is also known as sensitivity, recall or efficiency, while the Positive Predictive Value is known as purity, or precision.

with T and F denoting, respectively, true and false classification into P and N classes.

As the model performance is not uniform between coincidence classes, we defined a confusion matrix for each model. A visual representation of model prediction correctness, with rows corresponding to true event class and columns to model predictions, while matrix elements are a count of events for a given pair of true and predicted label (section III B).

We verify two modes of true event selection based on the model response. For the *threshold* mode, we select an optimal working point by considering the TPR as a function of PPV – the receiver operating characteristic curve. As a reference point, we selected the model response threshold corresponding to a TPR (sensitivity) of 95% and treated all events that passed this threshold as the *TRUE* class. When the model performance was evaluated on a different dataset, both the data normalisation and the classifier working points were kept as defined during training to simulate application to real-world data, where selection of a new working point is not possible. For the *top-1* mode, the model response is the class with the largest model-assigned probability for a given event. Based on this, we select the events with the *TRUE* class being the top-1.

In addition, the Mean Squared Error (MSE) metric was used. The MSE between two images I_1 and I_2 is defined as:

$$MSE[I_1, I_2] = \frac{1}{N} \sum_{k=1}^N (I_1[k] - I_2[k])^2, \quad (18)$$

where N is the total number of voxels.

In our studies, the ToF-reconstructed, *TRUE* class image is used as a ground-truth reference, while the predicted image is a ToF reconstruction of ML-selected coincidences. Both the reference and ML-predicted images are first corrected using a combined scanner sensitivity and attenuation map and normalised to the simulated activity. Then, a median filter with kernel 2^3 is applied to both images. The MSE calculation is restricted to voxels within the phantom volume by a mask derived from the attenuation map.

H. Spatial quality maps

The model performance can vary spatially depending on the local environment of the emission point, e.g. activity, tissue type, tissue density, and position within the scanner Field of View (FOV). Commonly used global metrics, such as accuracy or MCC, fail to

capture localised degradations of model performance, while such spatial non-uniformity can be detrimental for medical diagnosis. We therefore propose complementing global metrics with 3D spatial maps to identify degraded regions. First, we divide all coincidences into TP, FP, TN, and FN subgroups based on the model’s response. Although both binary and multi-class definitions of this division are applicable, we adopt a binary distinction between the signal and the background for two reasons. First and foremost, the determination of the *TRUE* class is the ultimate goal of the classification. Second, the binary formulation allows direct comparison between two proposed classification modes: *top-1* and *threshold*.

Each coincidence subgroup is then reconstructed independently as described in section II F, providing a per-voxel estimate of TP, FP, TN and FN. Correction for attenuation and sensitivity is not required, as it cancels out when calculating the metrics defined in section II G. Finally, by calculating in each voxel three metrics: accuracy, TPR and PPV, we obtain 3D maps of model quality metrics. Resulting maps for the XGBoost model are presented in Fig. 15 and 14.

I. Feature analysis

To gain insight into the final model’s characteristics, it is useful to determine the feature importance metric, a relative measure of the feature’s usefulness for the classification task. Two approaches were considered: one for the BDT classifiers, where such metrics are naturally available, and the permutation feature importance for all considered models. In the case of the XGBoost, the feature importance is commonly an average *gain* (Eq. 4) across all leaves and all trees in the ensemble where the feature was used. For the AdaBoost, the *gini importance* is defined as the sum of node impurity decrease weighted by the fraction of samples reaching the node averaged over all trees in the ensemble. The impurity decrease (Eq. 5) is the difference between a node’s impurity and the Gini index - a weighted sum of the impurity measures of the two child nodes.

No such intrinsic metric exists for artificial neural networks; therefore, a good solution, albeit computationally intensive, is to determine the permutation feature importance Breiman (2001). It is defined as a reduction of a model score when applied to data in which one feature is randomly shuffled. By removing the relationship between the feature and the target, the model’s performance will reflect how crucial the feature’s information is.

III. RESULTS

A. Feature analysis

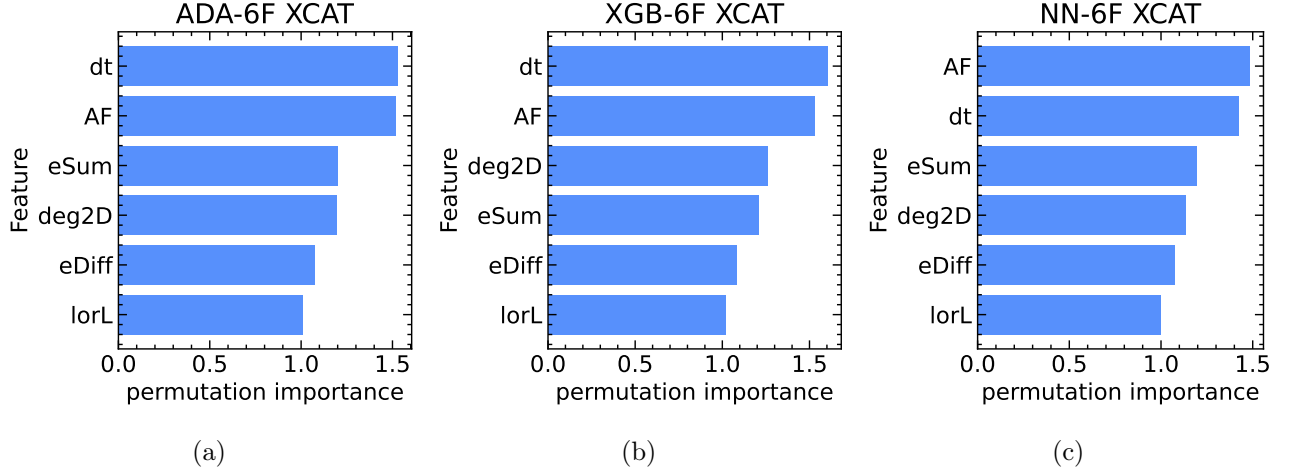


Figure 6. Permutation feature importance for the three considered models for the XCAT sample.

We present the permutation importance of the six features for the three considered model classes, obtained for the XCAT dataset. The two features with the highest score for all three models are *dt* and *AF*, as presented in Fig. 6. The first two features have similar importance values and form a distinct group, with *eSum* and *deg2D* features forming a second one. We observe that the ordering within closely valued groups is model-dependent.

Full results of the feature importance analysis are presented in Appendix B. We observe that for the NEMA IEC dataset, the *deg2D* gains importance over *AF* due to the simplified geometry. It is worth noting that, unlike permutation importance, the XGBoost gain metric identifies *eSum* as the most important feature across both datasets. While essentially free to compute, the XGBoost gain includes the regularisation terms, which are harder to interpret; therefore, a model-agnostic metric such as permutation importance is preferable.

B. Models performance

We present results of the coincidence classification for two datasets: NEMA IEC and XCAT. For each dataset, a total of six model configurations are considered. First, we evaluate the three model types trained on the full six-feature set: XGBoost (XGB-6F),

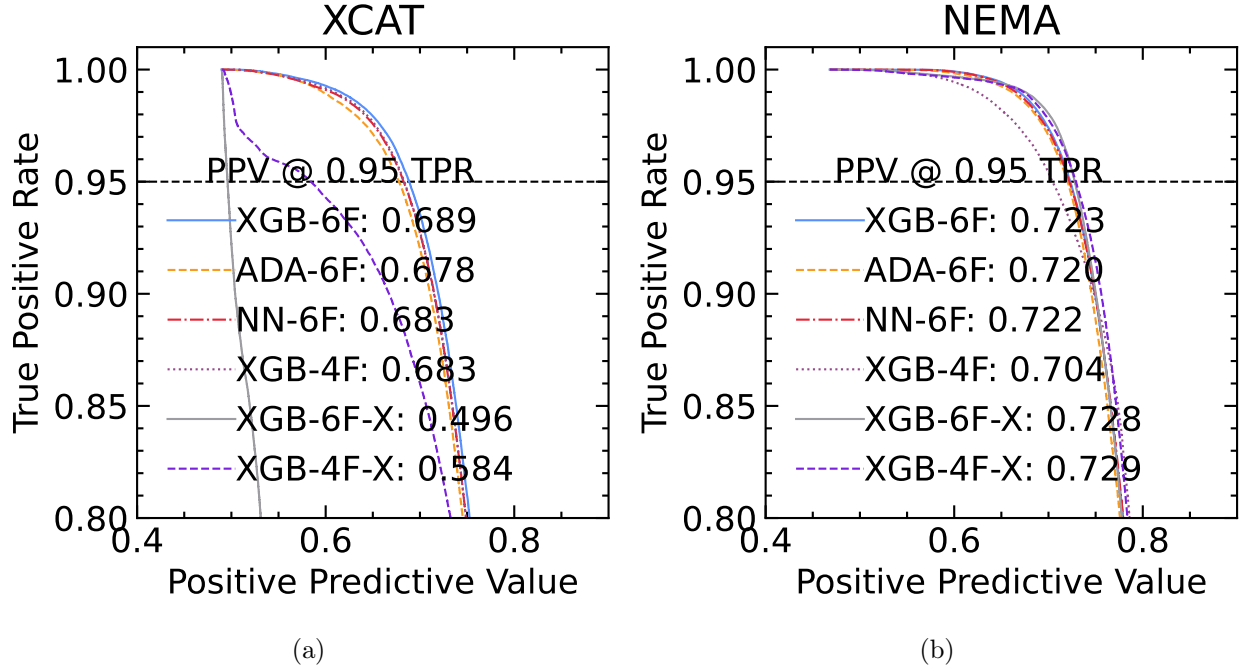


Figure 7. TPR as a function of PPV for all considered model configurations, evaluated on the XCAT (a) and NEMA IEC (b) samples.

AdaBoost (ADA-6F) and MLP (NN-6F). For the best architecture (XGBoost), we provide three additional tests: a variant trained on the four geometry-agnostic features (XGB-4F) and two cross-inference results in which the model is evaluated on an out-of-distribution dataset (XGB-6F-X and XGB-4F-X).

The performance metrics for the best variants of each architecture are provided in Table II. In addition, we present the fraction of *TRUE* coincidences for the baseline geometric cut, together with the model binary accuracy, for direct comparison.

The TPR dependence on PPV for all configurations is presented in Fig. 7, with numeric PPV values for binary classification with a model response threshold set to obtain a TPR equal to 0.95. As described in section II G, it is the working point of the *threshold* selection mode. A clear degradation in performance is observed for the NEMA IEC trained model when evaluated on out-of-distribution data. In Fig. 8, the receiver operating characteristic curve is presented for the considered configurations together with quoted values of the associated Area Under Curve (AUC) metric.

For the best architecture (XGBoost), we present in Figs. 9 and 10 confusion matrices evaluated on the test subsamples for the two datasets: NEMA IEC and XCAT. In addition,

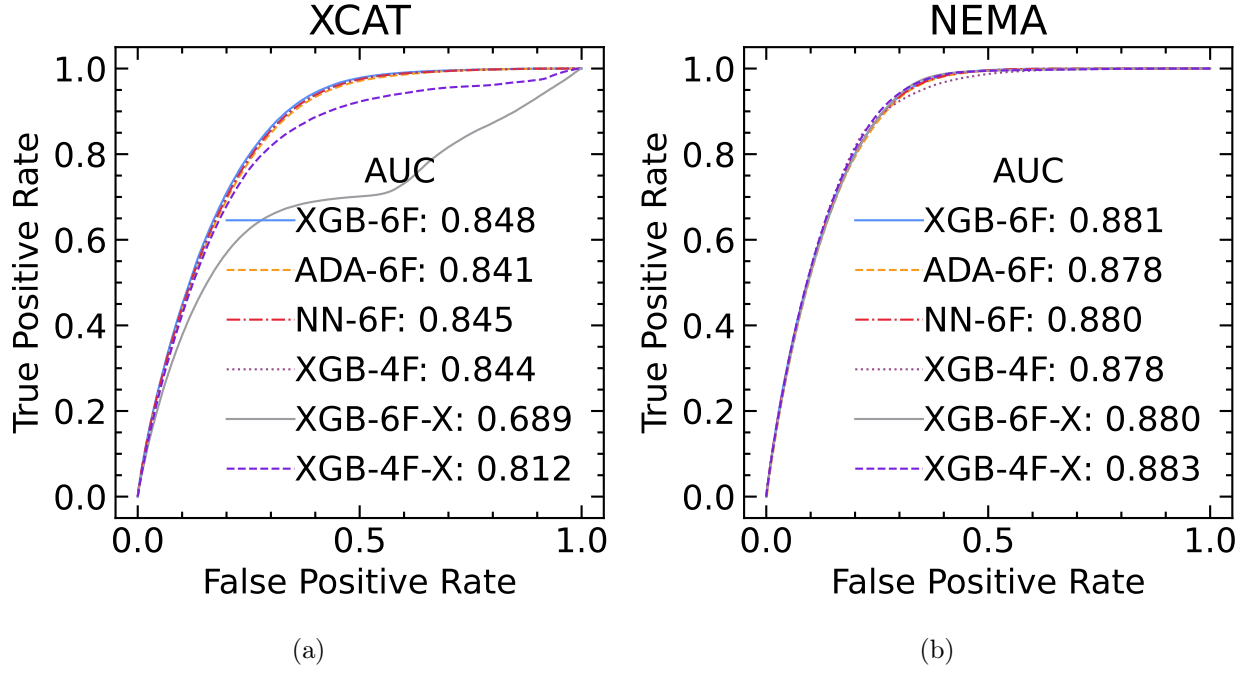


Figure 8. receiver operating characteristic curves for all considered model configurations, evaluated on the XCAT (a) and NEMA IEC (b) samples.

	NEMA IEC			XCAT		
	XGB	ADA	MLP	XGB	ADA	MLP
Baseline	0.468			0.490		
Binary Accuracy	0.806	0.804	0.806	0.765	0.754	0.760
Multi-class Accuracy	0.738	0.737	0.734	0.691	0.689	0.685
MCC	0.60	0.60	0.60	0.51	0.51	0.50
F1	0.71	0.71	0.70	0.66	0.65	0.65

Table II. Performance metrics for the best variant - 6-features and 4 classes - of each architecture: XGBoost, AdaBoost and MLP. The three left columns correspond to the NEMA IEC phantom while the three right columns correspond to the XCAT one. The baseline corresponds to the fraction of *TRUE* coincidences after applying the geometry cuts; binary accuracy is computed by treating all classes besides the *TRUE* as background. Multi-class accuracy, MCC and F1 metrics are described in the section II G.

the values of the multi-class Accuracy, PPV, and TPR metrics are quoted. It's evident that among the studied configurations, models struggle most to correctly classify the *DET* class.

This is not unexpected, as in events where the photon after Compton scattering deposits energy in a neighbouring crystal, the features are hardly perturbed compared to the *TRUE* class. On the other hand, such coincidences do not introduce large image smearing. Another class for which models struggle is the *PHT* class, where a substantial part of the coincidences is wrongly classified as *TRUE*.

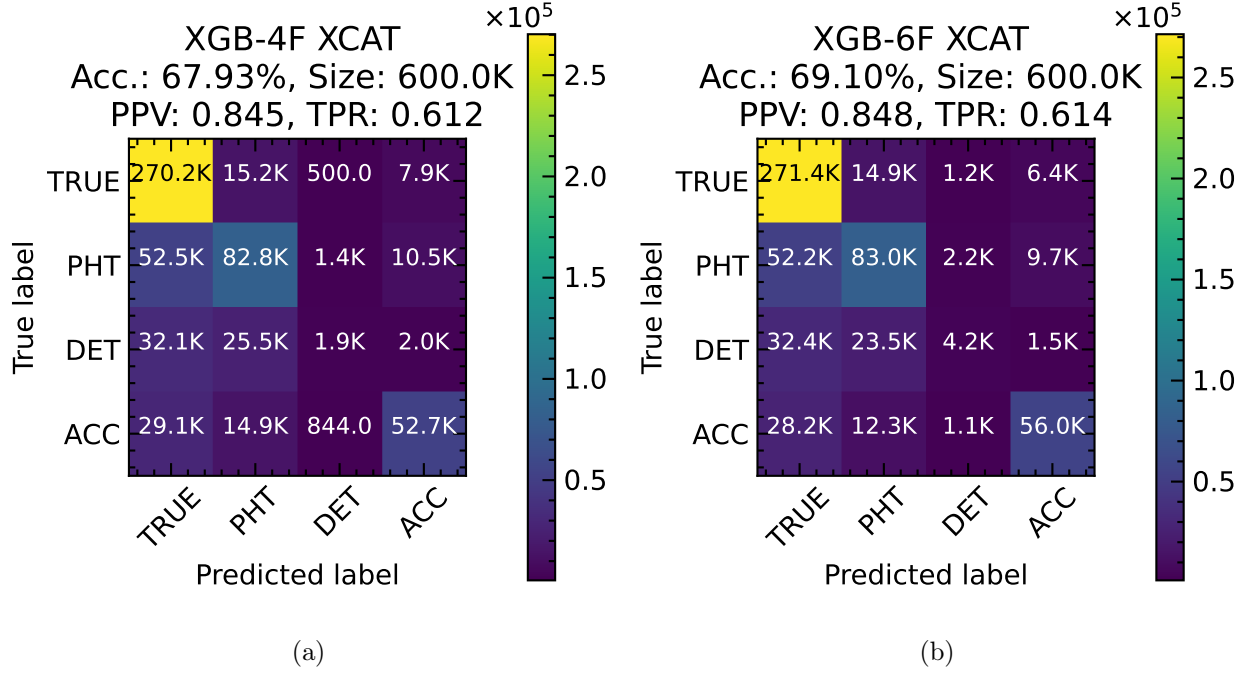


Figure 9. Confusion matrices for the best XGBoost models for the XCAT sample are presented. The left column (a) corresponds to a model trained with 4 features, while the right column (b) presents results for a 6-feature model variant.

A visual representation of the image quality for the best model on the XCAT sample is presented in Fig. 11. The XGB-6F selected coincidences were reconstructed with corrections for the scanner sensitivity and attenuation as described in section II F. The image is compared to the reconstruction of the *TRUE* class coincidences. A clear improvement is seen compared to the uncorrected image.

C. Robustness test of the models

In the proposed method, models are trained on a single phantom. This raises a question about the generality of the resulting models, particularly with respect to phantom geometry.

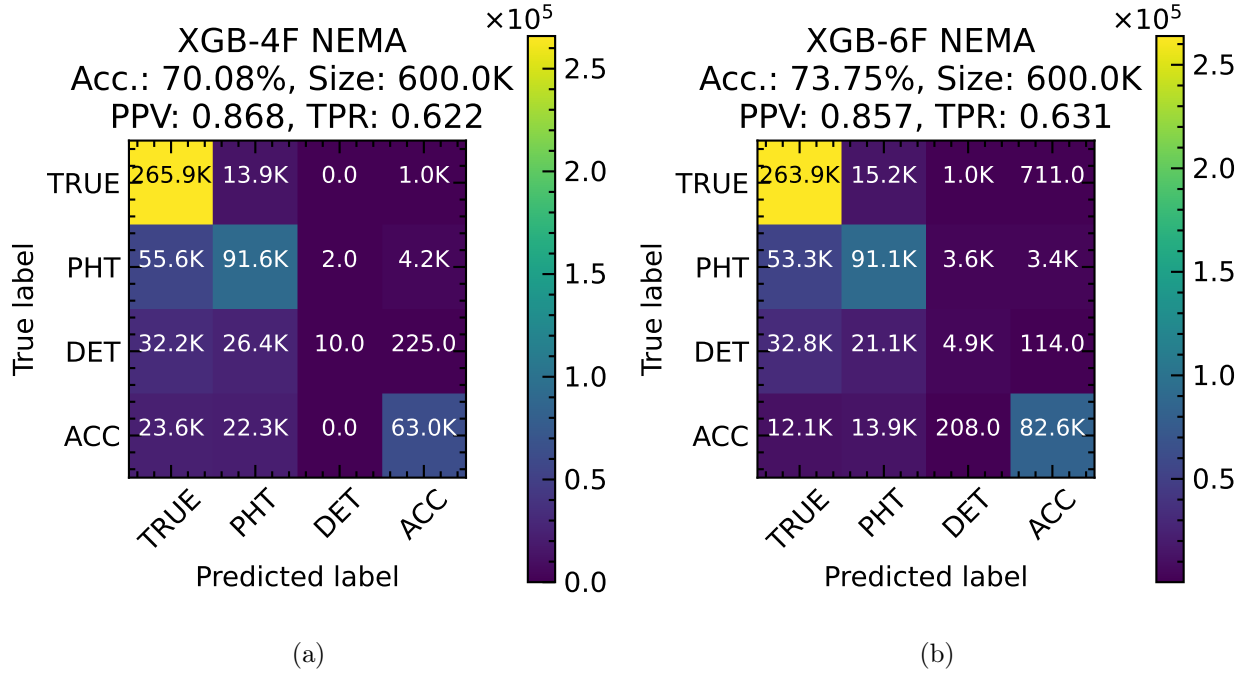


Figure 10. Confusion matrices for the best XGBoost models for the NEMA IEC sample are presented. The left column (a) corresponds to a model trained with 4 features, while the right column (b) presents results for a 6-feature model variant.

To verify this, we devised a cross-inference test where a model trained on one phantom is evaluated on a dataset from another phantom. For this work, models trained on the NEMA IEC phantom were evaluated on the XCAT sample and models trained on the XCAT were evaluated using the NEMA IEC phantom. The XCAT phantom is not only more than 7 times longer than NEMA IEC, but its geometry is also much more complex. Therefore, with this test, we can evaluate both the impact of the phantom’s position within the scanner and of different phantom shapes or orientations.

We observe that 6-feature models exhibit worse generalisation performance than the 4-feature case, where topological features are not considered. For example, the XGBoost model trained on the NEMA IEC data sample and evaluated on the XCAT data sample achieved accuracies of 0.561 for the 6-feature variant and 0.647 for the 4-feature one. Comparing this result to the performance of models trained on the XCAT sample, we observe a loss of accuracy of 0.130 and 0.044 for the 6- and 4-feature variants, respectively. The accuracy gap of the 4-feature XGBoost model to the 6-feature one, trained on the NEMA IEC sample, when evaluated on the same phantom is 0.037. This shows that it exhibits good generalisability

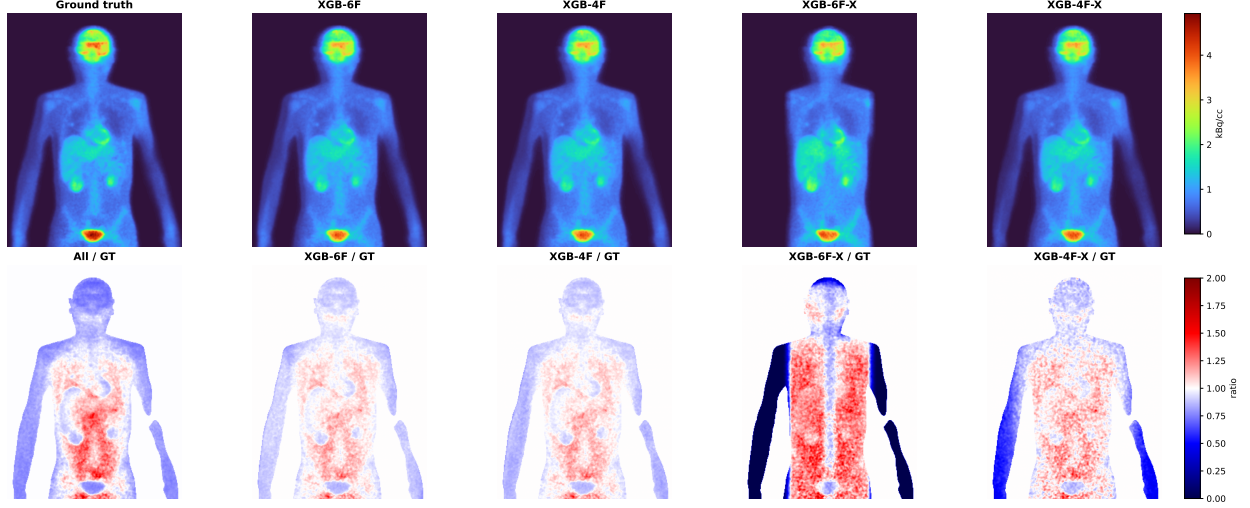


Figure 11. Top row: sagittal slices of activity normalized reconstructed XCAT images for *TRUE* coincidences (ground truth) and XGBoost selected coincidences in four variants: two trained on the XCAT sample with six (XGB-6F) and four features (XGB-4F), and two trained on the NEMA IEC sample also with six (XGB-6F-X) and four (XGB-4F-X) features. Bottom row: per-voxel ratio maps masked to the phantom volume - GT/All shows the *TRUE* class fraction, other columns follow the same convention as the top row and present the ratio of classifier-selected coincidences to *TRUE* ones.

as its performance profile is stable independent of the data sample. More interestingly, the performance gap narrows for models trained on the XCAT data sample to only 0.012; for a phantom with more diverse geometry, the topological features do not allow for simple yet robust geometry cuts. Once again, the gap is stable when considering cross-inference on the NEMA IEC phantom.

The results of the robustness test are summarised in Table III and in Fig. 12. Evaluating classifier performance with a multi-class version of the accuracy metric allows for an insight into how well it discerns between the background classes in addition to the *TRUE* one. Based on the obtained confusion matrices, the 4-feature variants do not discern as well as the 6-feature ones between *PHT* and *DET* classes.

sample	metric	XGBoost model variant			
		4F NEMA	4F XCAT	6F NEMA	6F XCAT
XCAT	accuracy	0.647 (-0.044)	<u>0.679</u> (-0.012)	0.561 (-0.130)	0.691 (0.0)
	F1	0.60 (-0.05)	<u>0.64</u> (-0.01)	0.54 (-0.11)	0.65 (0.0)
	MCC	0.44 (-0.07)	<u>0.49</u> (-0.02)	0.36 (-0.15)	0.51 (0.0)
NEMA IEC	accuracy	0.701 (-0.037)	0.720 (-0.018)	0.738 (0.0)	<u>0.728</u> (-0.010)
	F1	0.66 (-0.05)	0.68 (-0.03)	0.71 (0.0)	<u>0.69</u> (-0.02)
	MCC	0.54 (-0.06)	0.57 (-0.03)	0.60 (0.0)	<u>0.58</u> (-0.02)

Table III. Results of the robustness tests for XGBoost models. The first column identifies the evaluation data sample. The columns correspond to results for four models: 4F NEMA - a model trained on NEMA IEC data sample with 4-features, 4F XCAT - a model trained on XCAT data sample with 4-features, 6F NEMA - a model trained on NEMA IEC data sample with 6-features and 6F XCAT - a model trained on XCAT data sample with 6-features. The quoted values correspond to the accuracy, F1 and MCC metrics defined for multi-class classification. In parentheses, the metric reduction relative to the best result for the given data sample is provided. Best results are provided in bold while the second best are underlined.


D. Spatial quality maps

First, we evaluate the impact of the classification mode on the uniformity of the model’s response. In Fig. 13 a comparison of accuracy and TPR maps is presented for the *threshold* and the *top-1* modes, for the XGBoost model trained on the XCAT sample. The *top-1* selection leads to more uniform model response, especially for the case where we restrict the classification problem to three classes by merging *DET* with *TRUE*, as the feature distributions of those classes largely overlap.


We compare the impact of feature set selection and out-of-distribution evaluation on the XGBoost model response. First, the performance on the NEMA IEC sample is assessed

for four model variants (Fig. 14): two trained on the NEMA IEC sample with 6 features (XGB-6F) and four features (XGB-4F); two trained on the XCAT sample also with 6 features (XGB-6F-X) and 4 features (XGB-4F-X). We observe that the model trained on the NEMA IEC with 6 features uses the *deg2D* feature for a hard cylindrical rejection cut that tightly encompasses the phantom geometry. Another effect is visible around the lung insert: the model once again uses the *deg2D* feature for positional classification of the coincidences in this region, while it improves the accuracy and PPV metrics, a clear degradation in TPR is observed. The variant trained on the XCAT sample does not use such a hard threshold; nevertheless, the cylindrical shape with increased PPV metric is visible. Models trained on XCAT data exhibit lower accuracy and TPR metrics, when evaluated on the NEMA IEC data, on the phantom extremes along the horizontal axis. We hypothesise that this is an effect of the XCAT shape in which the only region that is close to the scanner main axis with unobstructed horizontal view is the phantom head. For the torso, the LORs originating from a similar region have an increased probability of crossing the phantom arms. This is not the case for the head; however, the horizontal extent of the XCAT phantom in this region is smaller than for the NEMA IEC phantom and coincides with the region of high accuracy in the cross-inference spatial quality map.


Next, in the same way, we evaluate the XGBoost model response uniformity on the XCAT sample (Fig. 15). First, we do not observe significant differences between the XGB-6F and the XGB-4F variants trained on the evaluated sample. The spatial diversity of the phantom prevents the model trained on a richer feature set from utilising simple geometrical shortcuts. On the other hand, the observed hard cuts for the 6-feature variant trained on the NEMA IEC sample (XGB-6F-X) are clearly visible. The effect is largely diminished in the four-feature variant (XGB-4F-X), with only the phantom’s hands affected. This is most likely an effect of the *dt* feature, which, while highly effective at rejecting the *ACC* coincidences, does encode the distance from the scanner main axis.

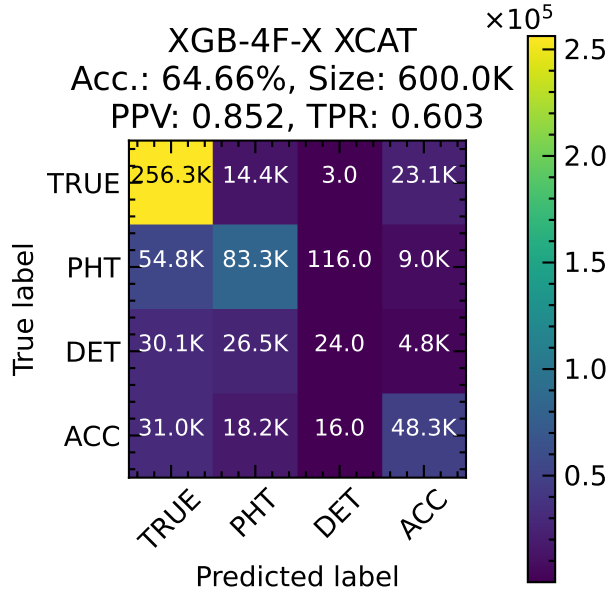


(a)

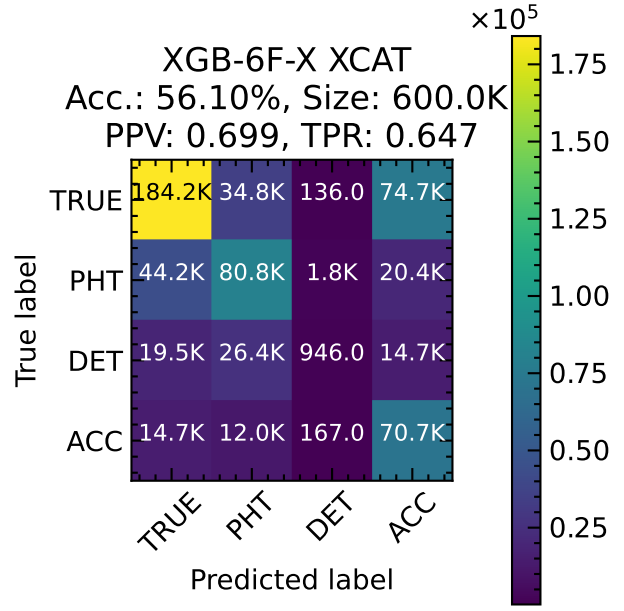

(b)

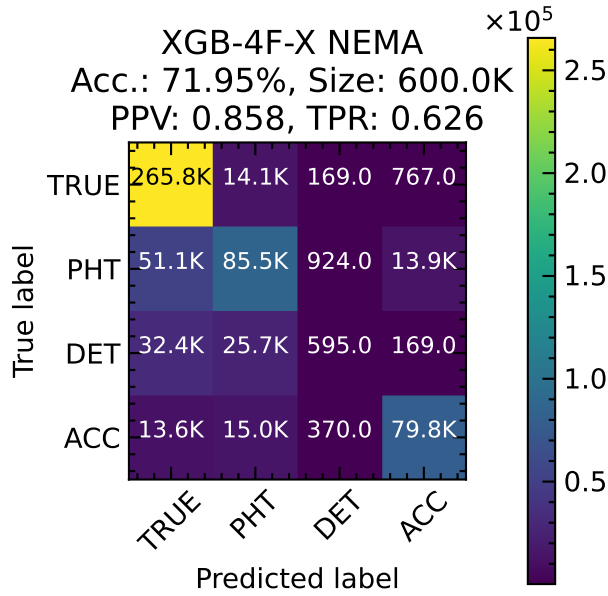


(c)

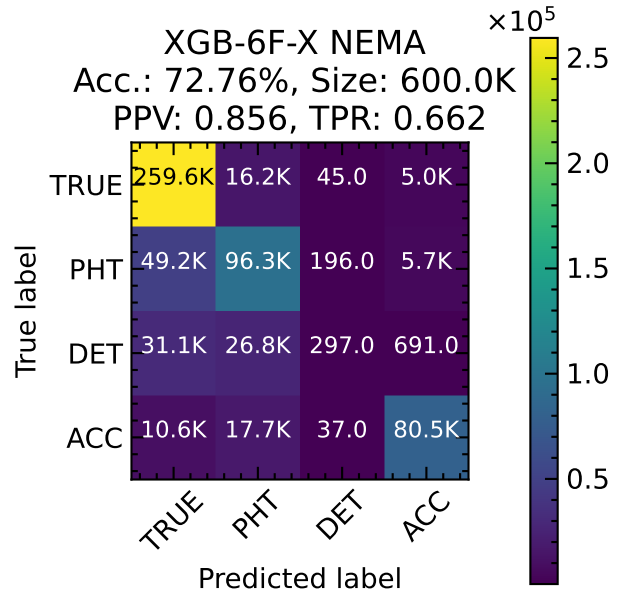


(d)

Figure 12. Confusion matrices for the robustness test. Results for XGBoost models are presented. In the first row (figures a) and b)) models trained on the NEMA IEC sample are evaluated on XCAT sample. For the bottom row (figures c) and d)) models trained on XCAT sample are evaluated on the NEMA IEC sample. The left column (figures a) and c)) corresponds to models trained with 4-features while the right column (figures b) and d)) presents results for 6-feature model variants.

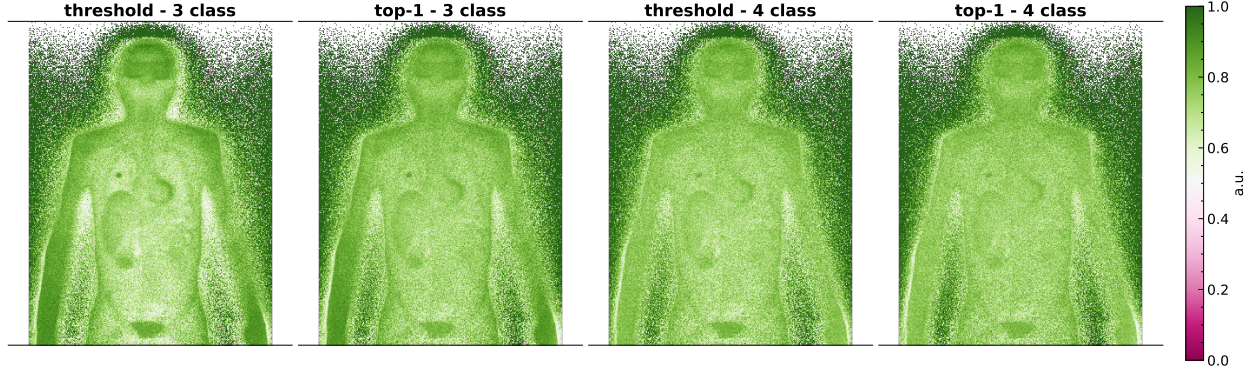


(a)

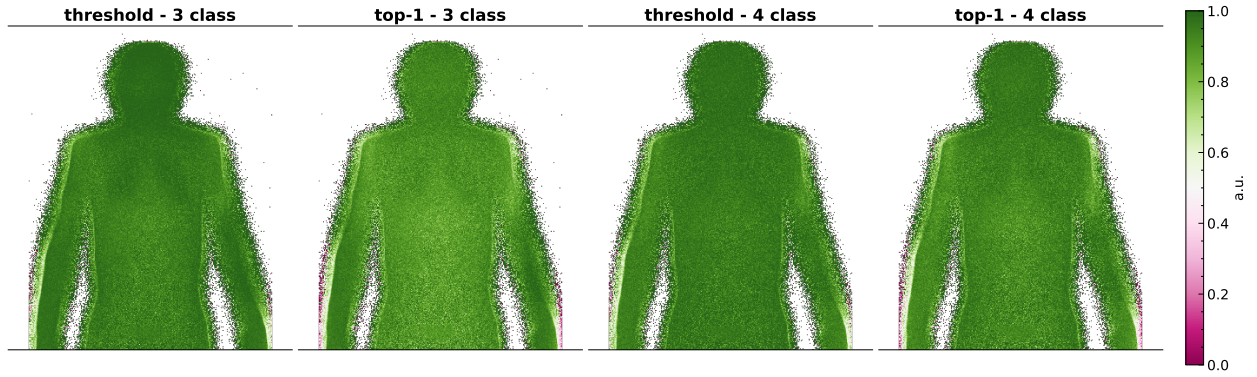


(b)


Figure 13. Comparison of spatial distribution of the Accuracy (a) and TPR (b) metrics between *top-1* and *threshold*-based selection. Two XGB models are considered: XGB-3C-6F - an XGB model trained to classify data into 3 classes based on 6 features, and XGB-6F - an XGB model trained to classify data into 4 classes based on 6 features.

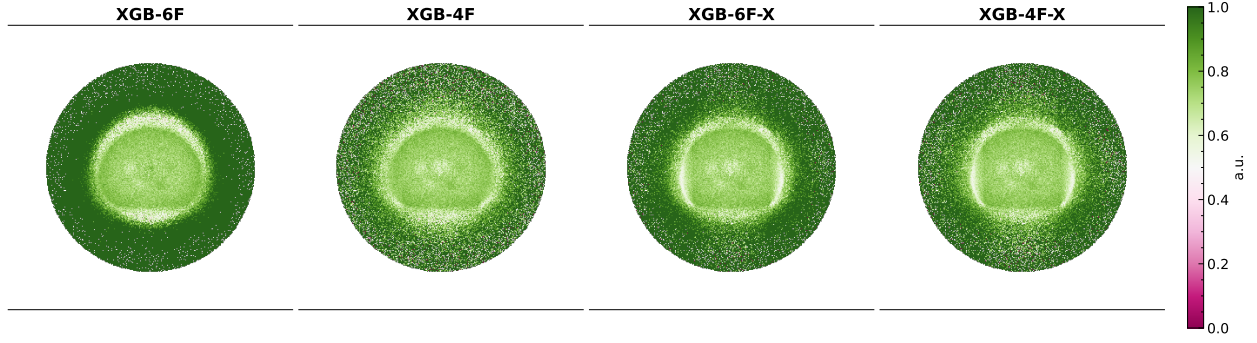

(a)

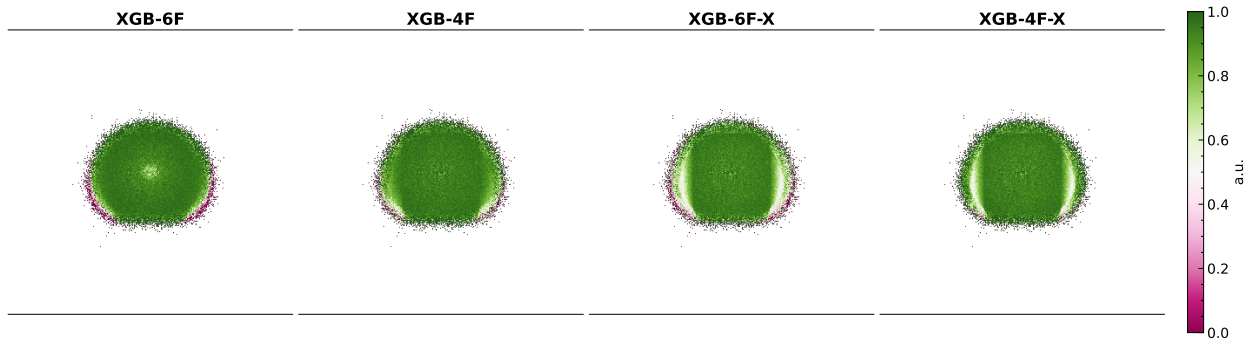


(b)

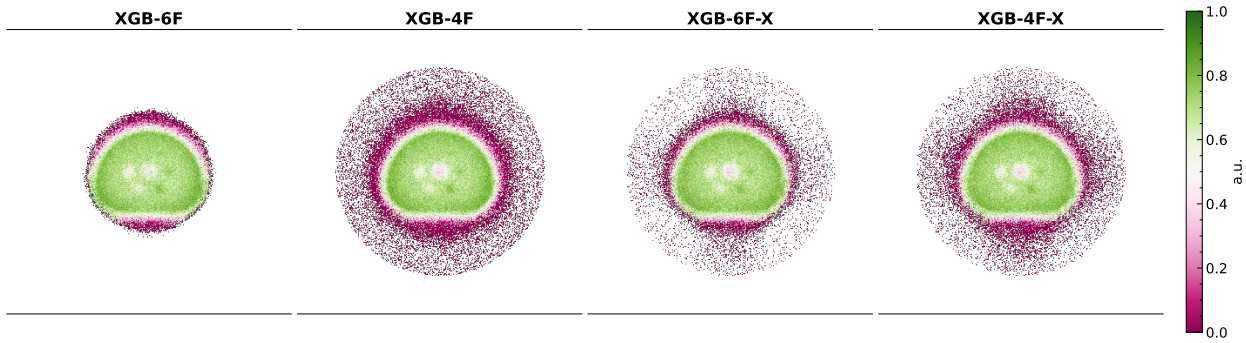


(c)


Figure 14. Comparison of spatial distribution of the Accuracy (a), TPR (b) and PPV (c) metrics for the NEMA IEC phantom, between 4 XGB models: XGB-6F - a model trained on 6 features and NEMA IEC data; XGB-4F - a model trained on 4 features and NEMA IEC data; XGB-6F-X - a model trained on 6 features and XCAT data; XGB-4F-X - a model trained on 4 features and XCAT data.

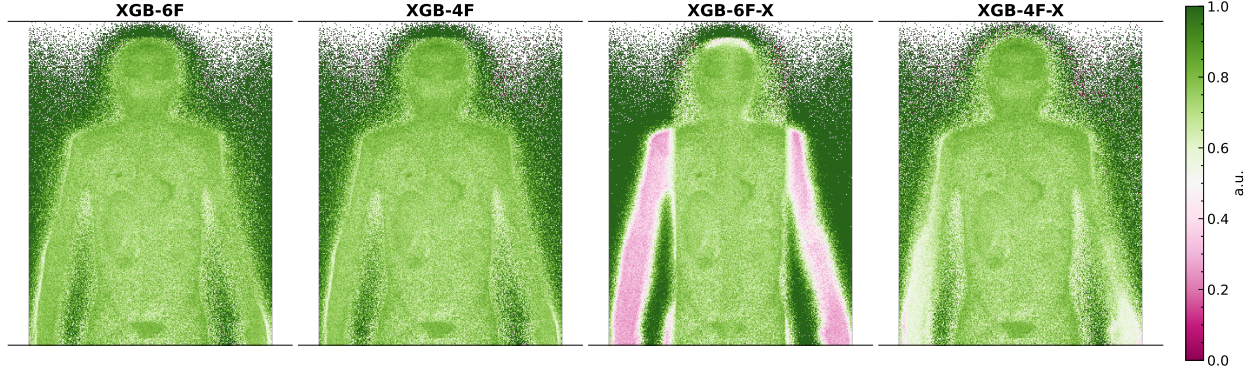

(a)

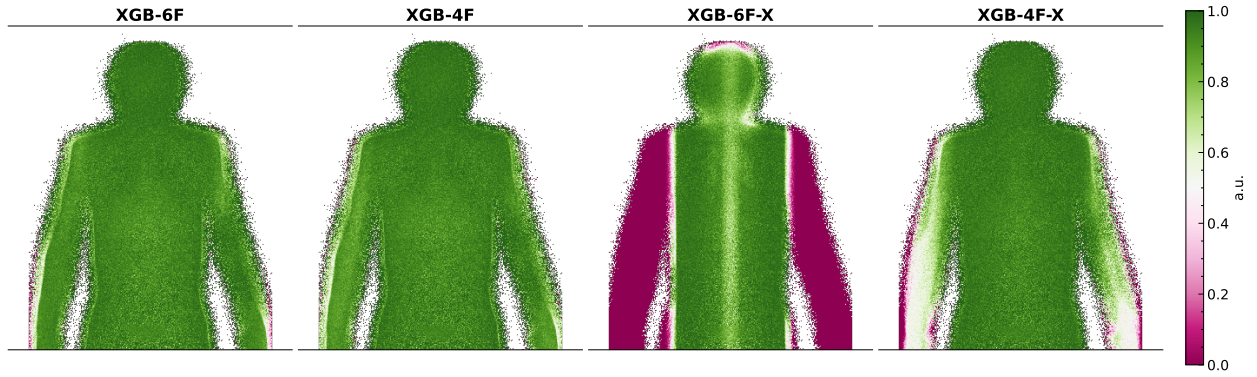

(b)

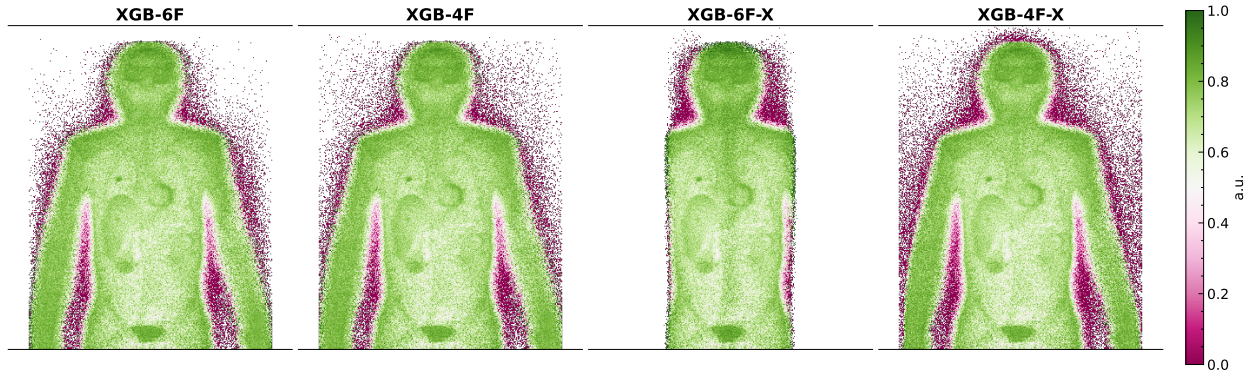

(c)

Figure 15. Comparison of spatial distribution of the Accuracy (a), TPR (b) and PPV (c) metrics for the XCAT phantom, between 4 XGB models: XGB-6F - a model trained on 6 features and XCAT data; XGB-4F - a model trained on 4 features and XCAT data; XGB-6F-X - a model trained on 6 features and NEMA IEC data; XGB-4F-X - a model trained on 4 features and NEMA IEC data.

IV. DISCUSSION

A. Feature importance interpretation

The permutation importance analysis shows that the photon time difference dt and the attenuation factor AF are the two most discriminating features across all model architectures and simulated phantom setups. This can be clearly interpreted in the context of the properties of background classes. Accidental coincidences are formed, by definition, from uncorrelated annihilation events, and the time difference between the two detected photons is therefore uncorrelated with the scanner geometry. This results in a broader dt distribution for accidental pairs than for true coincidences, where the time difference is constrained by the finite size of the emission region and the scanner time resolution. Therefore, this feature provides direct, geometry-independent discrimination against the *ACC* class. The energy-based features carry limited discriminative power for the *ACC* class by construction; e.g. accidental pairs are not expected to differ systematically from the true coincidences in their deposited energy distributions, as both consist of unscattered 511 keV photons in the first approximation. The attenuation factor encodes the total material traversed along the LOR. For phantom-scattered photons, the LOR is deflected; therefore, one can expect that the reconstructed line will, in general, traverse a different amount of attenuating material than a true coincidence originating from the same region. This makes the AF feature sensitive to the *PHT* class. Its advantage over the energy-based features $eSum$ and $eDiff$ suggests that spatial mislocation is a more reliable signature than energy deposition in the considered scenarios.

The relative importance of the secondary features, namely $eSum$ and $deg2D$, shows a dataset-dependent behaviour. For the NEMA IEC phantom, $deg2D$ gains importance relative to AF . We interpret it as the simplified, approximately cylindrical geometry of that phantom. The opening angle provides a way to encode the geometric cut separating in-phantom from out-of-phantom LORs. This behaviour is consistent with the spatial quality maps discussed in Section III D, where the 6-feature model trained on NEMA IEC phantom applies a hard cylindrical selection driven by $deg2D$. Therefore, it can be interpreted as a kind of geometry memorisation that directly explains the degraded cross-phantom generalisation of the 6-feature model discussed in Section III C.

B. Robustness and generalization

The cross-phantom results clearly show that model generalisation depends on the choice of feature set. The 6-feature variant, which incorporates the topology-dependent variables $deg2D$ and $lorL$, suffers a substantially larger loss in accuracy when evaluated on out-of-distribution data than the 4-feature variant. For the XGBoost model trained on NEMA IEC and evaluated on the geometrically more complex XCAT phantom, the accuracy loss amounts to -0.130 for the 6-feature variant, compared to -0.044 for the 4-feature one. This difference is physically expected: $deg2D$ and $lorL$ encode properties of the LOR that are sensitive to the phantom shape and the position within the scanner FOV. A model trained on a centrally positioned NEMA IEC phantom will learn decision boundaries in the topological feature space directly connected to the geometry. Therefore, their application to another anatomically complex phantom, such as XCAT, becomes inappropriate. This observation is confirmed by the spatial quality maps obtained. The 6-feature model trained on the NEMA IEC dataset and evaluated on XCAT introduces a hard cylindrical cut that removes a large portion of the XCAT phantom, as discussed in section III D. On the other hand, the 4-feature variant does not exhibit this sharp cut, and spatial degradation is greatly reduced. We attribute it to the removal of topology variables from the feature set; the remaining geometric sensitivity reflects the correlation of dt with the distance from the scanner axis.

It is worth noting that the generalisation performance is asymmetric with respect to the direction of cross-inference. Models trained on the more complex XCAT and evaluated on NEMA IEC suffer smaller accuracy losses than the reverse. In this case, a degradation in accuracy by -0.010 and -0.018 is observed for the 6-feature and 4-feature variants, respectively. However, we do observe two adverse effects: first, the 6-feature variant has a visible tendency to apply a circular cut in the transverse plane, visible in Fig. 14c - a result of the inclusion of the $deg2D$ feature. In the evaluated setup, this does not lead to performance degradation as the geometry of the small phantom is largely cylindrical. Second, both variants result in degraded accuracy at the NEMA IEC phantom's extreme horizontal edges, indicating a mismatch between the clean geometry of the smaller phantom, which mimics the patient's torso, and the sophisticated phantom that includes the patient's arms. The results indicate that a careful selection of the training data phantom is crucial, with the best approach being a mixture of diverse phantoms.

For the *top-1* selection mode, our best models achieve accuracies of up to 0.738 and 0.691 with an MCC metric of 0.60 and 0.51 for the NEMA IEC and XCAT phantoms, respectively, outperforming the geometry-based cut baseline. However, examination of the spatial quality maps and confusion matrices reveals an important limitation: the classifier’s background rejection power is highest for the out-of-phantom coincidences and regions where LORs do not traverse the full phantom cross-section, resulting in a smaller scatter fraction. This is physically understood: phantom-scattered photons, especially at small angles, share kinematic properties similar to those of true coincidences, and the features available in this study provide limited information for distinguishing them from true coincidences.

We therefore conclude that event-by-event ML classification with a minimal low-level feature set represents a viable, geometry-agnostic alternative to traditional cut-based coincidence rejection, but does not on its own constitute a complete solution to the background problem in LAFOV PET. Meaningful further suppression of in-phantom scattered background will likely require incorporating additional discriminating information — such as Time-of-Flight consistency, higher-level topological features computed with respect to an estimated patient density map, or integration with iterative reconstruction — as well as evaluation on a broader range of clinical activity distributions. These directions define the natural scope of future work building on the foundation established here.

V. CONCLUSIONS

We have presented a systematic study of event-by-event coincidence classification using machine learning as a pre-reconstruction background-rejection strategy for LAFOV PET scanners, evaluated via MC simulations of the Siemens Biograph Vision Quadra with NEMA IEC and XCAT phantoms. Three classifier architectures were compared: XGBoost, AdaBoost, and MLP across two feature sets and two phantom geometries, with generalisation assessed through cross-phantom inference.

Our central finding is that neither using a compact 4-feature representation that excludes topological variables nor using a more complex phantom as training data guarantees high model performance on out-of-distribution data. A careful selection of the training features is critical as it can introduce non-trivial biases and provide an easy path for the model to shortcut a solution. It is common in the literature to find studies in which a model is trained

on the largest available phantom that roughly covers the region of interest; for example, in [Oliver *et al.* \(2013\)](#), such an approach can lead to nontrivial model-deficiency regions. A recommended approach is to use a diverse set of phantoms during training to represent expected variations in the target data.

The spatial quality map analysis, which exploits the one-to-one correspondence between coincidence events and reconstructed voxels provided by direct TOF reconstruction, reveals localised performance patterns that global metrics alone would not detect. This methodology is proposed as a standard complement to aggregate performance evaluation in future studies of event-by-event ML filtering. In particular, they offer an important insight for the crucial task of feature and training data selection.

The primary performance boundary of the current approach is the phantom-scattered coincidence class, which constitutes approximately 25% of all events and remains difficult to reject with the considered feature set due to the overlap in observable properties with true coincidences. In this work, we establish a baseline and methodology for future work on extended event-by-event methods that will incorporate additional discriminating information.

ACKNOWLEDGMENTS

The authors acknowledge the technical support of A. Spirzewska. This work was completed with resources provided by the Świerk Computing Centre at the National Centre for Nuclear Research. We gratefully acknowledge Polish high-performance computing infrastructure PLGrid (HPC Center: ACK Cyfronet AGH) for providing computer facilities and support within computational grant no. PLG/2024/017403. The „IMPET – Industrial Multiphoton PET Tomography FENG.02.02-IP.05-0152/23” project is carried out within the FIRST TEAM FENG programme of the Foundation for Polish Science co-financed by the European Union under the European Funds for Smart Economy 2021-2027 (FENG).

REFERENCES

Agostinelli, S., Allison, J., Amako, K., Apostolakis, J., Araujo, H., Arce, P., Asai, M., Axen, D., Banerjee, S., Barrand, G., Behner, F., Bellagamba, L., Boudreau, J., Broglia, L., Brunengo, A., Burkhardt, H., Chauvie, S., Chuma, J., Chytracek, R., Cooperman, G., Cosmo, G., Degtyarenko, P., Dell'Acqua, A., Depaola, G., Dietrich, D., Enami, R., Feliciello, A., Ferguson, C., Fesefeldt, H., Folger, G., Foppiano, F., Forti, A., Garelli, S., Giani, S., Giannitrapani, R., Gibin, D., Gómez Cadenas, J., González, I., Gracia Abril, G., Greeniaus, G., Greiner, W., Grichine, V., Grossheim, A., Guatelli, S., Gumplinger, P., Hamatsu, R., Hashimoto, K., Hasui, H., Heikkinen, A., Howard, A., Ivanchenko, V., Johnson, A., Jones, F., Kallenbach, J., Kanaya, N., Kawabata, M., Kawabata, Y., Kawaguti, M., Kelner, S., Kent, P., Kimura, A., Kodama, T., Kokoulin, R., Kossov, M., Kurashige, H., Lamanna, E., Lampén, T., Lara, V., Lefebure, V., Lei, F., Liendl, M., Lockman, W., Longo, F., Magni, S., Maire, M., Medernach, E., Minamimoto, K., Mora De Freitas, P., Morita, Y., Murakami, K., Nagamatu, M., Nartallo, R., Nieminen, P., Nishimura, T., Ohtsubo, K., Okamura, M., O'Neale, S., Oohata, Y., Paech, K., Perl, J., Pfeiffer, A., Pia, M., Ranjard, F., Rybin, A., Sadilov, S., Di Salvo, E., Santin, G., Sasaki, T., Savvas, N., Sawada, Y., Scherer, S., Sei, S., Sirotenko, V., Smith, D., Starkov, N., Stoecker, H., Sulkimo, J., Takahata, M., Tanaka, S., Tcherniaev, E., Safai Tehrani, E., Tropeano, M., Truscott, P., Uno, H., Urban, L., Urban, P., Verderi, M., Walkden, A., Wander, W., Weber, H., Wellisch, J., Wenaus, T., Williams, D., Wright, D., Yamada, T., Yoshida, H., and Zschesche, D., [Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment](#) **506**, 250 (2003).

Arabi, H., AkhavanAllaf, A., Sanaat, A., Shiri, I., and Zaidi, H., [Physica Medica](#) **83**, 122 (2021).

Badawi, R. D., Shi, H., Hu, P., Chen, S., Xu, T., Price, P. M., Ding, Y., Spencer, B. A., Nardo, L., Liu, W., Bao, J., Jones, T., Li, H., and Cherry, S. R., [Journal of Nuclear Medicine](#) **60**, 299 (2019).

Baran, J., Krzemien, W., Parzych, S., Raczyński, L., Bała, M., Coussat, A., Chug, N., Czerwiński, E., Curceanu, C. O., Dadgar, M., Dulski, K., Eliyan, K., Gajewski, J., Gajos, A., Hiesmayr, B. C., Kacprzak, K., Kapłon, Ł., Klimaszewski, K., Korcyl, G., Kozik, T., Kumar, D., Niedźwiecki, S., Panek, D., Perez Del Rio, E., Ruciński, A., Sharma, S., Shivani, Shopa, R. Y., Skurzok,

- M., Stepień, E., Tayefiardebili, F., Tayefiardebili, K., Wiślicki, W., and Moskal, P., *Medical Physics* **52**, 2961 (2025).
- Brasse, D., Kinahan, P. E., Lartizien, C., Comtat, C., Casey, M., and Michel, C., *Journal of Nuclear Medicine* **46**, 859 (2005).
- Breiman, L., *Machine Learning* **45**, 5 (2001).
- Brochu, E., Cora, V. M., and de Freitas, N., *CoRR* **abs/1012.2599** (2010), 1012.2599.
- Chen, T. and Guestrin, C., in *Proceedings of the 22nd ACM SIGKDD International Conference on Knowledge Discovery and Data Mining* (ACM, San Francisco California USA, 2016) pp. 785–794.
- Chollet, F. *et al.*, “Keras,” <https://github.com/fchollet/keras> (2015).
- Daube-Witherspoon, M. E., Pantel, A. R., Pryma, D. A., and Karp, J. S., *BJR* **95**, 20220357 (2022).
- Debus, J., Debus, C., Dissertori, G., and Götz, M., in *2024 Neuro Inspired Computational Elements Conference (NICE)* (2024) pp. 1–9.
- Esquinas, P. L., Yousefirizi, F., Alberts, I., Karakatsanis, N. A., Rahmim, A., and Uribe, C. F., *PET Clinics* **21**, 43 (2026).
- Freund, Y. and Schapire, R. E., *Journal of Computer and System Sciences* **55**, 119 (1997).
- Head, T., Kumar, M., Nahrstaedt, H., Louppe, G., and Shcherbatyi, I., “Scikit-optimize/scikit-optimize,” Zenodo (2021).
- Jones, D., Schonlau, M., and Welch, W., *Journal of Global Optimization* **13**, 455 (1998).
- Karakatsanis, N. A., *British Journal of Radiology* , tqag060 (2026).
- Kingma, D. P. and Ba, J., *arXiv preprint arXiv:1412.6980* (2014), 10.48550/arXiv.1412.6980.
- Laurent, B., Bousse, A., Merlin, T., Nekolla, S., and Visvikis, D., *Physics in Medicine & Biology* **68**, 065004 (2023).
- Merlin, T., Stute, S., Benoit, D., Bert, J., Carlier, T., Comtat, C., Filipovic, M., Lamare, F., and Visvikis, D., *Phys. Med. Biol.* **63**, 185005 (2018).

- Michaud, J.-B., Tetrault, M.-A., Beaudoin, J.-F., Cadorette, J., Leroux, J.-D., Brunet, C.-A., Lecomte, R., and Fontaine, R., [IEEE Trans. Nucl. Sci. **62**, 82 \(2015\)](#).
- Mockus, J., *Journal of Global Optimization* **4**, 347 (1994).
- NEMA,, “Nema standards publication nu 2-2018: Performance measurements of positron emission tomographs (pet),” (2018), national Electrical Manufacturers Association (NEMA NU 2-2018).
- Oliver, J. F., Fuster-Garcia, E., Cabello, J., Tortajada, S., and Rafecas, M., [IEEE Trans. Nucl. Sci. **60**, 3399 \(2013\)](#).
- Pantel, A. R., Viswanath, V., Daube-Witherspoon, M. E., Dubroff, J. G., Muehllehner, G., Parma, M. J., Pryma, D. A., Schubert, E. K., Mankoff, D. A., and Karp, J. S., [J Nucl Med **61**, 144 \(2020\)](#).
- Prenosil, G. A., Sari, H., Fürstner, M., Afshar-Oromieh, A., Shi, K., Rominger, A., and Hentschel, M., [J Nucl Med **63**, 476 \(2022\)](#).
- Reader, A. J., Corda, G., Mehranian, A., Costa-Luis, C. D., Ellis, S., and Schnabel, J. A., [IEEE Trans. Radiat. Plasma Med. Sci. **5**, 1 \(2021\)](#).
- Sarrut, D., Arbor, N., Baudier, T., Borys, D., Etxebeste, A., Fuchs, H., Gajewski, J., Grevillot, L., Jan, S., Kagadis, G. C., Kang, H. G., Kirov, A., Kochebina, O., Krzemien, W., Lomax, A., Papadimitroulas, P., Pommranz, C., Roncali, E., Rucinski, A., Winterhalter, C., and Maigne, L., [Phys. Med. Biol. **67**, 184001 \(2022\)](#).
- Sarrut, D., Bała, M., Bardiès, M., Bert, J., Chauvin, M., Chatzipapas, K., Dupont, M., Etxebeste, A., M Fanchon, L., Jan, S., Kayal, G., S Kirov, A., Kowalski, P., Krzemien, W., Labour, J., Lenz, M., Loudos, G., Mehadji, B., Ménard, L., Morel, C., Papadimitroulas, P., Rafecas, M., Salvadori, J., Seiter, D., Stockhoff, M., Testa, E., Trigila, C., Pietrzyk, U., Vandenberghe, S., Verdier, M.-A., Visvikis, D., Ziemons, K., Zvolský, M., and Roncali, E., [Phys. Med. Biol. **66**, 10TR03 \(2021\)](#).
- Segars, W. P., Sturgeon, G., Mendonca, S., Grimes, J., and Tsui, B. M. W., [Medical Physics **37**, 4902 \(2010\)](#).
- Silva-Rodríguez, J., Aguiar, P., Domínguez-Prado, I., Fierro, P., and Ruibal, Á., *Revista Española de Medicina Nuclear e Imagen Molecular (English Edition)* **34**, 13 (2015).

- Slart, R. H. J. A., Tsoumpas, C., Glaudemans, A. W. J. M., Noordzij, W., Willemsen, A. T. M., Borra, R. J. H., Dierckx, R. A. J. O., and Lammertsma, A. A., [Eur J Nucl Med Mol Imaging](#) **48**, 4236 (2021).
- Surti, S., Pantel, A. R., and Karp, J. S., [IEEE Trans. Radiat. Plasma Med. Sci.](#) **4**, 283 (2020).
- Vandenberghe, S., Muller, F. M., Withofs, N., Dadgar, M., Maebe, J., Vervenne, B., Akl, M. A., Xue, S., Shi, K., Sportelli, G., Belcari, N., Hustinx, R., Vanhove, C., and Karp, J. S., [Eur J Nucl Med Mol Imaging](#) **50**, 3558 (2023).
- Wang, Q., Mikhaylova, E., Baikejiang, R., and Cherry, S. R., [Phys. Med. Biol.](#) **65**, 175016 (2020).
- Yamagishi, S., Miwa, K., Kamitaki, S., Anraku, K., Sato, S., Yamao, T., Kubo, H., Miyaji, N., and Oguchi, K., [J Nucl Med](#) **64**, 1990 (2023).
- Zincirkeser, S., Şahin, E., Halac, M., and Sager, S., *Journal of international medical research* **35**, 231 (2007).

Appendix A: Tuning of model hyperparameters

As described in section [II B](#) the model’s hyperparameters are tuned using Bayesian Optimisation. Both the search ranges and the best values for each hyperparameter are presented in the [Table IV](#). In the table the best values obtained for the NEMA IEC and XCAT samples are compared. It can be observed that most of them have comparable values for the two samples. The accuracy dependence on the hyperparameter values is presented in the [Figures 1, 16, 17, and 18](#), for the XGBoost, AdaBoost, and Neural Network models, respectively. For brevity it is only presented for the XCAT sample.

model	hyperparameter	range	prior	best NEMA	best XCAT
AdaBoost	learning rate	$(1.0 \times 10^{-2}, 1.0)$	log-uniform	0.35	0.05
	max depth	(1, 30)	uniform	3	7
	estimators	(2, 200)	log-uniform	200	200
MLP	learning rate	$(1.0 \times 10^{-2}, 1.0)$	log-uniform	0.2	0.2
	layer size	(2, 300)	log-uniform	205	300
	layer count	(2, 10)	uniform	2	2
	dropout	(0.0, 0.9)	uniform	0.0	0.0
	batch size	(32, 4096)	log-uniform	223	555
XGBoost	learning rate	$(1.0 \times 10^{-3}, 1.0 \times 10^{-1})$	log-uniform	0.1	0.08
	max depth	(1, 10)	uniform	8	9
	gamma	$(1.0 \times 10^{-6}, 1.0 \times 10^4)$	log-uniform	1.0×10^{-6}	0.05
	subsample	(0.5, 1.0)	uniform	0.79	0.58
	colsample bytree	(0.5, 1.0)	uniform	1.0	0.98
	min child weight	(1, 5)	uniform	5	2
	estimators	(2, 200)	log-uniform	200	175
	alpha	$(1.0 \times 10^{-6}, 1.0 \times 10^3)$	log-uniform	1.0×10^{-6}	5.0×10^{-6}
	lambda	$(1.0 \times 10^{-6}, 1.0 \times 10^3)$	log-uniform	1.0×10^{-6}	2.0×10^{-6}

Table IV. Model hyperparameters evaluated using Bayesian Optimisation, together with the best values obtained for each dataset.

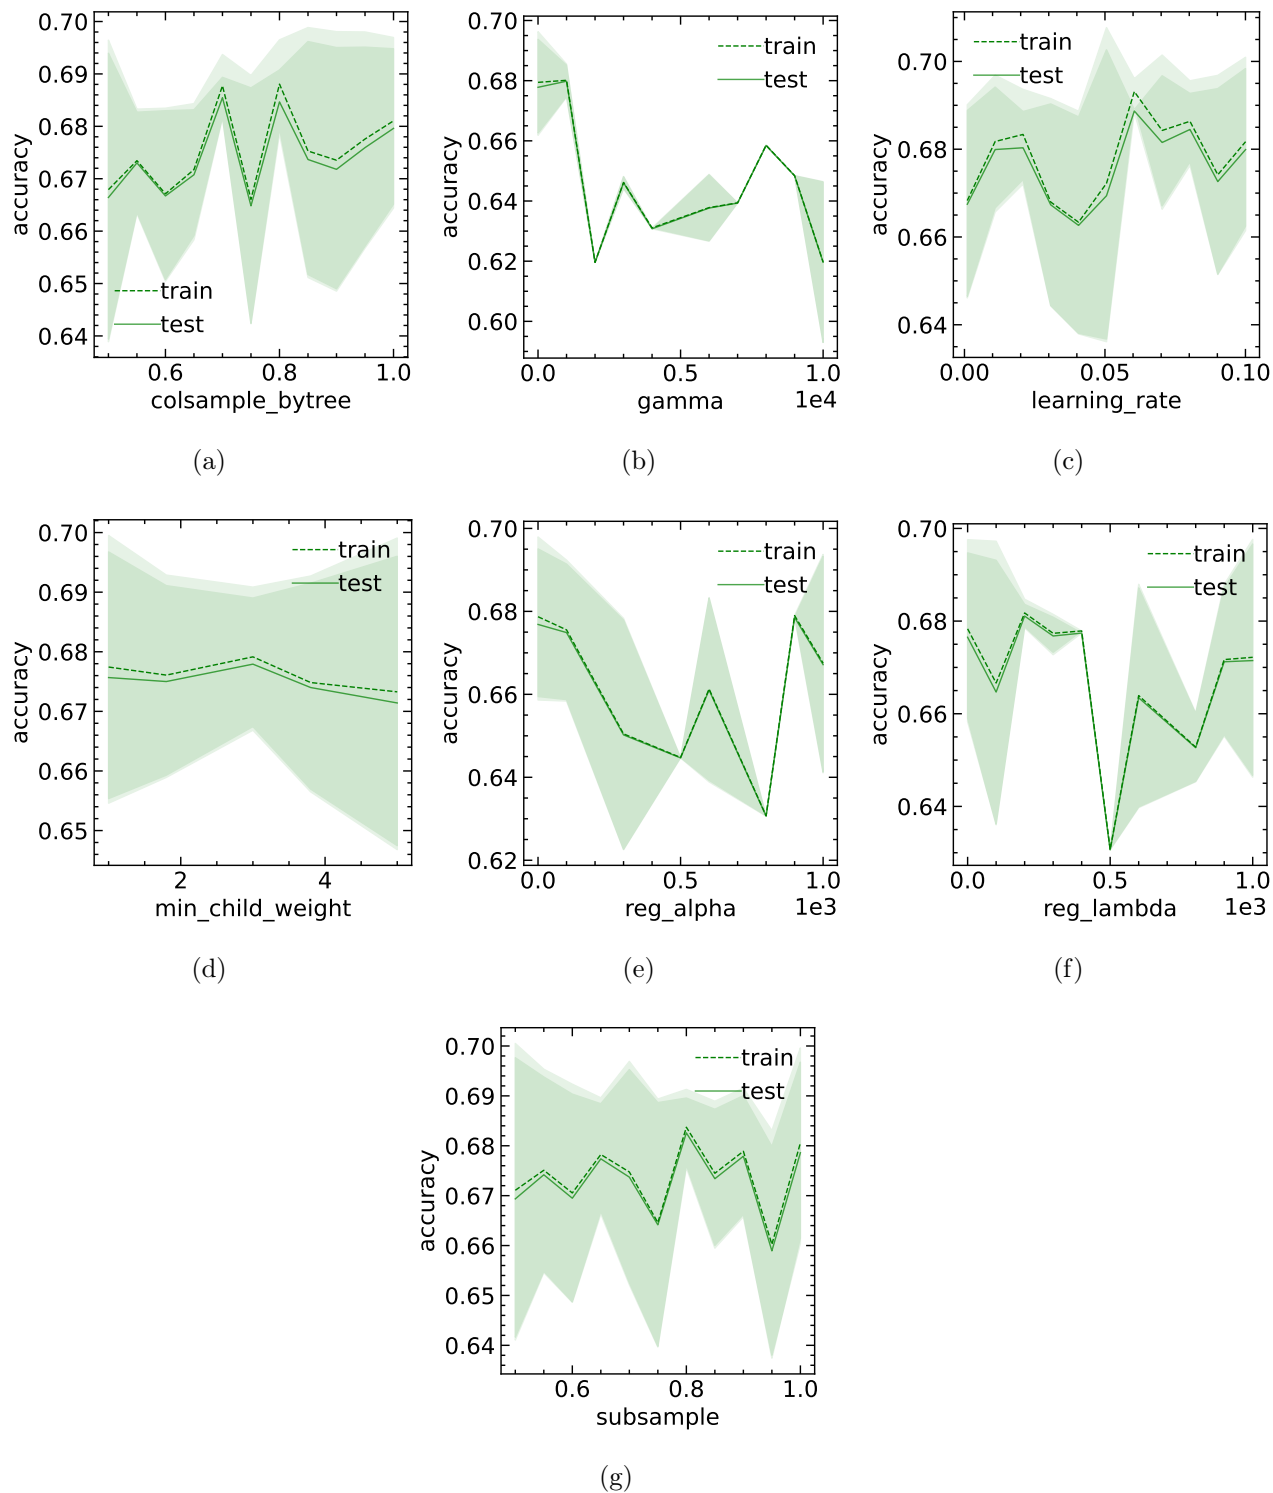


Figure 16. Distribution of accuracy as a function of regularisation hyperparameters values for the 6-feature XGBoost model trained on the XCAT sample.

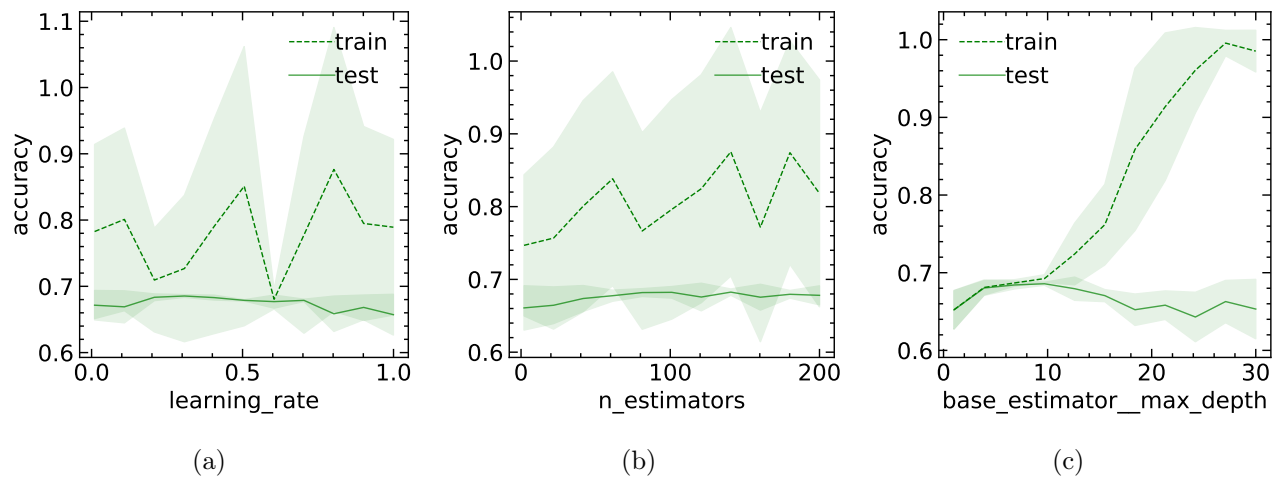


Figure 17. Distribution of accuracy as a function of hyperparameter values for the 6-feature AdaBoost model trained on the XCAT sample.

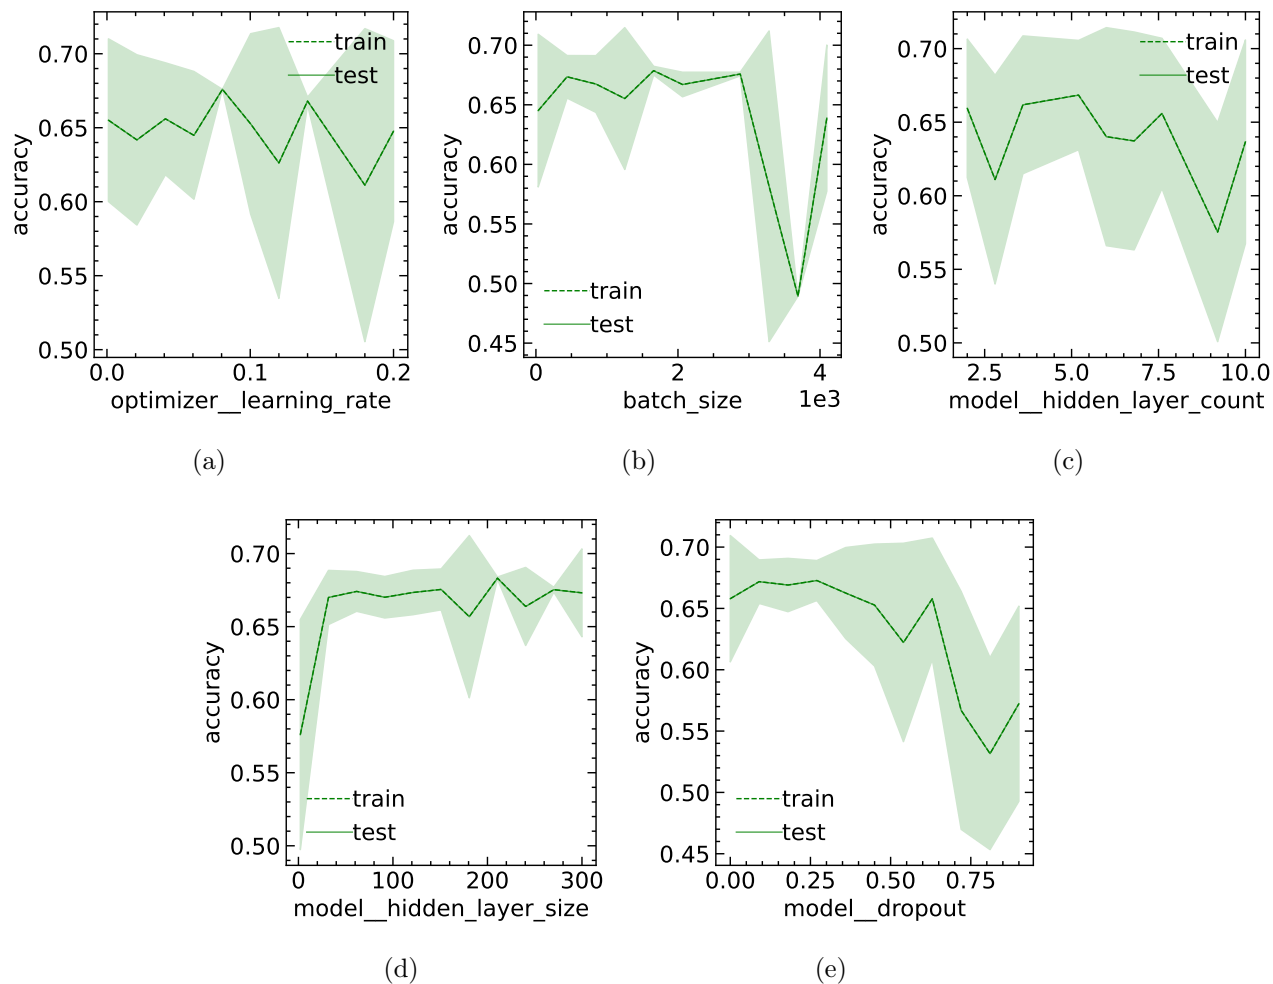


Figure 18. Distribution of accuracy as a function of hyperparameter values for the 6-feature NN model trained on the XCAT sample.

Appendix B: Feature importance

The feature importance, described in section IV A, for the 6-feature XGBoost and AdaBoost models trained on both the NEMA IEC and XCAT samples is presented in Fig. 19. For all models the permutation importance is presented in Fig. 20, also for both data samples.

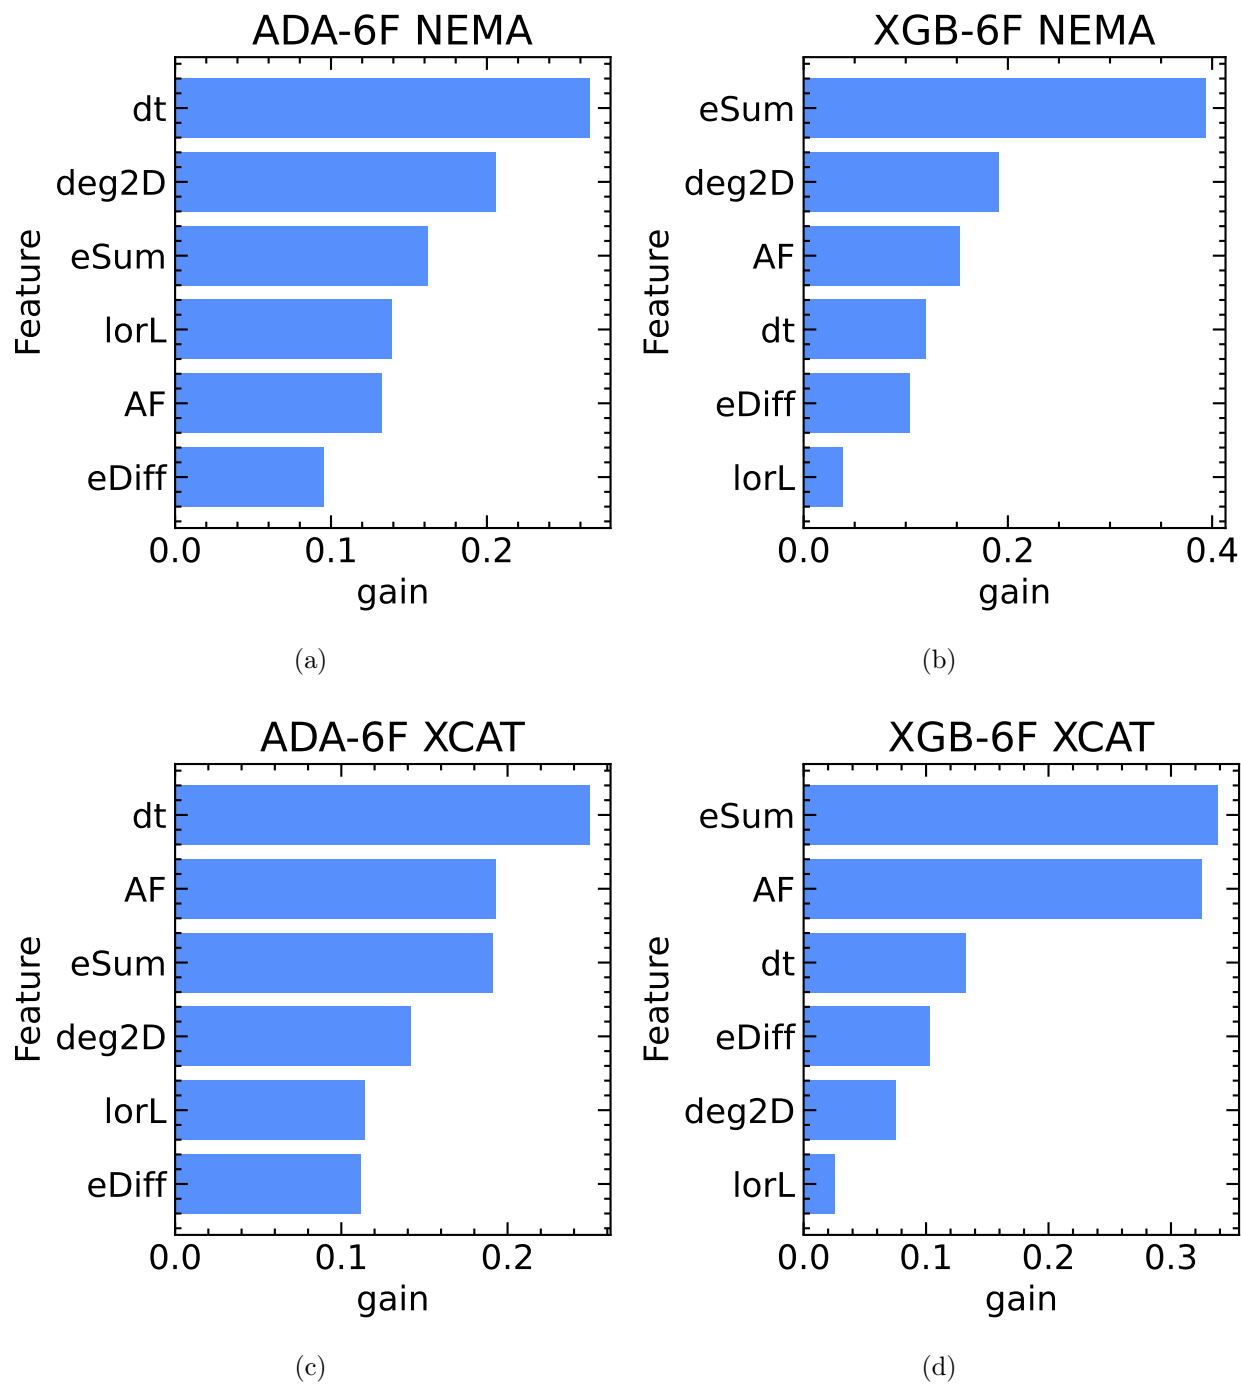


Figure 19. Feature importance for the AdaBoost (left column) and XGBoost (right column) models trained on the NEMA IEC (top row) and XCAT (bottom row) samples.

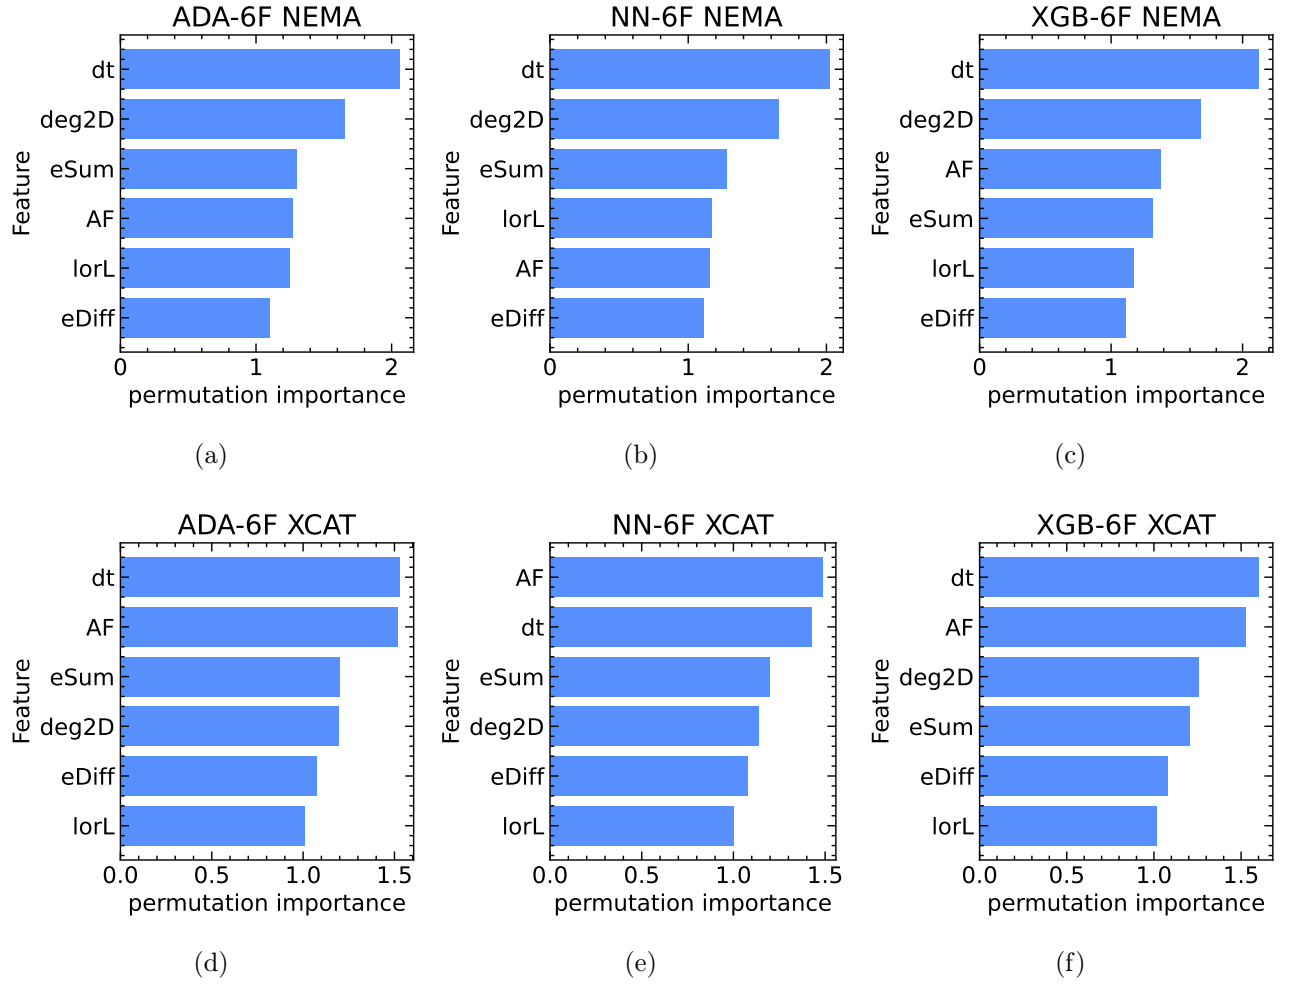


Figure 20. Permutation feature importance for the AdaBoost (left column), Neural Network (central column), and XGBoost (right column) models trained on the NEMA IEC (top row) and XCAT (bottom row) samples.