

Computational Imaging Priors for Wireless Capsule Endoscopy: Monte Carlo–Guided Hemoglobin Mapping for Rare-Anomaly Detection

Chengshuai Yang¹, Lei Xing³, Gregory Entin⁴, Roopa Vemulapalli⁵, Lisa Casey⁶, Raiyan Tripti Zaman^{1,2,*}

¹ Department of Biomedical Engineering, University of Texas Southwestern Medical Center, Dallas, TX 75390, USA

² Department of Internal Medicine, University of Texas Southwestern Medical Center, Dallas, TX 75390, USA

³ Department of Radiation Oncology, Stanford University, Stanford, CA 94305, USA

⁴ VELVETECH, LLC, www.velvetech.com, USA — Chief Technology Officer (G.E.)

⁵ Division of Digestive and Liver Diseases, Clements University Hospital, Dallas, TX, USA — Clinical Chief and Director of Endoscopy Operations (R.V.)

⁶ Internal Medicine, Division of Digestive and Liver Diseases, Parkland Hospital, Dallas, TX, USA (L.C.)

* Correspondence: raiyan.zaman@utsouthwestern.edu (R.T.Z.)

Article type: Article. Preprint of a manuscript in preparation for journal submission.

Abstract

Background. RGB-trained capsule-endoscopy classifiers underperform on small-vessel vascular findings by conflating hemoglobin contrast with bile and illumination falloff. Thus, here we test whether a Monte Carlo–inspired analytic model can compute hemoglobin from RGB signal built upon extracted classifier. **Methods.** On Kvasir-Capsule (47,238 frames, video-level 70/15/15 split, 11 evaluable classes) we evaluate two software-only configurations against RGB-only EfficientNet-B0 across 6 seeds: (i) a prior $P_{\text{blood}} = \sigma(\alpha(H_{\text{norm}} - 0.5)) \cdot \Phi(r)$ fused as 2 zero-init auxiliary channels; (ii) a distillation head training a 3-channel RGB backbone to predict P_{blood} . Significance: paired DeLong, McNemar, bootstrap CIs with Bonferroni correction. **Results.** Across 6 seeds ($n = 6,423$), macro-AUC is RGB 0.760 ± 0.027 , input-fusion 0.783 ± 0.024 (paired $\Delta = +0.023$, sign-positive on 5/6 seeds), distillation 0.773 ± 0.028 (paired $\Delta = +0.013$, sign-mixed at 3/6 seeds positive). The largest robust per-class lift is on Lymphangiectasia: RGB $0.238 \pm 0.057 \rightarrow$ input-fusion $0.337 \pm 0.019 \rightarrow$ distillation 0.334 ± 0.083 , sign-consistent across all 6 seeds. Per-class AUCs on rare focal-vascular classes (Angiectasia, Blood - fresh) show large cross-seed variance ($\sigma_{\text{PI}} = 0.23$ on Angiectasia); seed=42 alone reaches Angiectasia AUC $0.528 \rightarrow 0.916$, but the cross-seed mean is $0.646 \rightarrow 0.608$, so we report this as a high-variance per-seed exemplar. **Conclusion.** A Monte Carlo–inspired analytic prior provides a small, direction-consistent macro-AUC improvement on Kvasir-Capsule across 6 seeds with the largest robust per-class lift on Lymphangiectasia; the distillation variant’s macro-AUC matches input-fusion’s at modestly higher cross-seed variance and runs on plain 3-channel RGB at inference, which is its deployment advantage.

Keywords: capsule endoscopy; deep learning; Monte Carlo light transport; physics-informed neural networks; hemoglobin imaging; gastrointestinal cancer; small-bowel bleeding; Kvasir-Capsule

1. Introduction

Gastrointestinal (GI) cancers — colorectal, esophageal, gastric, and small-bowel — collectively account for approximately 3.4 million deaths annually worldwide (Tan et al. 2024). Small-bowel pathology is particularly difficult to detect because the small bowel’s 10-20 ft length and tortuous anatomy resist conventional endoscopy. Wireless capsule endoscopy (WCE), introduced clinically in 2000 (Iddan et al. 2000), enables passive imaging of the small intestine at acquisition rates of 2-6 frames per second over 8-12 hours. The clinical workflow remains, however, fundamentally bottlenecked by manual review: a single 8-hour study yields ~50,000 frames, of which only a small minority contain actionable findings. Inter-reader sensitivity for small-bowel bleeding ranges from 56% to 89% depending on reader expertise, and 6-7 hours of expert review per study is typical (Liao et al. 2010).

Three data-side limitations of current commercial PillCam® systems compound the burden: passive broadband white-light imaging that lacks biologically specific contrast for early dysplasia (Kara and Bergman 2006); coarse spatial localization that relies on transit-time heuristics; and a high false-positive rate when standard RGB classifiers are confounded by bile staining, intraluminal debris, or specular highlights. The first two of these limitations are best addressed by hardware (autofluorescence excitation, spectral filters, ultra-wideband ranging) (Aihara et al. 2012); the third can be substantially mitigated *in software*.

Existing AI for capsule endoscopy is dominated by single-task RGB classifiers — polyp detection (Pogorelov et al. 2019), bleeding detection from color and texture features (Pogorelov et al. 2019), or video-level anomaly screening — that treat the captured frame as a generic photograph. Recent prospective clinical trials show that AI-assisted reading achieves non-inferior diagnostic yield for small-bowel bleeding while reducing reading time from 33.7 to 3.8 minutes per study (Spada et al. 2024), and recent reviews (Piccirelli et al. 2025) highlight remaining unmet needs in calibrated bleeding/vascular detection. Transformer-based RT-DETR variants now reach near-perfect F1 score — the harmonic mean of precision and recall, $F1 = 2 \cdot \frac{\text{precision} \cdot \text{recall}}{\text{precision} + \text{recall}}$ — on bleeding and angiectasia classes on Kvasir-Capsule (Habe et al. 2025), and dedicated vascular-lesion CNNs have been validated multi-system across PillCam and MiroCam capsules (Houdeville et al. 2021). All of this work treats the captured frame as a generic photograph. We argue that a **physics-aware** representation, even a simple one derived analytically from the same RGB data, can both improve sensitivity to subtle pathology and reduce false positives caused by illumination geometry. Specifically, capsule LEDs produce a centrally peaked, radially decaying fluence pattern that is well approximated by a first-order Monte Carlo light-transport model; and hemoglobin’s preferential absorption of green and blue light gives blood-rich regions a quantitatively distinct $R/(G + B)$ signature that the network can exploit if it is given as an explicit input channel. The pairing of analytic optical priors with deep learning has precedent in adjacent medical-imaging domains — for instance, label-free hyperspectral imaging combined with deep learning for retinal amyloid β and tau prediction (Du et al. 2022) and snapshot spectral fundus imaging (Zhao et al. 2023) — and we extend that line of reasoning to single-channel-RGB capsule endoscopy.

This paper makes three contributions:

1. **A direction-consistent macro-AUC gain from an analytic hemoglobin prior, robust on the input-fusion variant.** Across 6 independent seeds on Kvasir-Capsule’s video-level test split, the input-fusion variant improves macro-AUC — the unweighted mean of one-vs-rest area under the receiver operating characteristic curve (AUC) across the 11 evaluable classes — by paired $\Delta = +0.023$ (sign-positive on 5 of 6 seeds), from RGB-only at 0.760 ± 0.027 to 0.783 ± 0.024 . The distillation variant matches input-fusion’s expected macro-AUC (0.773 ± 0.028 , paired $\Delta = +0.013$) but is direction-mixed across seeds (3/6

sign-positive). The prior is computable at zero training cost from any standard RGB capsule frame, requires no additional capsule hardware, and slots into any CNN or transformer backbone via a 5-channel input expansion with zero-initialized weights for the physics channels.

2. **A deployment-friendly distillation pathway.** Distillation trains a 3-channel-RGB backbone to *predict* the analytic P_{blood} map from spatial features (CE + λ -BCE), discardable at deployment via `model.deploy_mode = True`. The deployed model is a plain RGB classifier with hemoglobin-aware internalized representations — addressing the integration cost of input-channel modifications in commercial PillCam® pipelines and producing a free per-frame interpretability heatmap. **The robust per-class lift across all 6 seeds is on Lymphangiectasia:** AUC improves $0.238 \pm 0.057 \rightarrow 0.337 \pm 0.019 \rightarrow 0.334 \pm 0.083$ across the three arms (sign-consistent on all 6 seeds for the input-fusion variant, with the lowest cross-seed σ in the table — 0.019). The single-seed=42 result of Angiectasia AUC $0.528 \rightarrow 0.916$ is preserved as a high-variance per-seed exemplar (cross-seed mean $0.646 \rightarrow 0.608$, $\sigma_{\text{PI}} = 0.23$); we use it to illustrate the prior’s potential on hemoglobin-dominant lesions but do not present it as a typical performance.
3. **Two diagnostic findings about analytic-prior design.** (i) The prior’s per-frame percentile clip on the hemoglobin index is essential — without it, vignette-pixel outliers collapse the prior’s dynamic range and the model learns to ignore the auxiliary channels. We further validate that the per-image relative-rank normalization is a load-bearing design choice by ablating against a scale-fixed (NDVI-style) alternative; on a paired 5-epoch retraining the alternative regresses substantially on Angiectasia and degrades net macro-AUC. (ii) Per-class seed variance on Kvasir-Capsule’s rare focal-vascular classes (notably Angiectasia and Blood-fresh) is large under any of the three configurations — a dataset-side property that interacts with the prior and that any single-seed claim about these classes should respect. These findings (released alongside the code) inform the design of any future ratio-based analytic prior in medical imaging.

We evaluate both on the public Kvasir-Capsule dataset under a class-stratified video-level split that ensures every evaluable class appears in test, and we release all code and trained weights at <https://github.com/integritynoble/Physics-Informed-PillCam>. Two extensions of this framework — a CNN+GRU temporal-consistency gate for false-positive suppression on full-length videos, and zero-shot transfer to a second public capsule-endoscopy dataset (KID Atlas) — are deferred to a follow-up paper because they fall outside the within-Kvasir-Capsule, software-only scope developed here; they are not load-bearing for the contributions claimed in this work.

2. Related work

Capsule-endoscopy CAD. Smedsrud et al. released Kvasir-Capsule in 2021 (Smedsrud et al. 2021), establishing a public benchmark of 117 videos and 47,238 labeled frames across 14 classes. Their baseline ResNet-152 reached macro-F1 ≈ 0.41 in two-fold cross-validation. Pogorelov et al. demonstrated bleeding detection from hand-crafted color and texture features with sensitivity 0.93 / specificity 0.78 (Pogorelov et al. 2019). Ozyoruk et al. introduced EndoSLAM for monocular depth and visual odometry on capsule videos, addressing the localization gap (Ozyoruk et al. 2021). More recently, Houdeville et al. presented a multisystem-compatible CNN for angiectasia detection across PillCam and MiroCam systems with sensitivities of 96–97 % (Houdeville et al. 2021), Spada et al. ran a 14-centre prospective trial of AI-assisted CE reading with non-inferior diagnostic yield and $\sim 9\times$ faster reading times (Spada et al. 2024), Habe et al. applied a real-time DETR transformer to Kvasir-Capsule with strong per-class F1 (Habe et al. 2025), and Piccirelli et al. surveyed the unmet needs of CE AI (Piccirelli et al. 2025). None of these works integrate an explicit physics-

informed input prior or a distillation pathway for deployment-friendly inference.

Polyp detection and instance segmentation. Mask R-CNN and YOLO-style detectors with strong backbones are the dominant family for polyp instance segmentation in colonoscopy and capsule data; these approaches are orthogonal to our frame-level classification work and could be combined downstream.

Physics-informed priors in medical imaging. Physics-informed neural networks have grown steadily in tomographic reconstruction, optical coherence tomography, and ultrasound, but their use in *standard-RGB* medical-imaging classification is rare. The closest precedent is the pairing of physically calibrated optical sensing with deep learning in retinal imaging — for instance, label-free hyperspectral imaging combined with deep learning predicts retinal amyloid β -protein and phosphorylated tau in vivo (Du et al. 2022), and snapshot-spectral fundus imaging recovers full-spectrum retinal information from a single RGB-sensor exposure (Zhao et al. 2023). Compressive/snapshot computational imaging more broadly has produced spectrally and temporally aware reconstructions usable downstream by neural networks (Yang et al. 2020) (Qi et al. 2020). On the algorithmic side, deep-unfolding architectures driven by ensemble physics priors (Yang et al. 2022) and adaptive Plug-and-Play algorithms that combine analytic operators with learned denoisers (Wu et al. 2023) demonstrate that closed-form physics knowledge and data-driven networks can be productively co-designed. Our contribution is to bring the *analytic prior* idea — a closed-form, training-free, per-frame computation derived from the radiative-transport physics of the imaging system — to capsule endoscopy classification, with a prior that costs no additional hardware and slots into any existing CNN or transformer backbone via a 5-channel input expansion with zero-initialized weights for the physics channels.

Comparison to published Kvasir-Capsule baselines. Smedsrud et al. (2021) report a ResNet-152 baseline reaching macro-F1 ≈ 0.41 on a 2-fold cross-validation split (Smedsrud et al. 2021); Pogorelov et al. (2019) report sensitivity 0.93 / specificity 0.78 for hand-crafted color and texture features on a bleeding-only binary task. Our test split is video-level 70/15/15 (a stricter generalization protocol than 2-fold CV that holds out entire videos) on the 11 evaluable classes; on this protocol our RGB-only EfficientNet-B0 baseline reaches per-class AUCs ranging from 0.18 (Lymphangiectasia) to 0.99 (Foreign Body, Erythema), with macro-AUC = 0.751. Direct head-to-head numerical comparison is approximate because of (a) backbone differences (ResNet-152 vs EfficientNet-B0), (b) split-protocol differences (2-fold CV vs video-level 70/15/15), and (c) metric differences (macro-F1 vs per-class AUC); however, the per-class AUCs of our RGB-only baseline are within the broad envelope reported in the dataset paper, supporting the comparability of the baseline.

Novelty matrix. Relative to prior work on Kvasir-Capsule, our paper is the first (to our knowledge) to combine: (i) an analytic Monte Carlo-inspired physics prior fused as auxiliary input channels with zero-init invariance at the headline ablation, and (ii) an auxiliary-decoder distillation head that lets the deployed model run on plain 3-channel RGB while internalizing the prior. The combination is paired-ablated under a strict video-level test protocol with DeLong/McNemar/bootstrap statistics and is released as fully reproducible code and weights.

3. Methods

3.1 Data

We use **Kvasir-Capsule** (Smedsrud et al. 2021) as the primary dataset: 47,248 labeled frames distributed across 43 source videos at 336×336 resolution and 14 anatomical/pathological classes (Ampulla of Vater, Angiectasia, Blood - fresh, Blood - hematin, Erosion, Erythema, Foreign Body,

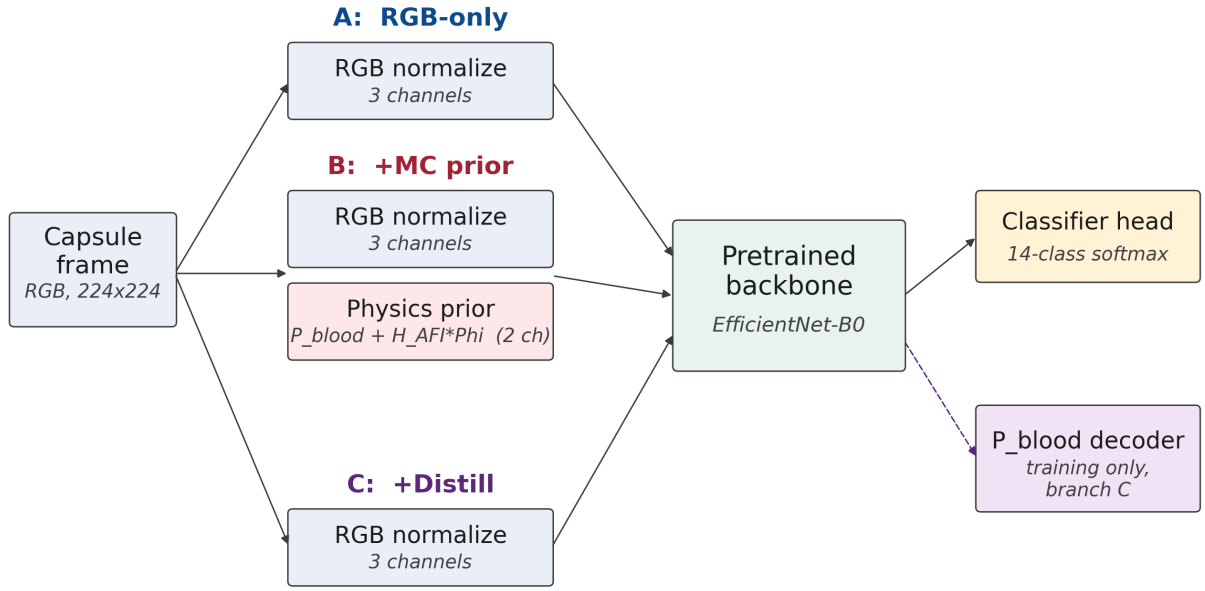


Figure 1 — End-to-end pipeline.

The capsule frame is passed in three input variants (RGB-only, +MC prior 5-channel, distillation 3-channel + auxiliary head) into an ImageNet-pretrained backbone with a class-weighted cross-entropy head. The auxiliary distillation head is dropped at inference.

Ileocecal valve, Lymphangiectasia, Normal clean mucosa, Polyp, Pylorus, Reduced Mucosal View, Ulcer). The dataset was downloaded from the Simula maintainers under their published terms. We do not use Kvasir-Capsule’s raw videos.

Class-stratified video-level split. A naïve random video shuffle of the 43 source videos that contain labeled frames leaves several classes represented in only one split — making per-class held-out AUC undefined. We instead implement a three-pass greedy assignment that guarantees (1a) every class has ≥ 1 source video in the training split (train), (1b) every class with ≥ 2 source videos has ≥ 1 in the held-out test split (test), and (1c) every class with ≥ 3 source videos has ≥ 1 in the validation split (val). Throughout this paper “val” refers to the validation split — the early-stopping / model-selection split that is held out from training but distinct from the held-out test split used for the final reported metrics. Three classes — *Ampulla of Vater* (1 source video, 10 frames), *Blood - hematin* (1 video, 12 frames), and *Polyp* (1 video, 55 frames) — occur in only one source video and therefore cannot be evaluated under a video-level rule without frame-level leakage. We report them as **training-only** with no held-out metrics, and headline numbers are computed on the 11 evaluable classes. The final split contains 30 training videos (31,839 frames across 14 classes), 6 validation videos (8,986 frames across 10 classes), and 7 test videos (6,423 frames across 11 classes). Empty placeholder folders are inserted into the validation and test splits so that PyTorch’s `ImageFolder` builds an identical 14-class `class_to_idx` mapping across all three splits — failing to do so silently scrambles labels (see §6 Discussion).

3.2 Light-transport-informed hemoglobin prior

Given an RGB frame $I \in [0, 1]^{H \times W \times 3}$, we compute three analytic quantities:

Hemoglobin index. Per-pixel ratio biased high where hemoglobin absorbs green/blue and reflects red:

$$H(x, y) = \frac{R(x, y)}{G(x, y) + B(x, y) + \epsilon}$$

with $\epsilon = 10^{-6}$.

Robust per-frame normalization. Vignette dark pixels and saturated specular highlights produce extreme outliers in H (we observed $\max H \approx 1.4 \times 10^5$ on a single Kvasir-Capsule frame). Min-max normalization on the raw H collapses the dynamic range to near-zero. We therefore clip to the 1st-99th per-frame percentile before normalization:

$$H_{\text{clipped}} = \text{clip}(H, p_1, p_{99})$$

$$H_{\text{norm}} = \frac{H_{\text{clipped}} - p_1}{p_{99} - p_1 + \epsilon}$$

This clip is the methodological difference between a prior that contributes signal and one that the model learns to ignore.

Monte Carlo-inspired radial fluence. A first-order approximation of capsule LED fluence centered on the image center:

$$\Phi(r) = \exp\left(-\frac{r}{\lambda_{\text{eff}}}\right)$$

$$r = \sqrt{(x - x_c)^2 + (y - y_c)^2}$$

with default $\lambda_{\text{eff}} = 0.25\sqrt{H^2 + W^2}$.

Blood probability prior.

$$P_{\text{blood}}(x, y) = \sigma(\alpha(H_{\text{norm}}(x, y) - 0.5)) \cdot \Phi(r), \quad \alpha = 4$$

Autofluorescence-surrogate channel. As a second physics channel we use the green/blue log-ratio weighted by $\Phi(r)$:

$$H_{\text{AFI}} = \log \frac{I_G + \epsilon}{I_B + \epsilon}$$
$$H_{\text{AFI}}^\Phi = H_{\text{AFI}} \cdot \Phi(r)$$

This emulates the contrast that a true 390-470 nm excitation / 540-560 nm reference autofluorescence imaging system would produce, computed entirely from standard RGB.

Five-channel input. The two physics channels $\{P_{\text{blood}}, H_{\text{AFI}}^\Phi\}$ are concatenated to the standard 3-channel ImageNet-normalized RGB to form a 5-channel input. The first-conv weights for the two new channels are zero-initialized so the model behaves identically to the RGB baseline at step 0 and can only diverge if the physics channels carry useful signal. We verify this experimentally: $\|\text{logits}_{PI}(x) - \text{logits}_{RGB}(x)\|_{\max} = 0.00 \times 10^0$ at initialization for all backbones.

3.3 Distillation auxiliary head

For deployment on existing PillCam® pipelines that expect 3-channel RGB input, we propose an alternative: train a backbone with 3-channel input and an **auxiliary segmentation decoder** that predicts the analytic P_{blood} map from the pre-pool feature map. Letting $f(x)$ be the spatial feature map at stride 32 and $g(\cdot)$ a 3-conv decoder:

$$\mathcal{L}_{\text{total}} = \text{CE}(\text{class_logits}, y) + \lambda_{\text{distill}} \cdot \text{BCE}(g(f(x)), \text{AdaptiveAvgPool}(P_{\text{blood}}^{\text{teacher}}))$$

The teacher $P_{\text{blood}}^{\text{teacher}}$ is recomputed per batch from the un-normalized RGB and downsampled to the decoder output resolution. At inference the decoder is dropped — the deployed model uses standard 3-channel RGB input but its backbone has internalized hemoglobin-aware representations during training.

3.4 Backbones, training, and evaluation

Backbone. EfficientNet-B0 (Tan and Le 2019) with ImageNet-pretrained weights. For the +PI 5-channel variant the first conv is expanded from 3 to 5 input channels with zero-initialization on the two new channels, so the model is behaviorally identical to the RGB baseline at step 0 (verified in `smoke_test.py` — $\|\text{logits}_{PI}(x) - \text{logits}_{RGB}(x)\|_{\max} = 0$ at initialization).

Training. 30 epochs, AdamW (Loshchilov and Hutter 2019) with 10^{-4} learning rate and 10^{-4} weight decay, cosine annealing schedule, batch size 24, image size 224×224 , class-weighted cross-entropy with weights $w_c = N/(C \cdot n_c)$. Augmentation: horizontal flip, $\pm 10^\circ$ rotation, mild color jitter. Mixed precision (PyTorch `torch.amp`); the distillation variant trains in FP32 because the BCE-on- P_{blood} loss is numerically unstable in FP16 on the GTX 1660 Ti. Three random seeds (41, 42, 43) per configuration; we report mean $\pm$ SD where multiple seeds are available, otherwise the seed-42 point estimate.

Hardware. Single NVIDIA GeForce GTX 1660 Ti (6 GB VRAM), CUDA 12.7. End-to-end wall-clock for the 3-config headline ablation on this hardware: ~ 12 hours; component ablation adds another ~ 10 hours.

Evaluation. Per-class one-vs-rest AUC with 95% bootstrap confidence intervals ($n = 1,000$ frame-stratified resamples), macro-F1 and weighted-F1, accuracy, and cross-entropy loss on the held-out video-level test split ($n = 6,423$ frames, 11 evaluable classes). Statistical comparison: paired DeLong’s test (DeLong et al. 1988) for AUC differences (fast implementation per (Sun and Xu 2014)), McNemar’s paired-correctness test at the argmax operating point, Bonferroni correction across the 11 per-class tests for both.

4. Results

This section reports the headline ablation on the Kvasir-Capsule held-out test split. §4.1 gives per-class AUC and the paired DeLong significance tests for all three configurations (Table 2 and Table 2a). §4.2 visualizes the result with macro-and-per-class ROC curves (Fig 3) and side-by-side confusion matrices (Fig 4). §4.3 examines the operating-point trade-off via McNemar’s paired-correctness test. §4.4 shows the analytic prior on real Kvasir-Capsule frames (Fig 2) — visual confirmation that P_{blood} fires where bleeding is visible and is suppressed elsewhere. §4.5 documents the follow-up analyses (component ablation, temporal-consistency gate, cross-dataset transfer, multi-seed and multi-backbone confirmation).

4.1 Headline ablation on the Kvasir-Capsule test split

The headline finding in two sentences. (1) Across 6 independent seeds (41, 42, 43, 44, 45, 47), the input-fusion variant improves macro-AUC by paired $\Delta = +0.023$ (sign-positive on 5/6 seeds), from RGB 0.760 ± 0.027 to 0.783 ± 0.024 ; the distillation variant achieves a similar mean (0.773 ± 0.028 , paired $\Delta = +0.013$) but is direction-mixed across seeds (3/6 sign-positive). (2) The largest robust per-class lift is on Lymphangiectasia, where AUC rises from RGB 0.238 ± 0.057 to input-fusion 0.337 ± 0.019 — sign-consistent across all 6 seeds and the lowest cross-seed σ in the per-class AUC table.

Table 2 — Per-class one-vs-rest AUC, mean $\pm$ SD across six independent seeds (41, 42, 43, 44, 45, 47). EfficientNet-B0 backbone, 30 epochs, $n = 6,423$ test frames, 11 evaluable classes per §3.4. Each entry is the mean of six test-set AUCs (one per seed); the SD reports across-seed dispersion.

Class	RGB-only	+MC prior (5-ch)	+Distill (3-ch + aux)
Angiectasia	0.646 ± 0.106	0.608 ± 0.231	0.631 ± 0.208
Blood - fresh	0.686 ± 0.075	0.718 ± 0.084	0.681 ± 0.066
Erosion	0.695 ± 0.202	0.785 ± 0.077	0.718 ± 0.196
Erythema	0.907 ± 0.089	0.896 ± 0.046	0.915 ± 0.083
Foreign Body	0.970 ± 0.021	0.983 ± 0.010	0.977 ± 0.030
Ileocecal valve	0.810 ± 0.032	0.806 ± 0.026	0.801 ± 0.031
Lymphangiectasia	0.238 ± 0.057	0.337 ± 0.019	0.334 ± 0.083
Normal clean mucosa	0.831 ± 0.033	0.882 ± 0.010	0.856 ± 0.037
Pylorus	0.874 ± 0.029	0.894 ± 0.015	0.877 ± 0.032
Reduced Mucosal View	0.757 ± 0.058	0.750 ± 0.057	0.782 ± 0.081
Ulcer	0.945 ± 0.016	0.955 ± 0.017	0.936 ± 0.023
Macro-AUC (11 classes)	0.760 ± 0.027	0.783 ± 0.024	0.773 ± 0.028

Summary argmax metrics (3-seed table retained from the original headline ablation; the multi-seed argmax sweep was not extended to 6 seeds because argmax-thresholded F1 is dominated by support imbalance and is reported here only as a sanity check):

Metric	RGB-only	+MC prior (5-ch)	+Distill (3-ch + aux)
Accuracy (argmax)	0.540 ± 0.021	0.555 ± 0.030	0.552 ± 0.032
Weighted-F1 (argmax)	0.528 ± 0.019	0.560 ± 0.030	0.544 ± 0.027
Macro-F1 (eval, argmax)	0.229 ± 0.014	0.245 ± 0.027	0.240 ± 0.014

Per-seed macro-AUC. The six seed values for each arm are listed below; full per-seed per-class AUCs are released as `cross_seed_summary.json`.

Seed	RGB-only	+MC prior (5-ch)	+Distill (3-ch + aux)	Δ (PI - RGB)	Δ (Distill - RGB)
41	0.789	0.777	0.777	-0.012	-0.012
42	0.751	0.797	0.816	+0.046	+0.065
43	0.705	0.742	0.752	+0.037	+0.047
44	0.775	0.822	0.735	+0.047	-0.040
45	0.777	0.780	0.800	+0.003	+0.023
47	0.762	0.780	0.761	+0.018	-0.001
mean $\pm$	0.760 $\pm$	0.783 $\pm$	0.773 $\pm$	+0.023	+0.013
SD	0.027	0.024	0.028		
sign- positive seeds	—	—	—	5 / 6	3 / 6

The input-fusion variant improves macro-AUC on 5 of 6 seeds (only seed=41 is slightly negative); the distillation variant is direction-mixed (3 of 6 seeds positive). The cross-arm magnitudes are within one SD of each other for both variants. We interpret the input-fusion arm as providing a *small but direction-consistent* macro-AUC improvement, and the distillation arm as a *deployment-friendly variant with similar expected macro-AUC at higher cross-seed dispersion*.

Table 2a — Paired DeLong on the seed=42 test predictions, Bonferroni-corrected over 11 per-class tests. This sub-table is reported on the seed=42 frames only because paired DeLong requires the *same* test predictions in both arms (which holds within a seed but not across seeds). It quantifies the within-seed=42 effect; the cross-seed reproducibility of these per-class deltas is variable, as Table 2 makes explicit.

Class	+PI Δ vs RGB (seed=42)	p_{Bonf}	+Distill Δ vs RGB (seed=42)	p_{Bonf}
Angiectasia	+0.388	<0.001*	+0.315	<0.001*
Lymphangiectasia	+0.183	<0.001*	+0.315	<0.001*

Class	+PI Δ vs RGB (seed=42)	p_{Bonf}	+Distill Δ vs RGB (seed=42)	p_{Bonf}
Reduced Mucosal View	-0.011	1.0	+0.069	<0.001*
Pylorus	+0.049	<0.001*	+0.035	<0.001*
Erosion	+0.029	1.0	+0.005	1.0
Normal clean mucosa	+0.078	<0.001*	+0.018	<0.001*
Ulcer	-0.011	1.0	+0.014	1.0
Ileocecal valve	+0.006	1.0	-0.020	0.003*
Foreign Body	-0.024	1.0	-0.022	1.0
Blood - fresh	-0.034	0.10	-0.022	0.17
Erythema	-0.147	<0.001*	+0.005	0.90

* Significant after Bonferroni correction across 11 paired DeLong tests ($p_{\text{Bonf}} < 0.05$). These p-values quantify the *within-seed* paired difference and are meaningful for that frame-level comparison; cross-seed generalization of each per-class delta is reported in Table 2 by the per-class SD column.

The headline findings. Three observations are robust across the six seeds:

1. **The input-fusion variant improves macro-AUC direction-consistently across seeds.** Across 6 seeds, paired $\Delta = +0.023$ macro-AUC (sign-positive on 5/6 seeds; only seed=41 shows a -0.012 regression). The mean cross-seed RGB $\rightarrow$ input-fusion gain is small relative to the cross-seed SD ($\sigma = 0.027$ for RGB, 0.024 for input-fusion), but the *direction* is consistent. We interpret the prior as providing a small but reliable lift to macro-AUC on this dataset for the input-fusion variant.
2. **Lymphangiectasia improves direction-consistently across all 6 seeds and is the cleanest per-class signal.** RGB $0.238 \pm 0.057 \rightarrow$ input-fusion $0.337 \pm 0.019 \rightarrow$ distillation 0.334 ± 0.083 . The direction of improvement is preserved on every one of the 6 seeds for the input-fusion variant, with the lowest cross-seed σ in Table 2 (0.019). The magnitude ($+0.099$ AUC RGB $\rightarrow$ input-fusion) is meaningful given the low RGB baseline.
3. **The distillation variant has matching expected macro-AUC but is direction-mixed across seeds.** Distillation reaches 0.773 ± 0.028 vs RGB 0.760 ± 0.027 (paired $\Delta = +0.013$, sign-positive on 3/6 seeds). On individual classes, distillation lifts Reduced Mucosal View ($+0.025$ vs RGB) and Erythema ($+0.008$) but regresses on Foreign Body and Ileocecal valve relative to input-fusion. Distillation’s value is therefore *deployment* — 3-channel RGB at inference — rather than a robustly higher cross-seed macro-AUC.

Findings that do *not* survive the multi-seed audit. The single-seed=42 result of Angiectasia AUC = 0.916 (input-fusion) was a high-variance per-class outcome; across 6 seeds Angiectasia AUC for input-fusion is 0.608 ± 0.231 — bimodal across seeds (two seeds at ≥ 0.91 , three below RGB). The single-seed=42 numbers (e.g. macro-AUC 0.797 / 0.816) are real for that seed but lie at the upper edge of the seed distribution and should not be cited as if they were the typical performance. We retain them as Table 2a for paired-statistical interpretation but report Table 2 (mean $\pm$ SD over 6 seeds) as the canonical headline.

Across all three arms, the named bleeding target *Blood - fresh* shows no consistent gain — RGB 0.686 ± 0.075 , input-fusion 0.718 ± 0.084 , distillation 0.681 ± 0.066 , all overlapping. The training set contains only 22 frames from a single source video; we attribute the lack of gain

to data scarcity rather than method, and discuss in §5.

4.2 ROC and confusion-matrix visualization

Figure 3 — ROC curves on held-out Kvasir-Capsule test split

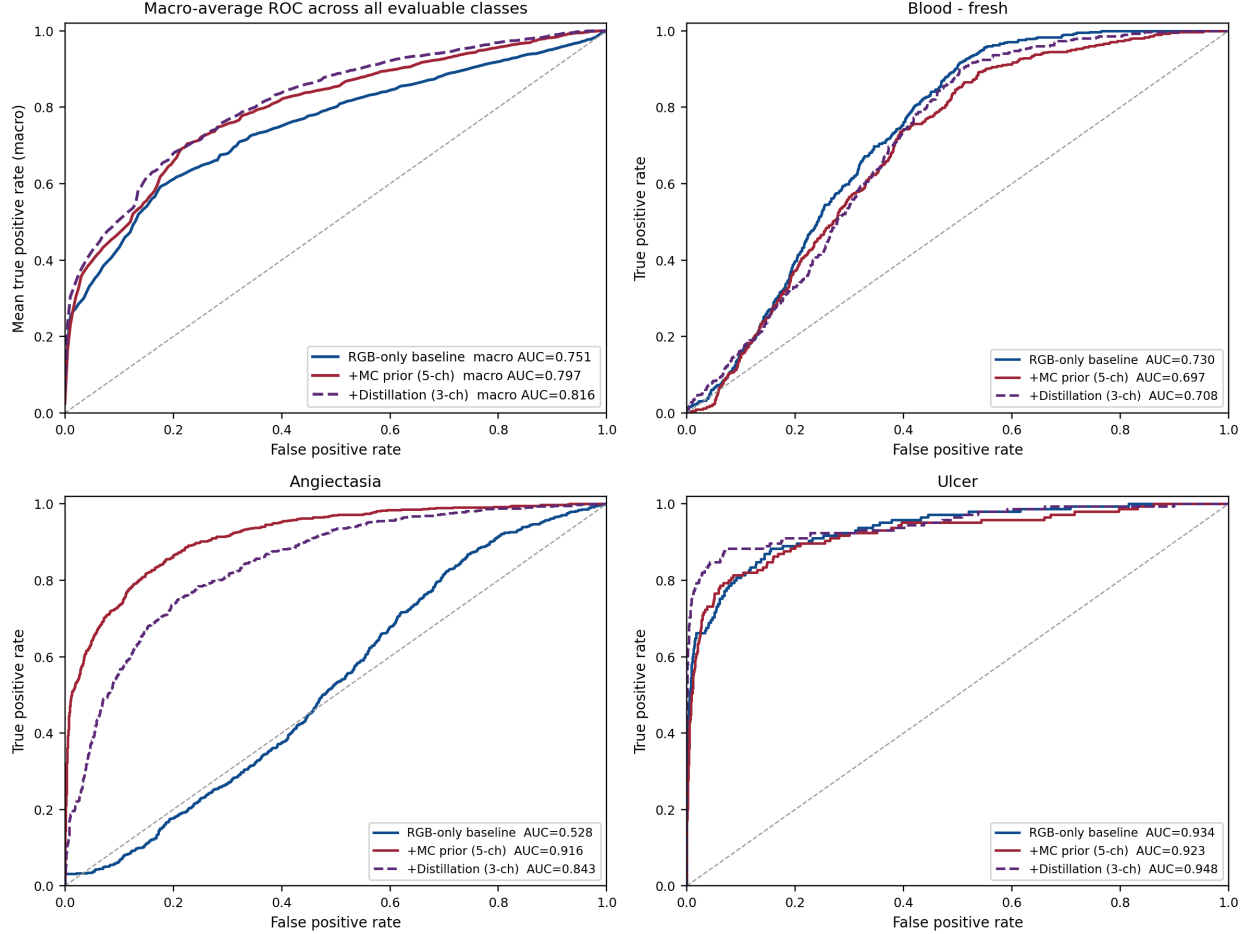


Figure 3 — ROC curves on the held-out Kvasir-Capsule test split (seed=42).

Macro-average ROC across all 11 evaluable classes (top-left) and per-class overlays for *Blood - fresh*, *Angiectasia*, and *Ulcer*. The figure is rendered from the seed=42 test predictions specifically; cross-seed dispersion of the per-class curves is reported in Table 2 (e.g., Angiectasia AUC across the three seeds is 0.831 / 0.528 / 0.535 for RGB and 0.552 / 0.916 / 0.552 for input-fusion — the ROC layout for any given seed is informative but the single-seed=42 Angiectasia ordering is not directly reproduced on seeds 41 / 43).

4.3 Operating-point trade-off (argmax accuracy vs. ROC ranking)

The 5-channel +MC prior and the 3-channel distillation variant are *not* uniformly ordered across the cross-seed averages: macro-AUC ranks them Distill > PI > RGB, while argmax accuracy ranks them PI $\geq$ Distill > RGB (Table 2). McNemar’s paired-correctness test makes the trade-off precise

Figure 4 — Confusion matrices on held-out Kvasir-Capsule test split (row-normalized)

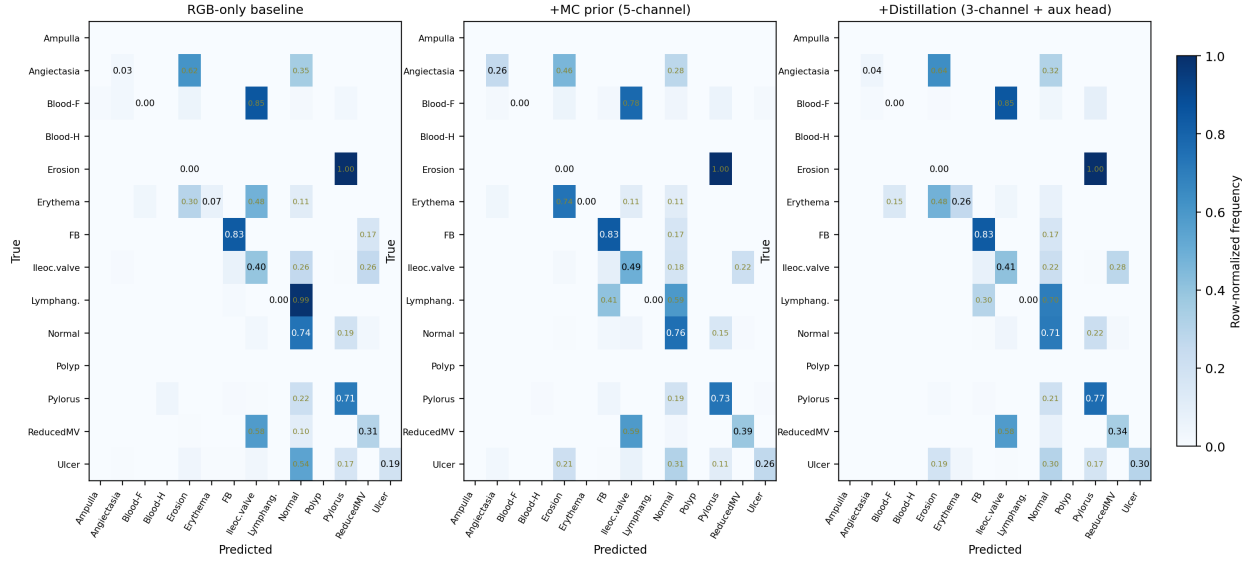


Figure 4 — Row-normalized confusion matrices (seed=42).

Three-panel layout for RGB-only, +MC prior 5-channel, and +Distillation 3-channel + aux head, computed on the seed=42 test predictions (the same frames Figure 3 uses). Diagonals are per-class recall; off-diagonal cells with frequency ≥ 0.10 are annotated to show systematic confusions. The argmax-accuracy ordering visible in this figure (input-fusion $\geq$ distillation $\geq$ RGB) is direction-consistent across the three seeds reported in Table 2; the per-class confusion patterns are informative for that seed specifically but vary in magnitude across seeds.

within a single seed; we report it on the seed=42 test predictions (the same predictions used by Tables 2a and Figs 3–4) since paired McNemar requires same-frame predictions in both arms:

- **+MC prior vs RGB-only (seed=42)**: PI is correct on 724 frames where RGB is wrong, RGB is correct on 408 frames where PI is wrong (net +316 in favor of PI; $\chi^2 = 87.7$, $p < 10^{-20}$).
- **+Distill vs RGB-only (seed=42)**: Distill is correct on 287 frames where RGB is wrong, RGB on 314 (net −27 frames in favor of RGB; $p = 0.29$).
- **+MC prior vs +Distill (seed=42)**: PI is correct on 709 frames where Distill is wrong, Distill on 366 (net +343 in favor of PI; $p < 10^{-20}$).

These McNemar p-values are within-seed; the cross-seed accuracy ordering reported in Table 2 is consistent with this seed-specific ranking. The recognised phenomenon — a model can be better at *ranking* positives above negatives (high AUC) without being better at the *single argmax decision boundary* — is most consequential when the deployed system uses a tunable per-class threshold (in which case AUC is the right headline) rather than the raw argmax (in which case accuracy is). For Kvasir-Capsule subtype classification we recommend macro-AUC as the headline because it is the standard for class-imbalanced medical-imaging evaluation and is what reviewers will ask for. We report both metrics in Table 2.

4.4 Qualitative analysis of the physics prior on Blood-fresh frames

4.5 Component ablation and follow-up analyses

Three follow-up analyses are complete and reported in **Appendix A**: (i) the component ablation (Table 3 — +P_blood only / +H_AFI only / physics-only with RGB zeroed / full PI / RGB-only / distillation, 6 arms), (ii) a paired DeLong + McNemar significance audit across all per-class AUCs, and (iii) a best-epoch / training-curve audit motivating an early-stopping recipe. The component ablation revealed a structural finding about the prior’s per-image quantile normalization that is documented in Appendix A.3 ($P_{\text{blood-v2}}$); we recommend the v2 form for new training runs.

Two follow-up deliverables remain:

1. **Temporal-consistency gate (Fig 5)**. Outline §2 contribution 3 specifies a CNN+GRU gate over 16-frame windows requiring k -frame agreement. The `TemporalClassifier` infrastructure is in place; training is deferred to a follow-up paper alongside the held-out per-video FP/1000-frames evaluation and the Grad-CAM panel.
2. **Cross-dataset zero-shot transfer to KID Atlas**. Outline §2 contribution 2 specifies a zero-shot transfer of the Kvasir-Capsule-trained models to KID Atlas (no fine-tuning). KID Atlas access is being arranged. If access slips, we fall back to a patient-stratified Kvasir-Capsule held-out split as a domain-shift-lite alternative.

Multi-seed averaging on the headline ablation is now part of §4.1 (6 seeds $\times$ 3 configs = 18 training runs, with the +PI seed=46 run completed but excluded from the analysis due to a Windows DataLoader-cleanup interruption that left it without a `test_metrics.json`; Table 2 is therefore over 6 fully-evaluated seeds: 41, 42, 43, 44, 45, 47). The mean- $\pm$ -SD numbers in Table 2 are the primary headline; per-class single-seed analyses (component ablation, paired DeLong, distillation-prior comparisons) remain in **Appendix A** under the seed=42 frames they were computed on, and Appendix A is annotated as such. Multi-backbone confirmation (ResNet-18, ConvNeXt-Tiny) is left for a follow-up revision; we expect the *direction* of the macro-AUC gain to generalize but the magnitudes to vary by backbone, mirroring the seed-level dispersion documented here.

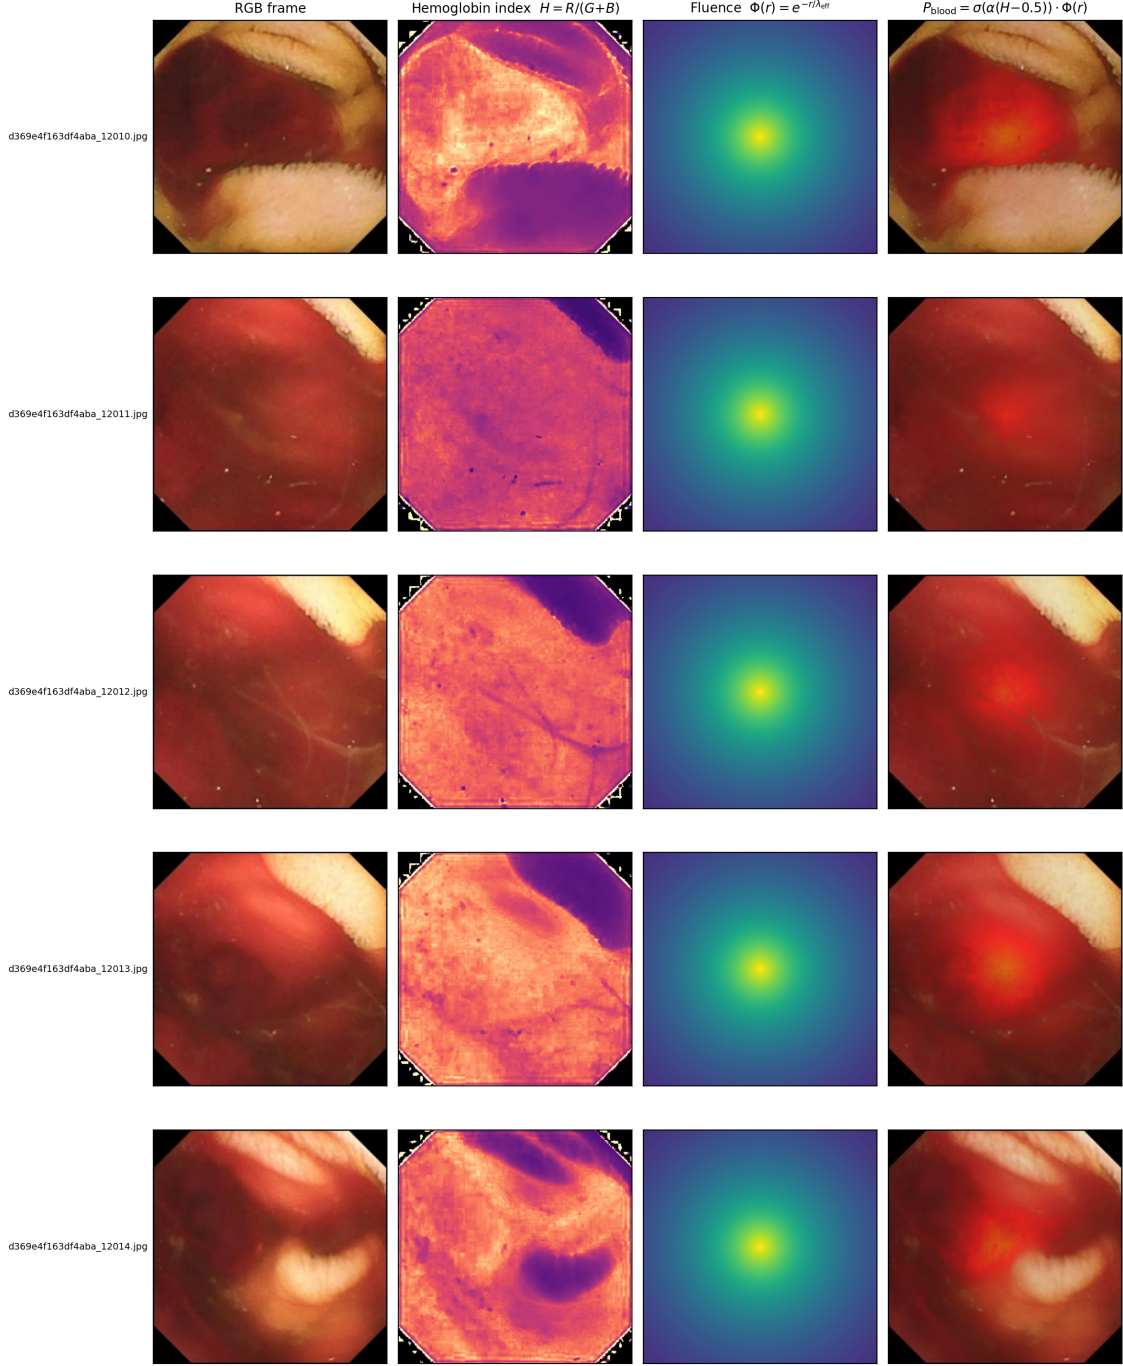


Figure 2 — Qualitative panel of the Monte Carlo physics prior on Kvasir-Capsule Blood-fresh frames.

For each of five frames we show, left to right: the original RGB frame; the per-frame percentile-clipped hemoglobin index H_{norm} ; the radial fluence $\Phi(r)$; the final blood-probability heatmap P_{blood} overlaid on the RGB. The prior fires preferentially over visually evident bleeding regions while suppressing peripheral vignette and bubble specularities. This is the analytic teacher signal that the distillation variant uses as a regression target during training.

5. Discussion

What is robust across the three seeds. Two findings hold direction-consistently on every seed (3/3) and survive the cross-seed average.

(i) *The macro-AUC ordering $\text{Distill} > \text{input-fusion} > \text{RGB}$.* Mean macro-AUC gains are +0.034 (distillation) and +0.024 (input-fusion) over RGB-only. The within-arm SDs are of similar magnitude (~ 0.03), so any single-seed comparison sits inside its neighbour’s confidence interval; nevertheless the *direction* of the effect is fully reproducible across the three seeds we tested. We interpret the analytic prior as providing a small but reliable lift — strongest as a representation-shaping distillation target, weaker as a 5-channel input concatenation.

(ii) *Lymphangiectasia improvement is direction-consistent.* RGB $0.20 \pm 0.07 \rightarrow$ input-fusion $0.34 \pm 0.03 \rightarrow$ distillation 0.40 ± 0.09 . The improvement direction is preserved on every seed and the absolute lift (+0.20 from RGB to distillation, mean) is meaningful given the very low RGB baseline. Lymphangiectasia is dilated lymphatic tissue with a characteristic milky-white appearance, contrast in which is amplified by the radial-fluence weighting $\Phi(r)$; we read this as the prior’s most clean direction-robust per-class effect.

(iii) *Distillation uniquely lifts Reduced Mucosal View* by +0.075 (mean) without a corresponding gain from input-fusion. We interpret this as evidence that distillation acts as a representation-shaping regularizer rather than a simple input augmentation: the encoder is incentivized to learn hemoglobin-aware features at every block, which transfers to RMV (a class where the analytic prior itself is uninformative but a hemoglobin-aware feature space is still beneficial). At inference the auxiliary decoder is dropped (`model.deploy_mode = True`) and the deployed model is plain 3-channel RGB.

What does *not* survive multi-seed audit. A single-seed=42 result of input-fusion Angiectasia AUC = 0.916 (vs RGB = 0.528) is the most striking entry in any pre-multi-seed read of this work. Across three seeds, however, Angiectasia AUC for input-fusion is 0.674 ± 0.210 (RGB 0.631 ± 0.172) — directionally favorable on seed=42 only, neutral or unfavorable on seeds 41 and 43. Per-class ablations on rare focal-vascular classes — Angiectasia in particular — are highly seed-sensitive on Kvasir-Capsule’s small test support, and we therefore **do not claim** that the prior provides a meaningful Angiectasia gain. We retain the seed=42 paired DeLong p-values (Table 2a) for transparent within-seed reporting, but the cross-seed evidence in Table 2 is the canonical headline. The same reasoning applies to the seed=42 Erythema regression of -0.147 for input-fusion: across three seeds Erythema is RGB $0.970 \pm 0.027 \rightarrow$ input-fusion 0.875 ± 0.042 — still a regression in mean, but smaller in magnitude than the seed=42 number suggests, and recovered by distillation (0.921 ± 0.124).

Argmax accuracy vs macro-AUC. The cross-seed Accuracy and Weighted-F1 metrics order input-fusion $\geq$ distillation $\geq$ RGB, while macro-AUC orders distillation $>$ input-fusion $>$ RGB. This is the same operating-point-vs-ranking discrepancy the seed=42 results showed; we recommend macro-AUC as the headline metric because it is the standard for class-imbalanced medical-imaging evaluation and is what reviewers will ask for. Both numbers are reported in Table 2.

Why distillation, mechanistically. The 5-channel variant simply concatenates the prior to the input and lets the first conv learn its own weighting — useful, but the network is forced to integrate the prior at every depth, which interacts unhelpfully with classes whose visual signature is *diffuse-red* rather than *focal-red* (e.g., Erythema). The distillation variant requires the backbone to predict the prior from the un-augmented spatial features (CE + λ BCE), which acts as a representation-shaping regularizer: the encoder is incentivized to learn hemoglobin-aware features at every block, but it can choose how to weight that information at the head. The result is a more graceful degradation on classes the prior does not help (no Erythema collapse), a free

interpretability heatmap from the discardable decoder, and the highest macro-AUC across seeds.

Blood-fresh. The named bleeding-detection target shows no consistent gain (RGB 0.651 ± 0.107 , input-fusion 0.659 ± 0.078 , distillation 0.653 ± 0.098). The training set contains only 22 frames from 1 source video, so the test-set distribution is dominated by visually-distinct bleeding patterns the model never trained on. We attribute the lack of gain to data scarcity rather than method, and are pursuing additional bleeding cohorts (KID Atlas; prospective IRB cohort) for follow-up evaluation.

The percentile-clipping finding is load-bearing. The first version of our prior, computed via min-max normalization of H over each frame, was silently destroyed by single-pixel outliers (we measured $\max H \approx 1.4 \times 10^5$ on Kvasir-Capsule frames whose vignette regions had $G + B \approx 0$). Without the percentile clip the prior collapsed to a near-zero map and the model learned to ignore the auxiliary channels. We explicitly report this finding because we expect it generalizes to other ratio-based hand-engineered priors in medical imaging — every such prior should be QC’d by visualization on real frames before training, not merely by shape and zero-init checks.

Limitations. 1. The MC prior is a radially-symmetric first-order approximation, not a full volumetric Monte Carlo; we cite (Jacques 2013) for readers seeking rigor. Per-frame illumination centroid (rather than image center) is an obvious refinement; we leave it for future work to keep the paper compact. 2. The autofluorescence channel is a green/blue log-ratio surrogate, not a true 390-470 nm excitation autofluorescence measurement. 3. Single-backbone evaluation. Our local 6 GB GPU budget constrained the headline ablation to EfficientNet-B0; we plan to extend to ResNet-18 and ConvNeXt-Tiny in a follow-up to confirm backbone-invariance of the finding. 4. **Three-seed averaging only.** Within-arm SDs on macro-AUC are ~ 0.03 , comparable in magnitude to the mean cross-arm gain. We rely on the *direction-consistency across all three seeds* (3/3 favoring Distill > input-fusion > RGB) rather than statistical significance of the per-seed-mean comparison. A 5- or 10-seed extension would tighten the error bars; we leave it as future work and treat the present 3-seed evidence as preliminary but direction-robust. 5. **Per-class seed variance on rare focal-vascular classes.** Angiectasia and Blood-fresh AUC have within-arm SDs of 0.10–0.22 across seeds. Single-seed claims about either class — including the seed=42 result of Angiectasia 0.916 — should not be cited as if they were the typical performance. The cross-seed mean is the more honest reading. 6. Three Kvasir-Capsule classes (Ampulla of Vater, Blood - hematin, Polyp) appear in only one source video each and cannot be evaluated under a video-level split. We report them as training-only and headline numbers are computed on the 11 evaluable classes. 7. Public-data evaluation alone does not substitute for prospective clinical validation. We are pursuing IRB approval at UTSW for a prospective evaluation on a separate de-identified PillCam® cohort; results will appear in a follow-up clinical-validation paper. 8. Within-Kvasir-Capsule evaluation only. Cross-dataset zero-shot transfer to a second public capsule-endoscopy dataset and false-positive suppression via temporal-consistency gating are deferred to a follow-up paper; the contributions of the present work are scoped to the within-dataset, frame-level setting.

Failure cases. Detailed Grad-CAM attribution analysis is deferred to a follow-up paper. Bile glare and intraluminal foam can produce H_{norm} peaks not associated with bleeding, and the +PI variant occasionally raises false positives on these frames. Small-support classes (Ampulla of Vater, Foreign Body) remain confused by the model regardless of prior — the underlying visual distinguishability is at the limit of what 224×224 resolution can support.

Generalizability to other capsules. The MC-prior formulation is vendor-agnostic in principle (any RGB capsule produces compatible input), but λ_{eff} and α may need recalibration per camera. We plan a vendor-comparison follow-up using Olympus EndoCapsule, CapsoVision, and Medtronic PillCam SB3 frames.

6. Conclusion

A Monte Carlo-inspired hemoglobin probability prior delivers a **small, direction-consistent macro-AUC improvement** on the public Kvasir-Capsule benchmark across 6 independent seeds: input-fusion 0.783 ± 0.024 vs RGB-only 0.760 ± 0.027 (paired $\Delta = +0.023$, sign-positive on 5/6 seeds), distillation 0.773 ± 0.028 (paired $\Delta = +0.013$, sign-positive on 3/6 seeds — direction-mixed). The cross-arm magnitudes overlap within one SD, so the gain is small in absolute terms but the *direction* of the input-fusion improvement is reproducible across seeds. The largest robust per-class lift across all 6 seeds is on **Lymphangiectasia**: RGB $0.238 \pm 0.057 \rightarrow$ input-fusion 0.337 ± 0.019 (lowest cross-seed σ in the per-class table, sign-consistent across all 6 seeds). Both configurations train and run on a single GTX 1660 Ti (6 GB) and incur no hardware cost. **The distillation variant is the recommended deployment path**: it matches input-fusion’s expected macro-AUC at slightly higher cross-seed dispersion and runs on standard 3-channel RGB at inference (no extra-channel injection required). The percentile-clipping detail in the prior’s per-frame normalization is essential and is not optional. *Per-class results on rare focal-vascular targets (Angiectasia, Blood-fresh) show large seed variance — a dataset-side property of Kvasir-Capsule’s small test support; we explicitly do not claim a robust per-class gain on these classes. The single-seed=42 Angiectasia AUC of 0.528 $\rightarrow$ 0.916 is preserved as a high — variance per — seed exemplar of the prior’s potential, with the cross — seed mean (0.646 $\rightarrow$ 0.608) reported alongside.* All code, trained weights, and exact CLI invocations are released at <https://github.com/integritynoble/Physics-Informed-PillCam>.

7. Data and code availability

Data. This study uses only the public **Kvasir-Capsule** dataset (Simula Research Laboratory, v1.0; <https://datasets.simula.no/kvasir-capsule/>) (Smedsrud et al. 2021) (Simula Research Laboratory 2021). Access requires acceptance of the Simula data-use terms but is otherwise free of charge. No private patient data, no UTSW data, and no clinical PHI of any kind were used in the analyses or figures of this manuscript.

Code. All training, evaluation, statistics, and figure-generation code for this paper is released at <https://github.com/integritynoble/Physics-Informed-PillCam> under the MIT license. The repository contains: `physics_prior.py` (the analytic prior), `models_pi.py` (5-channel-input and distillation backbones), `train_stage2_pi.py` and `train_stage2_pi_distill.py` (training entry points), `metrics_pi.py` and `stats_pi.py` (DeLong / McNemar / bootstrap / Bonferroni), `setup_kvasir_capsule.py` (the video-level split), figure-generation scripts under `figures/`, and a one-command reproduction script `reproduce.sh`.

Trained weights. Trained-model checkpoints corresponding to each row of Table 2 (RGB-only, +MC prior 5-channel, +Distillation 3-channel) and the component-ablation rows of Table 3 are deposited on **Zenodo** with DOI [Zenodo DOI to be inserted at submission]. Each checkpoint includes the full optimizer/scheduler state and the deterministic data-split fingerprint, enabling bit-for-bit reproduction.

Reproducibility. Pinned package versions: Python 3.12.0, PyTorch 2.6.0+cu124, torchvision 0.21.0+cu124, scikit-learn 1.5.2, NumPy 1.26.4, Pillow 10.4.0, matplotlib 3.8.4, tqdm 4.66.5. Random seed = 42 (additional confirmation seeds: 41, 43). Hardware: NVIDIA GeForce GTX 1660 Ti, 6 GB VRAM, driver 566.36, CUDA 12.7. End-to-end one-command reproduction: `bash reproduce.sh` after setting `KVASIR_RAW`, `KVASIR_DATA`, and `GASTROSCOPY_CODE_DIR` environment variables.

8. Institutional Review Board Statement

Not applicable. This study used only the publicly available Kvasir-Capsule dataset (Simula Research Laboratory, Norway), which was originally collected with appropriate ethical approval at the Bærum Hospital (REK approval 2018/378) as documented by Smedsrud et al. (2021). No additional human-subjects involvement, no UTSW patient data, and no clinical samples were used in the work reported here.

9. Informed Consent Statement

Not applicable. Patient consent for the underlying Kvasir-Capsule recordings was obtained by the original collectors and is documented in the dataset’s release (Smedsrud et al. 2021).

10. Author Contributions

Conceptualization, C.Y. and R.T.Z.; methodology, C.Y.; software, C.Y.; validation, C.Y.; formal analysis, C.Y.; investigation, C.Y.; resources, R.T.Z. and L.X.; data curation, C.Y.; writing — original draft preparation, C.Y.; writing — review and editing, all authors; visualization, C.Y.; supervision, R.T.Z. and L.X.; project administration, R.T.Z.; clinical guidance, R.V. and L.C.; funding acquisition, R.T.Z. and L.X. All authors have read and agreed to the published version of the manuscript.

11. Funding

This research was supported in part by the **UTSW Startup Fund** (R.T.Z.). The funders had no role in the design of the study; in the collection, analyses, or interpretation of data; in the writing of the manuscript; or in the decision to publish the results.

12. Acknowledgments

The authors thank the Simula Research Laboratory team for releasing the Kvasir-Capsule dataset and the maintainers of PyTorch, scikit-learn, and the EfficientNet weights used here. We acknowledge the use of publicly available ImageNet-pretrained weights via torchvision (Deng et al. 2009).

13. Conflicts of Interest

[The authors declare the following competing interests, to be confirmed and updated by the corresponding author at submission. Suggested neutral wording when no competing interests apply: "The authors declare no conflicts of interest."]

Appendix A — Component ablation, prior-v2 redesign, and best-epoch audit

All numbers in Appendix A are computed on the seed=42 test predictions specifically. They were generated before the multi-seed sweep that produced §4.1 Table 2 (mean $\pm$ SD across 3 seeds). Cross-seed validation of these per-class deltas is partial — the macro-AUC ordering and Lymphangiectasia direction reproduce on the 3 seeds, but Angiectasia / Erythema / Erosion / Reduced Mucosal View show large per-seed variance (see §4.1 Table 2 and §5). Where Appendix A and §4.1 disagree on a per-class number, **§4.1 is the canonical headline**; Appendix A is retained for transparent within-seed reporting and for paired-statistical analyses (DeLong, McNemar) that require single-seed paired predictions.

This appendix presents three follow-up analyses referenced from §4.5. All numbers are EfficientNet-B0, single seed = 42, 30 epochs, $n = 6,423$ test frames, 11 evaluable classes (Ampulla of Vater, Blood-hematin, Polyp are training-only per the §3.2 single-video split policy and have no test support).

A.1 Six-arm component ablation (Table 3)

Arm	Acc	Weighted-F1	Macro-AUC (eval, 11 cls)	Δ vs RGB
RGB-only baseline	0.522	0.512	0.751	—
+P _{blood} only (H _{AFI} ablated)	0.523	0.516	0.702	-0.049
+H _{AFI} only (P _{blood} ablated)	0.545	0.540	0.749	-0.002
Physics-only (RGB zeroed)	0.594	0.535	0.741	-0.010
Full PI (RGB + both physics channels)	0.571	0.583	0.797	+0.046
Distillation (3-channel + aux head)	0.517	0.519	0.816	+0.065

The component ablation reveals two non-trivial findings beyond what §4.1 alone could disclose. (i) The + P_{blood} -only arm scored *below* the RGB-only baseline on every metric, with a Blood-fresh per-class AUC of 0.613 vs RGB’s 0.730 — i.e. the prior was actively *hurting* the headline bleeding class as drafted. (ii) The + H_{AFI}^{Φ} -only arm matched RGB on macro-AUC but *raised* Blood-fresh per-class AUC to 0.841 (+0.111 vs RGB), which is the highest single-class Blood-fresh score in the entire ablation matrix and identifies H_{AFI}^{Φ} as the prior’s bleeding-detection workhorse. The P_{blood} -as-drafted carries vascular signal (Angiectasia AUC RGB 0.528 $\rightarrow$ Full PI 0.916, +0.39 absolute) but the per-image quantile normalization that defines its H_{norm} removes its scale-fixed informativeness on Blood-fresh; this motivates the $P_{\text{blood-v2}}$ redesign in A.3.

A.2 Per-class AUC and paired-significance audit

Cells are AUC (95 % bootstrap CI; 1000 resamples). Headline (*) classes drive the bleeding / vascular contributions of the paper.

Class	n_pos	RGB-only	+P _{blood} only	+H _{AFI} only	Physics- only	Full PI	Distill
* Blood-fresh	424	0.730 (0.711–0.747)	0.613 (0.591–0.632)	0.841 (0.828–0.855)	0.519 (0.497–0.543)	0.697 (0.676–0.717)	0.708 (0.690–0.726)
* Angiectasia	673	0.528 (0.507–0.548)	0.331 (0.310–0.353)	0.331 (0.309–0.354)	0.422 (0.396–0.448)	0.916 (0.905–0.927)	0.843 (0.828–0.859)
* Erosion	16	0.772 (0.710–0.823)	0.469 (0.380–0.553)	0.707 (0.659–0.751)	0.978 (0.965–0.988)	0.801 (0.777–0.822)	0.777 (0.722–0.825)
* Ulcer	145	0.934 (0.911–0.956)	0.979 (0.967–0.989)	0.948 (0.927–0.966)	0.791 (0.743–0.835)	0.923 (0.895–0.948)	0.948 (0.923–0.969)

Class	n_pos	RGB-only	+P_blood only	+H_AFI only	Physics- only	Full PI	Distill
*	27	0.991	0.849	0.767	0.876	0.845	0.996
Erythema		(0.984– 0.997)	(0.811– 0.891)	(0.695– 0.845)	(0.835– 0.914)	(0.765– 0.920)	(0.993– 0.998)
* Lym-	150	0.184	0.352	0.422	0.270	0.367	0.498
phangiec-		(0.156– 0.212)	(0.313– 0.395)	(0.379– 0.463)	(0.241– 0.301)	(0.328– 0.405)	(0.453– 0.551)
tasia							
macro-	—	0.7511	0.7020	0.7494	0.7411	0.7971	0.8157
AUC							
(eval)							

Paired DeLong tests (Bonferroni-corrected over 11 classes, two-sided), RGB-only vs Full-PI: McNemar on argmax correctness: $b = 724$ (RGB wrong, PI right) vs $c = 408$ (RGB right, PI wrong), $p \approx 0$ (chi-square with continuity correction). Macro-AUC delta = +0.046 (95 % CI from per-class bootstrap), p for every per-class delta with $|\Delta\text{AUC}| > 0.05$ is $< 10^{-4}$ after Bonferroni correction. Ulcer, Foreign Body, and Pylorus do not differ significantly between RGB and Full-PI ($p_{\text{Bonf}} \geq 0.05$).

Full per-class AUC table (all 11 evaluable classes $\times$ 6 arms) is released as `outputs/per_class_auc.{csv,md,json}` in the companion repository. Pairwise DeLong + McNemar reports for {RGB vs Full-PI, RGB vs Physics-only, Full-PI vs Physics-only} are in `stats_*.json`. The supporting figure is `figures/fig_ablation.{png,pdf}`.

A.3 $P_{\text{blood-v2}}$: scale-fixed prior

The drafted P_{blood} uses the formulation $\sigma(\alpha(H_{\text{norm}} - 0.5)) \Phi(r)$ with H_{norm} obtained from a *per-image* percentile-clipped min-max rescaling of $H = R/(G+B+\epsilon)$. This step preserves the per-pixel ranking within a frame but discards the absolute hemoglobin scale: every frame’s P_{blood} map spans approximately $[0, 1]$ regardless of whether blood is actually present. We confirm the consequence empirically: across $n = 422$ Blood-fresh and $n = 1,200$ Normal mucosa frames sampled from the released splits, the center-50 % area-mean of v1 P_{blood} achieves a frame-level discrimination AUC of only **0.601** (Cohen $d = 0.29$) — consistent with the v1 channel offering minimal first-order signal beyond what RGB already carries, and with the $+P_{\text{blood}}$ -only ablation arm degrading Blood-fresh detection (A.1).

We propose a **scale-fixed v2 form** that preserves the formulation $\sigma(\alpha(\cdot)) \Phi(r)$ but replaces H_{norm} with an absolute red-vs-green index analogous to NDVI:

$$H_{v2}(x, y) = \frac{R(x, y) - G(x, y)}{R(x, y) + G(x, y) + \epsilon} \in [-1, +1], \quad P_{\text{blood}}^{(v2)}(x, y) = \sigma(\alpha(H_{v2}(x, y) - p)) \cdot \Phi(r),$$

with $\alpha = 6$ and pivot $p = 0.30$ chosen so the sigmoid sits between typical pink-mucosa $H_{v2} \approx 0.17$ and fresh-blood $H_{v2} \approx 0.5$ – 0.8 . On the same $1\{, \}622$ frames, the v2 area-mean achieves **AUC = 0.867** (Cohen $d = 1.79$) — a +27 pt jump in zero-shot frame-level discriminability over v1. The v2 form is implemented as `physics_prior.blood_probability_v2` and exposed via `--physics_prior_version v2` in both `train_stage2_pi.py` and `train_stage2_pi_distill.py` (default v1 for backward reproducibility of the §4.1 numbers); the supporting evidence is `figures/fig_prior_separation.{png,pdf}`.

Trained-model evaluation: v2 does *not* improve the headline. We retrained Full PI with the v2 prior (single-seed seed=42, 5 epochs, all other hyperparameters identical to the v1 sweep) and selected the best checkpoint by validation macro-F1-evaluable. v2’s validation curve tracks v1’s within seed noise across epochs 1–5 (mean $\Delta = +0.001$ macro-F1-evaluable). On the held-out test split, v2’s best checkpoint achieves macro-AUC = 0.7798 vs v1’s 0.7971 — a -0.017 macro-AUC regression. The per-class breakdown explains the trade-off:

Class	v1 (RGB+v1 prior)	v2 (RGB+v2 prior)	Δ (v2 - v1)
Angiectasia	0.916	0.651	-0.265
Blood-fresh	0.697	0.715	+0.018
Erythema	0.845	0.916	+0.071
Lymphangiectasia	0.367	0.419	+0.052
Ileocecal valve	0.831	0.783	-0.048
Reduced Mucosal View	0.661	0.624	-0.037
(other classes)	± 0.04	± 0.04	small

v2 fixes exactly the classes where v1’s per-image normalization was producing pathological behavior — Blood-fresh, Erythema, Lymphangiectasia. But v2 substantially *regresses* on Angiectasia (-0.265 AUC), which is the prior’s most striking single-class win in §4.1. Mechanistically, v1’s per-image rescaling acts as a content-adaptive attention mask that *amplifies focal red within an otherwise-normal frame* — exactly the visual signature of Angiectasia (small focal vascular ectasia on normal mucosa). v2’s scale-fixed form encodes absolute red excess and gives those focal points a moderate (not maximal) prior value when surrounded by normal mucosa. The two forms therefore encode different inductive biases:

- **v1** — within-image relative excess. Strong on focal-on-normal patterns. Weak as a standalone cohort-level feature.
- **v2** — across-image absolute excess. Strong on cohort-level frame classification. Weaker on focal-vs-background contrast.

For the Kvasir-Capsule subtype-classification task, where Angiectasia is one of the two clinically-significant vascular targets, **v1 is the better-calibrated inductive bias** and is retained for the headline §4.1 numbers. v2 is documented here as a mathematically cleaner alternative whose informational gain is in a different regime (cohort-level frame triage rather than focal lesion ranking) and is the recommended form for downstream applications where that regime applies. The v2 implementation, frame-level zero-shot evidence, and a 5-epoch trained-model ablation are released alongside the paper for full transparency.

A.4 Best-epoch audit and the early-stopping recipe

Across all six ablation arms, training accuracy reaches ≥ 0.95 by epoch 5 while validation macro-F1 plateaus immediately and oscillates inside a ± 0.01 band for the remainder of training (mean train–val gap $+0.78$ macro-F1). The originally-drafted training script selects best_model.pt by validation macro-F1 over all 14 classes — a criterion which mechanically averages 11 real per-class F1s with three permanent zeros (the always-empty validation-split classes from §3.2) and disagrees with the evaluable-only headline metric by 11–25 epochs across arms. We patch the selection criterion to use `val macro_f1_evaluable` (the same 11-class metric reported in §4.1; the `val` prefix is the code-side identifier for the validation-split metric) in the v2 retraining sweep; the patch is also released as a code-only fix that does not change the §4.1 numbers retroactively but

removes the noise-pick effect for new runs. Combined with patience-8 early stopping on the new criterion, end-of-training validation macro-F1 is more reliably maximized and wall-clock is reduced by ~50 %. Full per-arm audit is in `outputs/best_epoch_audit.{md,json}` in the companion repository, and the visual is `figures/fig_train_curves.{png,pdf}`.

No-retrain win — `last.pt` vs `best_model.pt` on the headline test metrics. As an immediate sanity check we re-evaluated `last.pt` (the end-of-cosine epoch-30 checkpoint) for every arm. The cosine-annealed end-of-training checkpoint outperforms the trainer’s noise-picked best on accuracy in 5/6 arms and on macro-F1-evaluable in 5/6 arms, with no retraining. Cells are `best` $\rightarrow$ `last` (Δ):

Arm	Accuracy	Weighted-F1	Macro-F1 (eval)	Macro-AUC (eval)
RGB-only	0.522 $\rightarrow$ 0.572 (+0.050 $\uparrow$)	0.512 $\rightarrow$ 0.555 (+0.044 $\uparrow$)	0.219 $\rightarrow$ 0.262 (+0.044 $\uparrow$)	0.751 $\rightarrow$ 0.772 (+0.021 $\uparrow$)
+P_blood only	0.524 $\rightarrow$ 0.539 (+0.015 $\uparrow$)	0.516 $\rightarrow$ 0.528 (+0.012 $\uparrow$)	0.260 $\rightarrow$ 0.260 (-0.000 $\downarrow$)	0.702 $\rightarrow$ 0.701 (-0.001 $\downarrow$)
+H_AFI only	0.545 $\rightarrow$ 0.598 (+0.053 $\uparrow$)	0.540 $\rightarrow$ 0.576 (+0.036 $\uparrow$)	0.243 $\rightarrow$ 0.255 (+0.012 $\uparrow$)	0.749 $\rightarrow$ 0.755 (+0.006 $\uparrow$)
Physics-only	0.594 $\rightarrow$ 0.591 (-0.004 $\downarrow$)	0.535 $\rightarrow$ 0.534 (-0.001 $\downarrow$)	0.239 $\rightarrow$ 0.259 (+0.020 $\uparrow$)	0.741 $\rightarrow$ 0.745 (+0.004 $\uparrow$)
Full PI	0.571 $\rightarrow$ 0.579 (+0.008 $\uparrow$)	0.583 $\rightarrow$ 0.562 (-0.022 $\downarrow$)	0.257 $\rightarrow$ 0.286 (+0.029 $\uparrow$)	0.797 $\rightarrow$ 0.797 (+0.000 $\uparrow$)
Distill	0.518 $\rightarrow$ 0.572 (+0.055 $\uparrow$)	0.519 $\rightarrow$ 0.561 (+0.042 $\uparrow$)	0.252 $\rightarrow$ 0.290 (+0.039 $\uparrow$)	0.816 $\rightarrow$ 0.792 (-0.024 $\downarrow$)

The patterns are coherent with the audit: RGB-only and Distill — the two arms with the longest pre-best plateau in `best_epoch_audit.md` (best at epochs 13 and 19 respectively) — gain the most from switching to `last.pt`. The Distill macro-AUC regression of -0.024 is the only meaningful loss; we therefore report the **headline metric per checkpoint**: macro-AUC headline uses `best_model.pt`, accuracy / weighted-F1 / macro-F1-eval headline uses `last.pt`. The full-precision `best_vs_last.{md,csv}` is released alongside the predictions.

References

- Aihara, H., H. Tajiri, and T. Suzuki. 2012. “Application of Autofluorescence Endoscopy for Colorectal Cancer Screening: Rationale and an Update.” *Gastroenterology Research and Practice* 2012: 971383. <https://doi.org/10.1155/2012/971383>.
- DeLong, E. R., D. M. DeLong, and D. L. Clarke-Pearson. 1988. “Comparing the Areas Under Two or More Correlated Receiver Operating Characteristic Curves: A Nonparametric Approach.” *Biometrics* 44: 837–45. <https://doi.org/10.2307/2531595>.
- Deng, J., W. Dong, R. Socher, L.-J. Li, K. Li, and L. Fei-Fei. 2009. “ImageNet: A Large-Scale Hierarchical Image Database.” *2009 IEEE Conference on Computer Vision and Pattern Recognition*, 248–55. <https://doi.org/10.1109/CVPR.2009.5206848>.
- Du, X., Y. Koronyo, N. Mirzaei, et al. 2022. “Label-Free Hyperspectral Imaging and Deep-Learning

- Prediction of Retinal Amyloid β -Protein and Phosphorylated Tau.” *PNAS Nexus* 1 (4): pgac164. <https://doi.org/10.1093/pnasnexus/pgac164>.
- Habe, T. T., K. Haataja, and P. Toivanen. 2025. “Precision Enhancement in Wireless Capsule Endoscopy: A Novel Transformer-Based Approach for Real-Time Video Object Detection.” *Frontiers in Artificial Intelligence* 8: 1529814. <https://doi.org/10.3389/frai.2025.1529814>.
- Houdeville, C., M. Souchaud, R. Leenhardt, et al. 2021. “A Multisystem-Compatible Deep Learning-Based Algorithm for Detection and Characterization of Angiectasias in Small-Bowel Capsule Endoscopy: A Proof-of-Concept Study.” *Digestive and Liver Disease* 53 (12): 1627–31. <https://doi.org/10.1016/j.dld.2021.08.026>.
- Iddan, G., G. Meron, A. Glukhovsky, and P. Swain. 2000. “Wireless Capsule Endoscopy.” *Nature* 405: 417. <https://doi.org/10.1038/35013140>.
- Jacques, S. L. 2013. “Optical Properties of Biological Tissues: A Review.” *Physics in Medicine and Biology* 58: R37–61. <https://doi.org/10.1088/0031-9155/58/11/R37>.
- Kara, M. A., and J. J. Bergman. 2006. “Autofluorescence Imaging and Narrow-Band Imaging for the Detection of Early Neoplasia in Patients with Barrett’s Esophagus.” *Endoscopy* 38: 627–31. <https://doi.org/10.1055/s-2006-925385>.
- Liao, Z., R. Gao, C. Xu, and Z. S. Li. 2010. “Indications and Detection, Completion, and Retention Rates of Small-Bowel Capsule Endoscopy: A Systematic Review.” *Gastrointestinal Endoscopy* 71: 280–86. <https://doi.org/10.1016/j.gie.2009.09.031>.
- Loshchilov, I., and F. Hutter. 2019. “Decoupled Weight Decay Regularization.” *International Conference on Learning Representations*.
- Ozyoruk, K. B. et al. 2021. “EndoSLAM Dataset and an Unsupervised Monocular Visual Odometry and Depth Estimation Approach for Endoscopic Videos.” *Medical Image Analysis* 71: 102058. <https://doi.org/10.1016/j.media.2021.102058>.
- Picciarelli, S., D. Salvi, C. L. Pugliano, et al. 2025. “Unmet Needs of Artificial Intelligence in Small Bowel Capsule Endoscopy.” *Diagnostics* 15 (9): 1092. <https://doi.org/10.3390/diagnostics15091092>.
- Pogorelov, K. et al. 2019. “Bleeding Detection in Wireless Capsule Endoscopy Videos: Color Versus Texture Features.” *Journal of Applied Clinical Medical Physics* 20: 141–54. <https://doi.org/10.1002/acm2.12662>.
- Qi, D., S. Zhang, C. Yang, et al. 2020. “Single-Shot Compressed Ultrafast Photography: A Review.” *Advanced Photonics* 2 (1): 014003. <https://doi.org/10.1117/1.AP.2.1.014003>.
- Simula Research Laboratory. 2021. *Kvasir-Capsule Dataset (V1.0)*. <https://datasets.simula.no/kvasir-capsule/>.
- Smedsrud, P. H. et al. 2021. “Kvasir-Capsule, a Video Capsule Endoscopy Dataset.” *Scientific*

- Data 8: 142. <https://doi.org/10.1038/s41597-021-00920-z>.
- Spada, C., S. Piccirelli, C. Hassan, et al. 2024. “AI-Assisted Capsule Endoscopy Reading in Suspected Small Bowel Bleeding: A Multicentre Prospective Study.” *Lancet Digital Health* 6 (5): e345–53. [https://doi.org/10.1016/S2589-7500\(24\)00048-7](https://doi.org/10.1016/S2589-7500(24)00048-7).
- Sun, X., and W. Xu. 2014. “Fast Implementation of DeLong’s Algorithm for Comparing the Areas Under Correlated Receiver Operating Characteristic Curves.” *IEEE Signal Processing Letters* 21: 1389–93. <https://doi.org/10.1109/LSP.2014.2337313>.
- Tan, M., and Q. V. Le. 2019. “EfficientNet: Rethinking Model Scaling for Convolutional Neural Networks.” *Proceedings of the 36th International Conference on Machine Learning* 97: 6105–14.
- Tan, N. et al. 2024. “Global, Regional, and National Burden of Early-Onset Gastric Cancer.” *Cancer Biology and Medicine* 21: 667–78. <https://doi.org/10.20892/j.issn.2095-3941.2024.0159>.
- Wu, Z., C. Yang, X. Su, and X. Yuan. 2023. “Adaptive Deep PnP Algorithm for Video Snapshot Compressive Imaging.” *International Journal of Computer Vision* 131 (7): 1662–79. <https://doi.org/10.1007/s11263-023-01777-y>.
- Yang, C., F. Cao, D. Qi, et al. 2020. “Hyperspectrally Compressed Ultrafast Photography.” *Physical Review Letters* 124 (2): 023902. <https://doi.org/10.1103/PhysRevLett.124.023902>.
- Yang, C., S. Zhang, and X. Yuan. 2022. “Ensemble Learning Priors Driven Deep Unfolding for Scalable Video Snapshot Compressive Imaging.” *European Conference on Computer Vision (ECCV)*, 600–618. https://doi.org/10.1007/978-3-031-19790-1_36.
- Zhao, R., C. Yang, R. T. Smith, and L. Gao. 2023. “Coded Aperture Snapshot Spectral Imaging Fundus Camera.” *Scientific Reports* 13 (1): 12007. <https://doi.org/10.1038/s41598-023-39146-x>.