

CALIBRATION CERTIFICATE

Model: 208C02
 Serial #: LW51963
 Description: Force Sensor
 Type: ICP

Date: 7/9/2019
 By: Monty Manning, Cal. Tech. *mm*
 Station: 0-100 lb Load Cell (Test Procedure AT501-5)

Sensitivity*: 49.67 mV/LBF
 11.17 mV/N

Temp: 75 deg F [24deg C]
 Humidity: 56 %

Linearity*: 0.1% FS
 Uncertainty**: +/- 1 %

Cert #: 756809

Bias: 10.39 VDC


* Zero based, least-squares straight line.

** Measurement uncertainty represented using a coverage factor of k=2 which provides a level of confidence of approximately 95 %.

Condition of Unit:

As Found: Not applicable

As Left: In tolerance, new unit

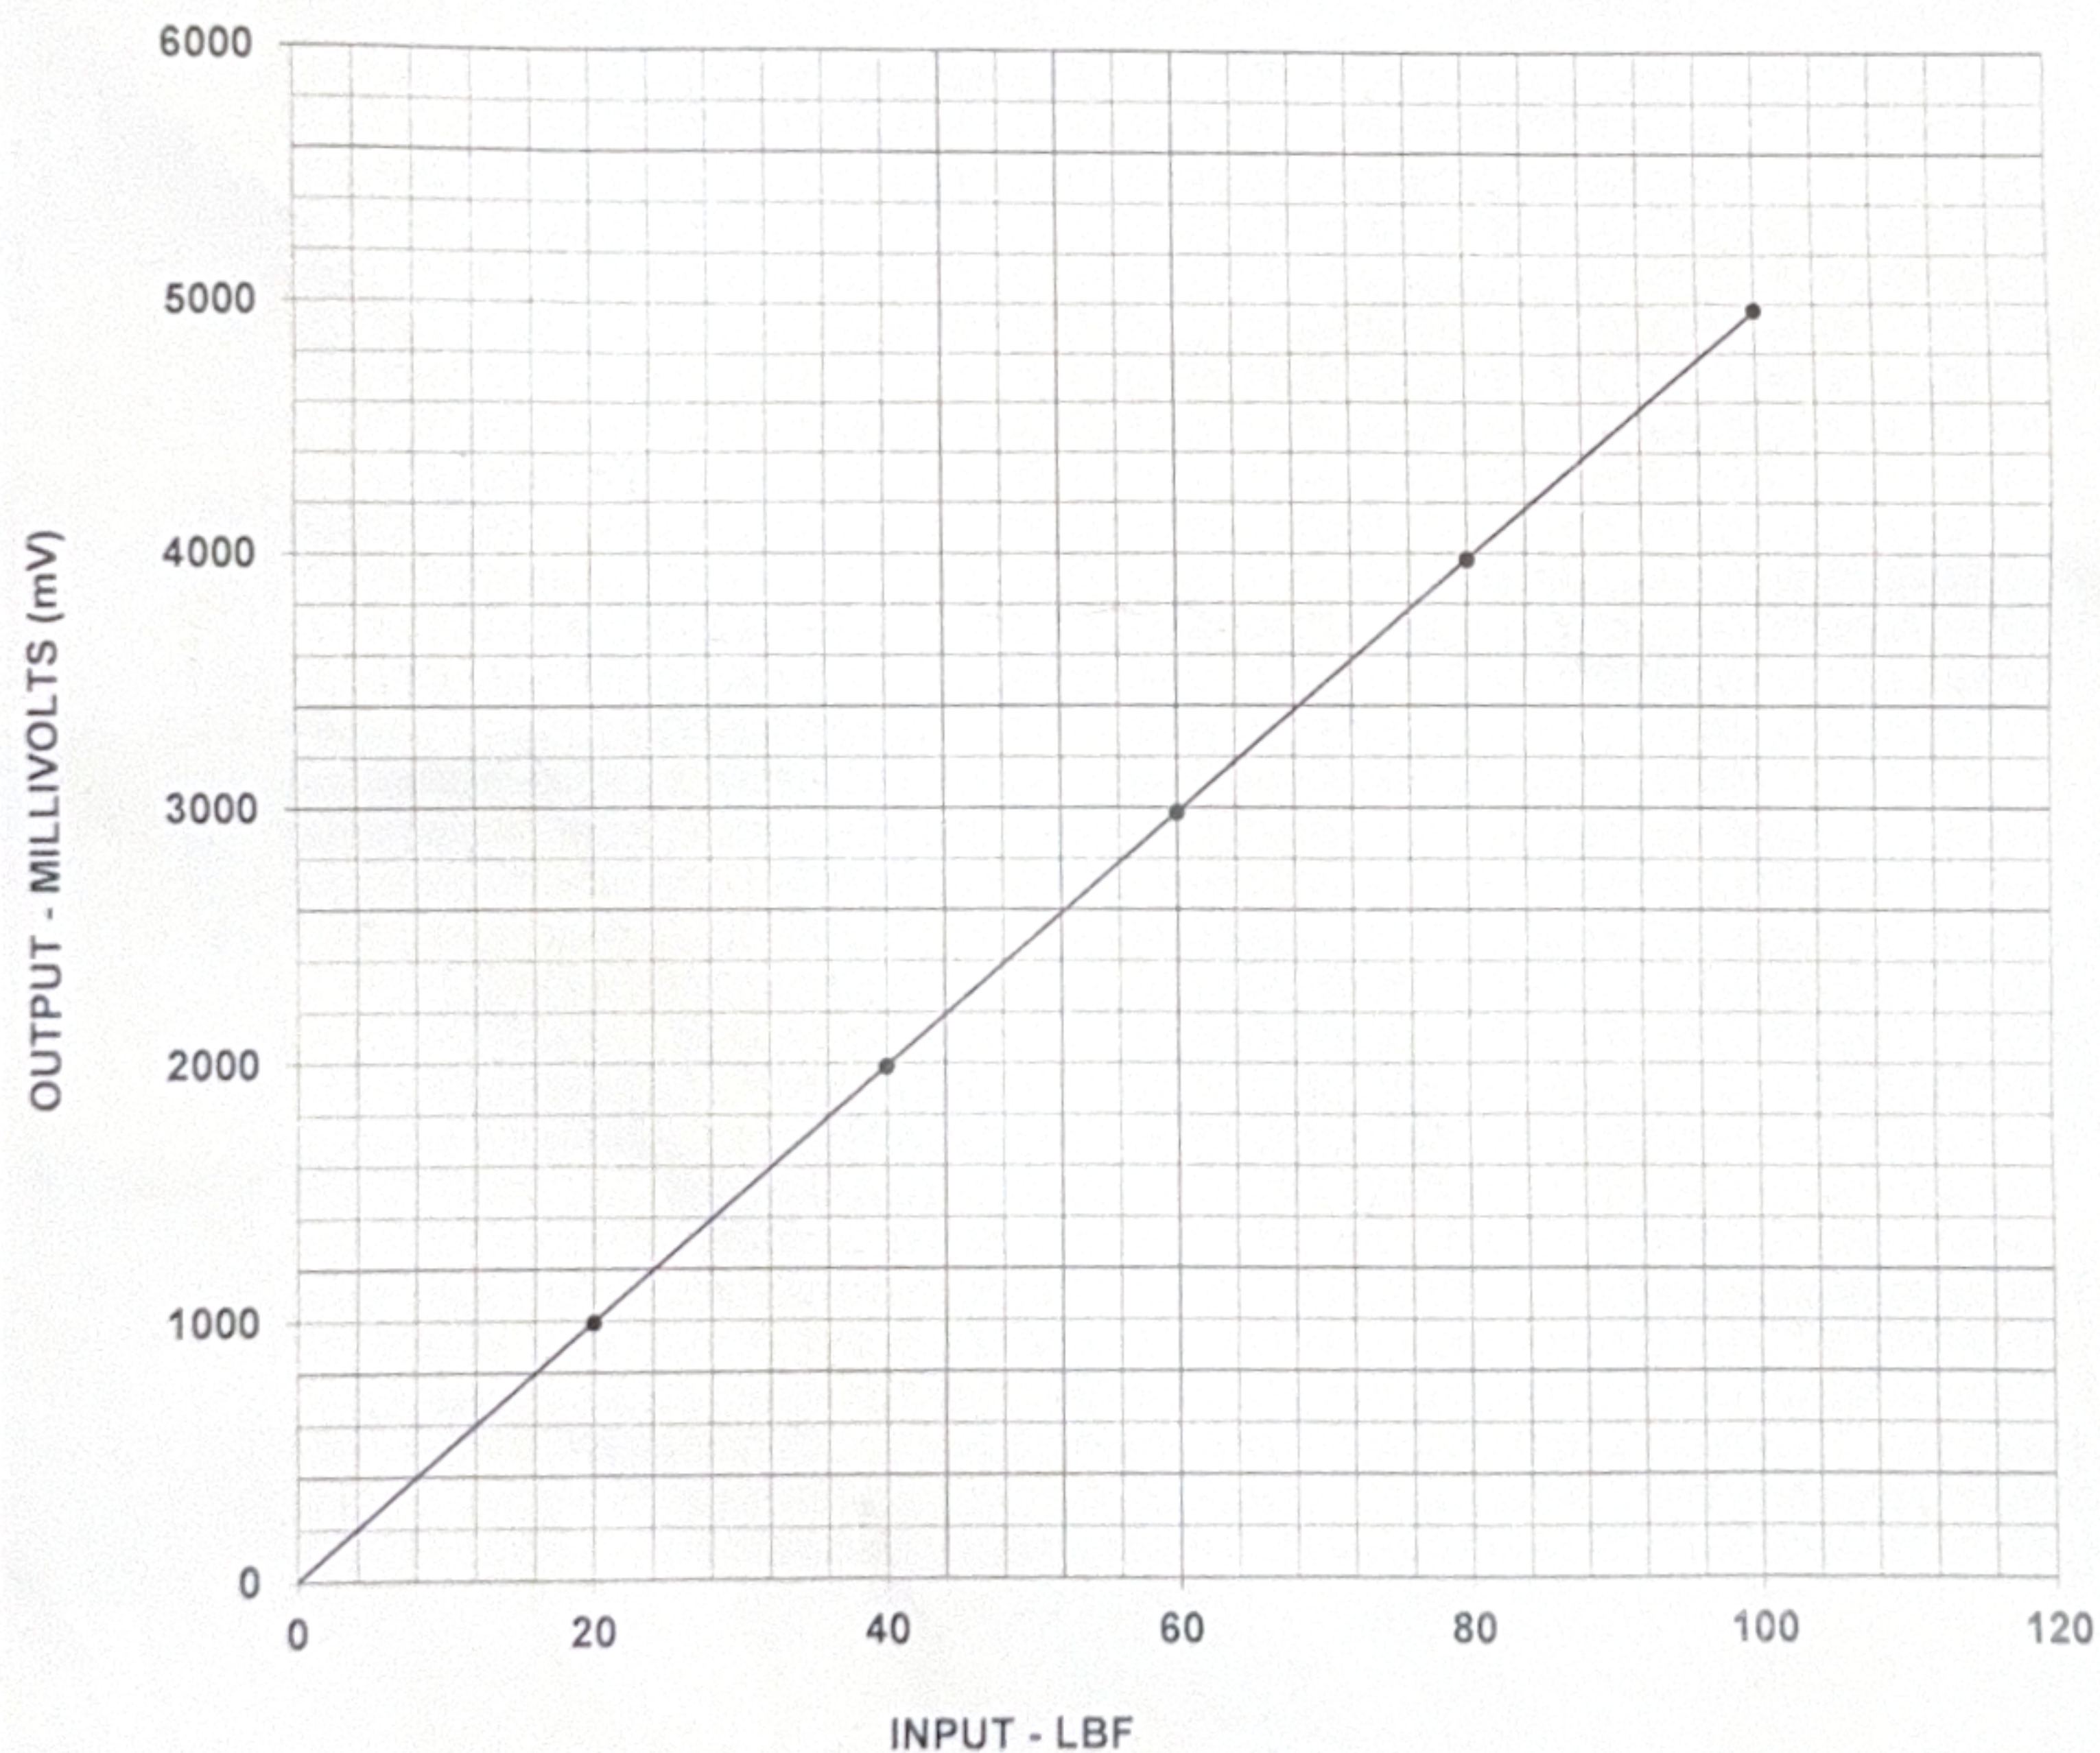

TEST DATA

INPUT (LBF)	OUTPUT (mV)
20.0	990
40.0	1984
60.0	2978
80.0	3971
100	4972

Notes:

- 1 Standard calibration is supplied in compression mode.
- 2 Station # 41
- 3 This sensor is torque to 20 in-lbs prior to calibration.
- 4 Calibration is traceable to NIST and is in compliance with ISO 17025 and ANSI/NCSL Z540.3.
- 5 NIST traceability through PCB control # NC017.
- 6 This certificate may not be reproduced, except in full, without written approval from PCB Piezotronics, Inc.



CALIBRATION CERT #1862.02

PCB PIEZOTRONICS INC.

Tel: 888-684-0013 Fax: 716-685-3886 Email: sales@pcb.com
 Headquarters: 3425 Walden Avenue, Depew, NY 14043
 Manufacturing and Calibration Facility: 10869 Highway 903, Halifax, NC 27839