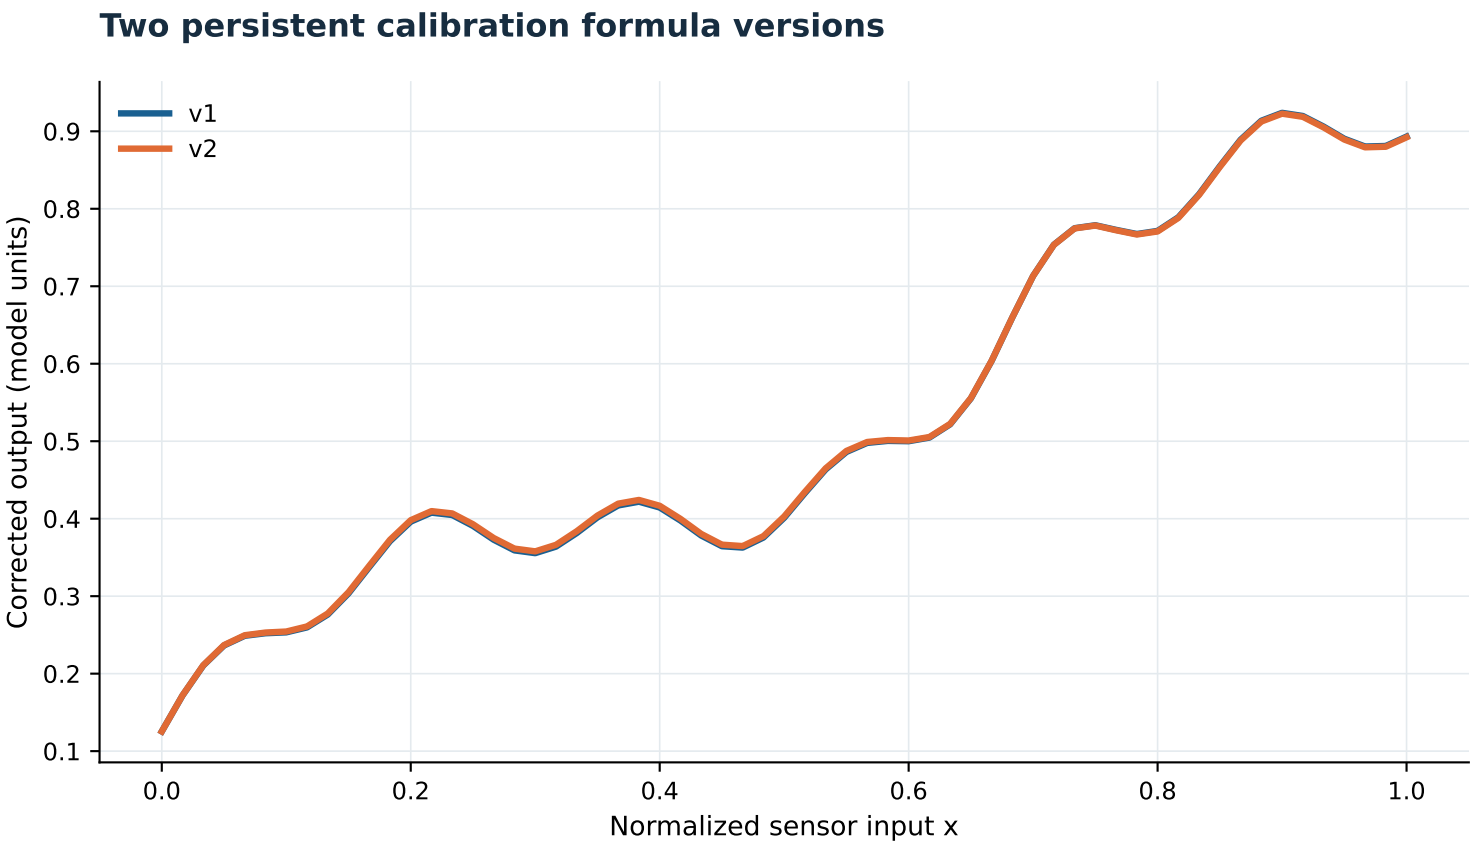
Two persistent calibration formula versions
v1
v2
Corrected output (model units)
0.1
0.2
0.3
0.4
0.5
0.6
0.7
0.8
0.9
0.0
0.2
0.4
0.6
0.8
1.0
Normalized sensor input x