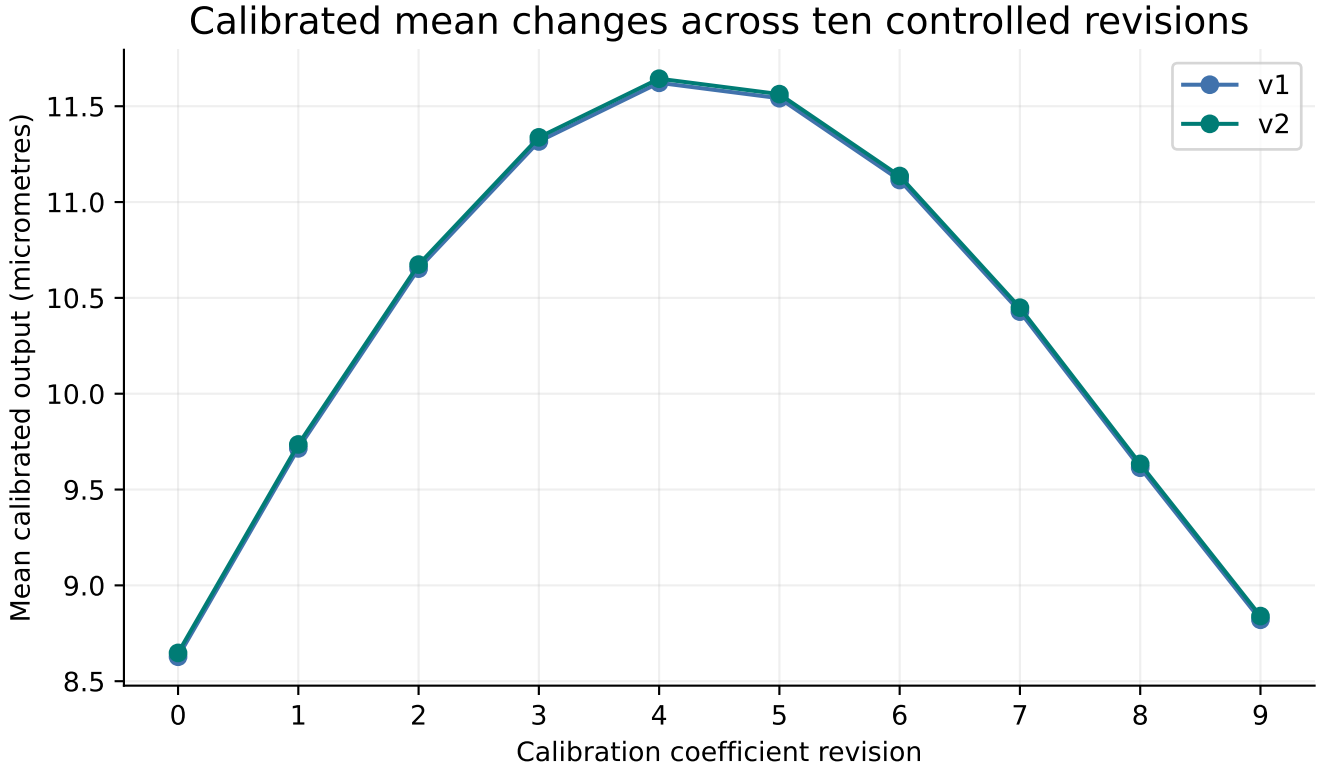
Calibrated mean changes across ten controlled revisions
Mean calibrated output (micrometres)
8.5
9.0
9.5
10.0
10.5
11.0
11.5
0
1
2
3
4
5
6
7
8
9
Calibration coefficient revision
v1
v2