

Patient Data

Administrative Data

□ □ □

female, 9/25/1997

ID: 12345610

Biological and Medical Baseline Data

Mask: **Blue, petite**
Height: **164 cm**
Weight: **69.0 kg**

BMI: **26**

BSA Calculation Method: **Dubois & Dubois**
BSA: **1.75 m2**

Normal Values

Variable	Author	Value	Unit
Maximum Oxygen Uptake	Wasserman weight algorithm	1.94	L/min
Maximum Relative Oxygen Uptake	Based on normal value of maximum oxygen uptake	28	ml/min/kg
Maximum Oxygen Pulse	Wasserman equation	11	ml
Maximum Heart Rate	Traditional formula for bicycle test	171	/min
Maximum Minute Ventilation	Individual normal value, based on MVV or FEV1	98.6	L/min
Maximum Breathing Frequency	Pollock et al. equation	34	/min
Maximum Work Rate	Based on normal maximum oxygen uptake	164	W
Maximum Arterial Blood Pressure	Japanese normal values	167	mmHg
Spirometry normal value set	GLI Standard Values (Quanjer, 2012)		
Distance	Bohannon 2011, Waters 1999	482	m
Relative Oxygen Uptake	Waters 1999	12	ml/min/kg
Relative Liberated Energy to Weight and Distance	Waters 1999	3.0	J/kg/m
Heart Rate	Waters 1999	99	/min
Relative Load of Walking	Relation of normal values for walking and maximum exercise	43	%

LBW: **69.0 kg**
IC: **2.39**


VC: **4.32**
FEV1: **3.52**

9-Panel-Plot Edition 2012



國泰綜合醫院
Cathay General Hospital

Name	□, □□	Weight	69.0 kg
ID	12345610	Height	164 cm
Age	29		
Sex	female		
Date	10/2/2026 4:40 PM	Workload Protocol	□□-10w/min
Duration	0:19:18	Kind of Test	Lab Test
Operator		Sport	Cycling
Device	MetaLyzer 3B-R3	Ambient Conditions	
Workload Device	Lode Corival (906900)	Temperature	25.6°C
		Pressure	1012mBar

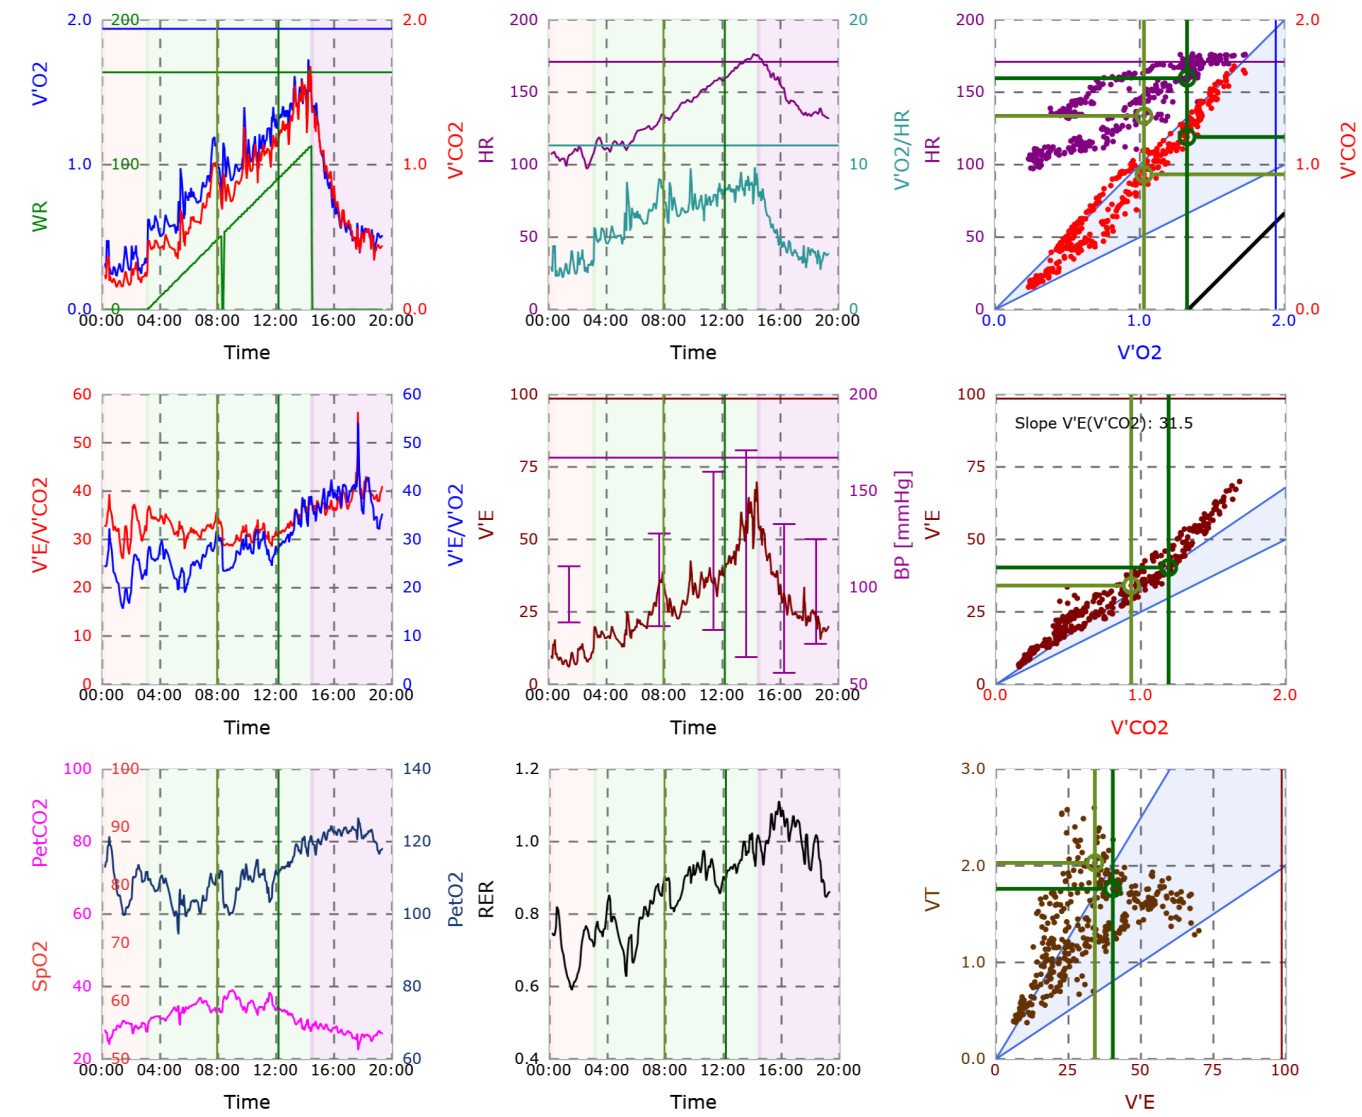


Signature

Measurements at Rest

Name	□, □□	Weight	69.0 kg
ID	12345610	Height	164 cm
Age	29		
Sex	female		
Date	10/2/2026 4:38 PM		

Maximum Flow-Volume Loop

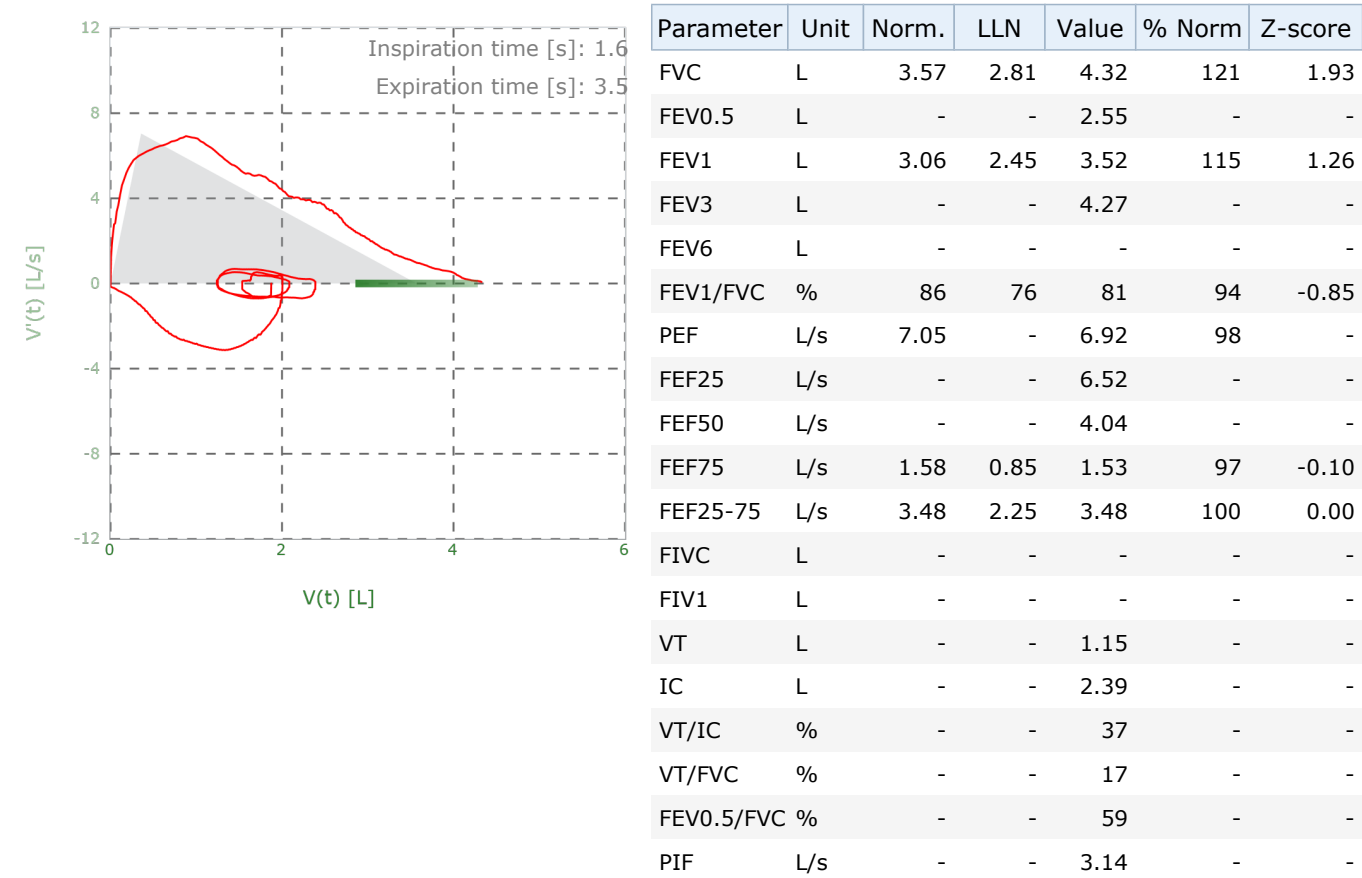



Detailed Information for VT1, VT2, V'O2peak Calculation

VT1 is determined based on smoothed data by Moving data points average method 3. The calculation range was 0:04:00-0:11:39.

VT2 is determined based on smoothed data by Moving data points average method 3. The calculation range was 0:08:40-0:14:05.

V'O2peak is determined based on smoothed data by Moving data points average method 3.

Lipid Metabolism is determined based on smoothed data by Moving data points average method 3.

Mean Values at Rest

Variable	Unit	Value	Variable	Unit	Value	Variable	Unit	Value
Begin	mm : ss	00:00	End	mm : ss	03:00	V'O2	L/min	0.32
V'CO2	L/min	0.22	RER		0.70	V'E	L/min	9.6
VT	L	0.53	BF	/min	18	V'E/V'O2		22.7
V'E/V'CO2		32.4	FIO2	Vol%	-	PetO2	mmHg	109
FICO2	Vol%	-	FECO2	Vol%	3.2	PetCO2	mmHg	29
HR	/min	106	WR	W	0	V'O2/HR	ml	3
BP	mmHg	111 / 82	SpO2	%	-	V'O2/kg	ml/min/kg	5
Q'/V'O2	1	12.52						

Data Table

Time [h:mm:ss]	V'O2/kg [ml/min/kg]	V'O2/HR [ml]	HR [/min]	PaO2 [mmHg]	PaCO2 (est.) [mmHg]	PetCO2 [mmHg]	PetO2 [mmHg]	RER	V'E/V'CO2	V'E/V'O2
Rest										
0:00:30	5	3	108	-	28	26	117	0.76	35.0	26.5
0:01:00	4	3	104	-	29	27	114	0.75	33.8	25.4
0:01:30	4	3	103	-	31	30	104	0.63	29.1	18.2
0:02:00	5	3	109	-	32	30	102	0.61	30.3	18.6
0:02:30	6	4	109	-	30	29	110	0.71	35.5	25.2
0:03:00	4	3	100	-	31	29	111	0.74	31.3	23.2
Exercise										
0:03:30	8	5	112	-	31	30	110	0.75	35.4	26.6
0:04:00	9	5	114	-	31	31	108	0.77	34.8	26.8
0:04:30	9	5	112	-	30	31	110	0.82	34.8	28.3
0:05:00	8	5	115	-	32	33	103	0.74	32.6	24.1
0:05:30	11	7	112	-	33	33	101	0.68	32.1	21.8
0:06:00	11	6	117	-	34	34	102	0.70	30.4	21.3
0:06:30	12	7	124	-	33	35	104	0.79	32.2	25.3
0:07:00	11	6	126	-	34	36	103	0.82	31.4	25.7
0:07:30	13	7	126	-	33	35	106	0.86	32.2	27.6
0:08:00	17	9	132	-	32	34	109	0.88	32.9	28.8
0:08:30	14	8	132	-	33	35	108	0.87	31.4	27.4
0:09:00	14	7	136	-	35	38	101	0.82	29.0	23.9
0:09:30	14	7	143	-	34	38	105	0.89	29.7	26.3
0:10:00	16	8	144	-	32	34	112	0.92	31.7	29.1

□□□□□□

Patient
□, □□

Date
10/2/2026 4:40 PM

Time [h:mm:ss]	V'O2/kg [ml/min/kg]	V'O2/HR [ml]	HR [/min]	PaO2 [mmHg]	PaCO2 (est.) [mmHg]	PetCO2 [mmHg]	PetO2 [mmHg]	RER	V'E/V'CO 2	V'E/V'O2
0:10:30	16	8	148	-	33	36	109	0.92	30.2	27.8
0:11:00	16	7	152	-	32	34	113	0.94	32.3	30.4
0:11:30	17	8	156	-	32	35	110	0.92	31.5	29.1
0:12:00	19	8	159	-	33	35	108	0.87	30.2	26.4
0:12:30	19	8	160	-	32	34	112	0.92	31.4	28.8
0:13:00	20	8	165	-	31	33	114	0.93	32.6	30.3
0:13:30	21	9	170	-	30	31	117	0.97	34.5	33.4
0:14:00	22	9	173	-	29	29	119	0.99	35.8	35.5

Recovery

0:14:30	23	9	175	-	28	29	119	0.98	36.8	35.9
0:15:00	20	8	171	-	28	29	119	0.97	36.8	35.8
0:15:30	15	6	164	-	29	29	121	1.03	36.4	37.6
0:16:00	12	5	159	-	28	28	123	1.08	36.8	39.7
0:16:30	10	4	150	-	28	28	123	1.06	37.2	39.4
0:17:00	9	4	144	-	28	27	123	1.04	38.3	39.7
0:17:30	8	4	139	-	27	26	123	1.03	39.1	40.3
0:18:00	8	4	135	-	27	25	123	0.96	43.1	41.4
0:18:30	8	4	135	-	26	26	122	0.99	41.7	41.0
0:19:00	7	4	136	-	27	26	121	0.92	39.2	36.2
0:19:30	7	4	133	-	28	28	117	0.85	39.0	33.3

Extended Data Table

Time [h:mm:ss]	V'CO2 [L/min]	V'O2 [L/min]	WR [W]	WR [W]	V'E/MVV	SpO2 [%]	Q'V'O2 [l]	BP [mmHg]	Borg	BF [l/min]	BR [L/min]						
Rest																	
0:00:30	0.29	0.38	0	0	0.10	-	10.96	-	-	17	111						
0:01:00	0.20	0.26	0	0	0.07	-	13.15	-	-	18	114						
0:01:30	0.18	0.28	0	0	0.06	-	13.01	111/82	7	17	116						
0:02:00	0.21	0.34	0	0	0.07	-	12.24	-	-	18	115						
0:02:30	0.30	0.42	0	0	0.11	-	10.92	-	-	21	110						
0:03:00	0.22	0.29	0	0	0.07	-	12.54	-	-	15	115						
Exercise																	
0:03:30	0.42	0.56	4	4	0.14	-	9.20	0/0	-	21	106						
0:04:00	0.47	0.61	9	9	0.15	-	9.88	-	-	13	105						
0:04:30	0.48	0.59	14	14	0.15	-	9.94	-	-	14	105						
0:05:00	0.42	0.57	19	19	0.12	-	10.39	-	-	9	108						
0:05:30	0.53	0.77	24	24	0.16	-	8.01	0/0	-	21	104						
0:06:00	0.52	0.75	29	29	0.15	-	8.83	-	-	21	105						
0:06:30	0.66	0.84	34	34	0.19	-	8.61	-	11	14	100						
0:07:00	0.64	0.79	39	39	0.18	-	8.96	-	-	12	102						

□□□□□□

Patient
□, □□

Date
10/2/2026 4:40 PM


Time [h:mm:ss]	V'CO2 [L/min]	V'O2 [L/min]	WR [W]	WR [W]	V'E/MVV	SpO2 [%]	Q'/V'O2 [l]	BP [mmHg]	Borg	BF [l/min]	BR [L/min]						
0:07:30	0.74	0.86	44	44	0.21	-	8.51	128/80	-	13	98						
0:08:00	1.01	1.16	49	49	0.29	-	6.48	-	-	19	88						
0:08:30	0.87	1.00	54	54	0.24	-	7.55	-	11	18	94						
0:09:00	0.82	0.99	59	59	0.20	-	7.46	-	-	12	98						
0:09:30	0.87	0.98	64	64	0.22	-	7.95	0/0	-	12	96						
0:10:00	1.02	1.11	69	69	0.28	-	7.06	-	13	21	88						
0:10:30	1.03	1.12	74	74	0.27	-	7.41	-	-	16	90						
0:11:00	1.05	1.12	79	79	0.30	-	7.31	-	-	22	87						
0:11:30	1.11	1.21	84	84	0.30	-	7.05	160/78	-	17	86						
0:12:00	1.17	1.33	89	89	0.30	-	6.55	-	-	19	86						
0:12:30	1.23	1.34	94	94	0.33	-	6.69	-	-	22	82						
0:13:00	1.27	1.37	99	99	0.36	-	6.53	-	-	27	78						
0:13:30	1.42	1.47	104	104	0.43	-	6.31	171/64	-	31	70						
0:14:00	1.50	1.51	109	109	0.47	-	6.18	-	15	36	65						
Recovery																	
0:14:30	1.55	1.59	0	0	0.50	-	5.91	-	-	38	61						
0:15:00	1.31	1.35	0	0	0.42	-	6.67	-	16	31	71						
0:15:30	1.06	1.03	0	0	0.34	-	7.82	-	-	31	81						
0:16:00	0.89	0.82	0	0	0.29	-	8.79	-	-	29	87						
0:16:30	0.70	0.66	0	0	0.23	-	9.61	133/56	12	24	94						
0:17:00	0.63	0.61	0	0	0.22	-	10.01	-	-	24	96						
0:17:30	0.56	0.54	0	0	0.20	-	10.09	-	-	23	98						
0:18:00	0.50	0.53	0	0	0.21	-	9.88	-	-	32	98						
0:18:30	0.56	0.57	0	0	0.21	-	9.78	125/71	11	19	97						
0:19:00	0.47	0.50	0	0	0.17	-	9.86	-	-	20	103						
0:19:30	0.43	0.51	0	0	0.15	-	10.86	-	-	16	104						

custo med GmbH

Maria-Merian-Str. 6
85521 Ottobrunn
Tel. +49 89 71098-00
Fax: +49 89 71098-10
e-Mail: info@customed.de
Web: http://www.customed.de

洪 筱昀

Pat. ID	12345610	Gender	Female
Date of birth	25.09.1997	Height	164 cm
Age	29	Weight	69.0 kg
		BMI	25.65 kg/m
CPX			
Evaluation	02.10.2026	17:00 o'clock	

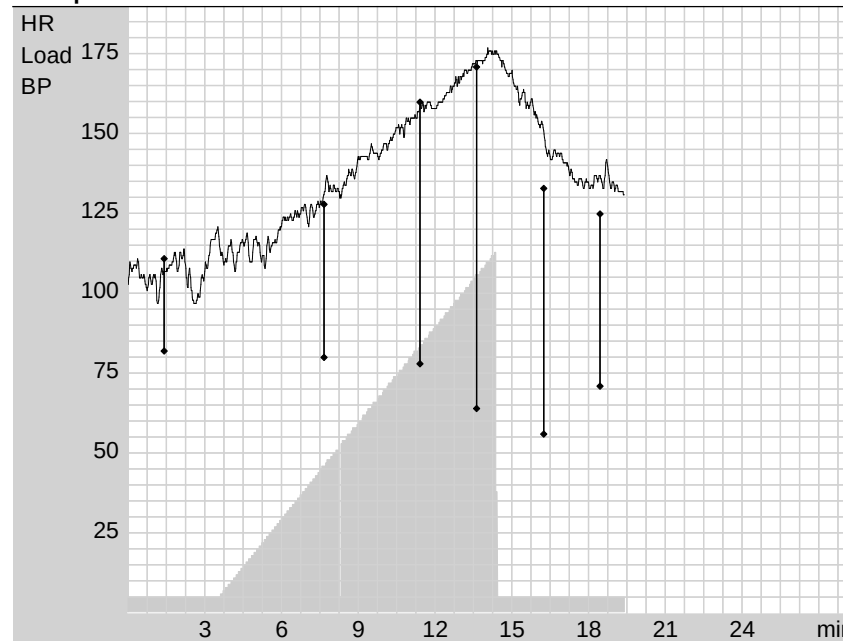Final protocol**Summary**

Duration total	19:25	min
Duration stress	19:25	min
Duration recovery		
Max. load	112	W
% of Reference 173	64	%
HR peak	177	1/min
% of Reference 191	92	%
BP rest	111 / 82	mmHg
BP max.	171 / 64	mmHg
HRxBP, max.	30096	
MET, maximum	6.6	

Evaluation data

PWC	W	W / kg	reference value
170			
150			
130			
max. 176	112	1.6	

Measured values

	Duration	Load	HR	MET	BP	ST Measurement (mV)											
						I	II	III	aVR	aVL	aVF	V1	V2	V3	V4	V5	V6
1	02:59	0	105	1.0	111/82	0.07	0.01	-0.05	-0.04	0.06	-0.02	0.07	0.03	0.01	0.00	-0.01	-0.01
2	A	112	128		128/80												
2	A	112															
2	A	112	156		160/78												
2	11:21	112	176	6.6	171/64	0.05	0.02	-0.03	-0.04	0.04	-0.00	-0.04	-0.06	-0.15		-0.14	-0.19
3	A	0	153		133/56												
3	05:05	0	132	1.0	125/71	0.04	-0.00	-0.04	-0.02	0.04	-0.02	0.05	0.03	-0.01	-0.02	-0.05	-0.05

Unconfirmed Report

submaximal charged


Max. load: 112 W at Load stage 2 at 14:10 min, 64 % of Reference 173.0 W, MET: 6.6

Max. HR: 176 1/min at Load stage 2 at 14:10 min, 92% of Reference 191 1/min

Max. ST Inclination at Channel V1: 0.07 mV at Load stage 1, Max. ST Depression at Channel V6: -0.19 mV at Load stage 2

ECG 02:49 1. Stress stage 0 W HR: 105 BP: 111/82 mmHg

(25 mm/s 10 mm/mV 0.05Hz - 45Hz / 50Hz / ADF)

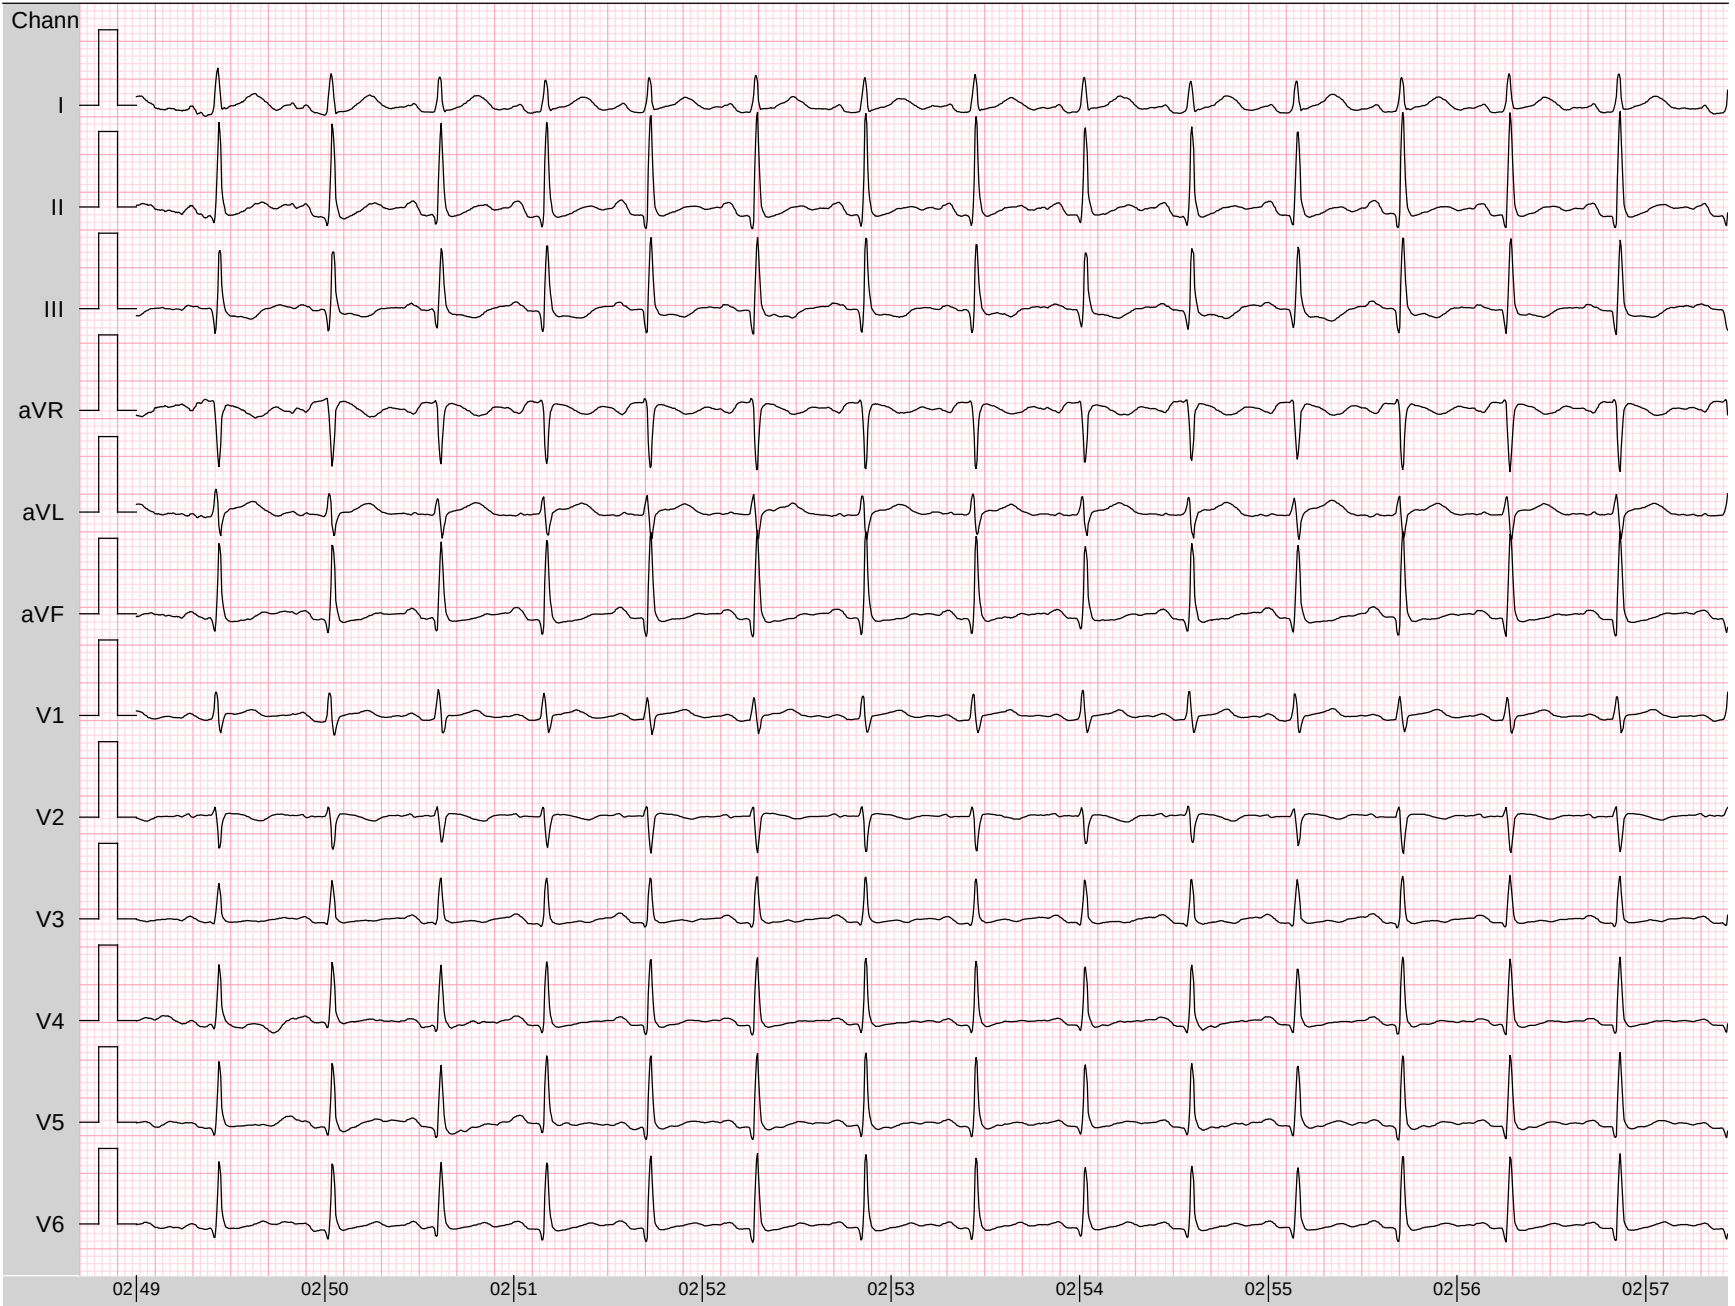

ECG 14:10 2. Stress stage 112 W HR: 176 BP: 171/64 mmHg

(25 mm/s 10 mm/mV 0.05Hz - 45Hz / 50Hz / ADF)

