
Device Settings (1 of 2)

Data Source: MiniMed 780G, MMT-1884 (NG3490631H)

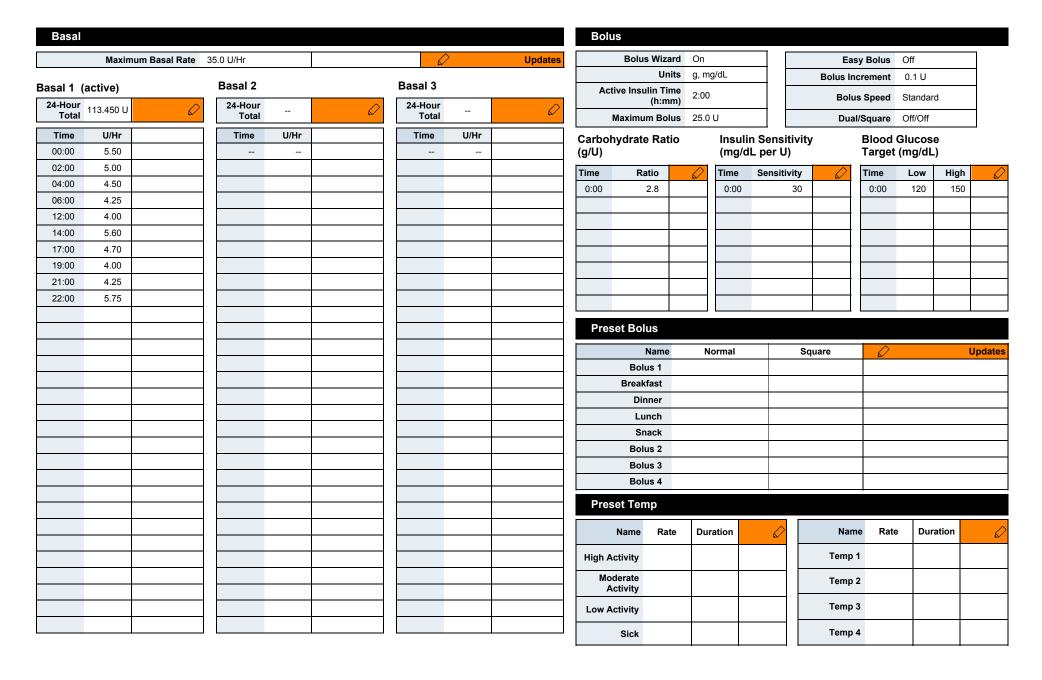

Generated: 09-18-2023, 13:02 Data Source: MiniMed 780G, MMT-1884 (NG3490631H)

SmartGuard	
SmartGuard	On
Target	120 mg/dL
Auto Correction	On

High Alerts			Off (	(Snooze 1:00)
Start Time	High (mg/dL)	Alert On High	Alert Before High	Rise Alert Limit (mg/dL)
				, and the second
	•			

Low A	Alerts		O	ff (Snooze	9 0:20)
Start Time	Low (mg/dL)	Suspend	Alert On Low	Alert Before Low	Resume Basal Alert

Sensor	
Sensor	On
Calibration Reminder	Off
Calibration Reminder Time	Off

	Calibration Reminder	Off
	Calibration Reminder Time	Off
Notes		
-		

_	Basal 4		Basal 5		Workday		Day Off		Sick Day	
	24-Hour Total		24-Hour Total		24-Hour Total		24-Hour Total		24-Hour Total	
	Time	U/Hr								
it										
ne										
ı										
_										
4										
									_	

Rem	

Low Reservoir Warning	Insulin Units
Amount	20 U
Bolus BG Check	Off
Set Change	Off

## Missed Meal Bolus

Name	Start	End
Meal 1	Off	Off
Meal 2	Off	Off
Meal 3	Off	Off
Meal 4	Off	Off
Meal 5	Off	Off
Meal 6	Off	Off
Meal 7	Off	Off
Meal 8	Off	Off

## **Personal Reminders**

Name	Time
Reminder 1	Off
Reminder 2	Off
Reminder 3	Off
Reminder 4	Off
Reminder 5	Off
Reminder 6	Off
BG Check	Off
Medication	Off

Utilities	
Block Mode	Off
Time Format	24 Hr
Brightness	Auto
Backlight Timeout	180 s
Audio Options	Audio
Alarm Volume	5
Auto Suspend	Off