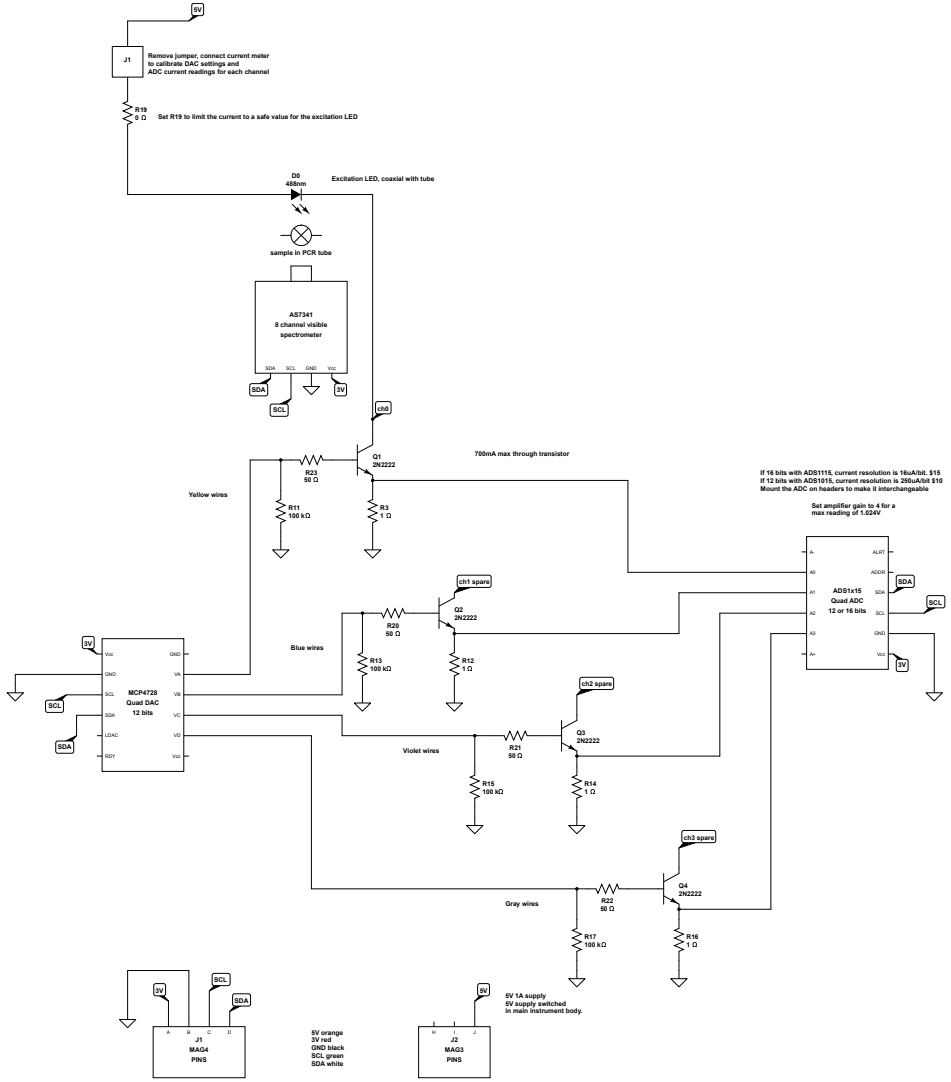


Safety Summary: protect user from potentially dangerous UV exposure
1. keep lid closed during startup
2. start measurement only when the lid is closed
3. do not open the lid when status == BUSY

STELLA-LS Lab_Spec Plugin
Paul Mirel for NASA -- 20260207