

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024


Clinical Path - Urine Routine Chemistry, Bilirubin (urine), -

	N
All Methods	396
Reflectance Photometry - (Your Method)	76
TransAsia Laura urine analyser - (Your Analyzer)	22

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

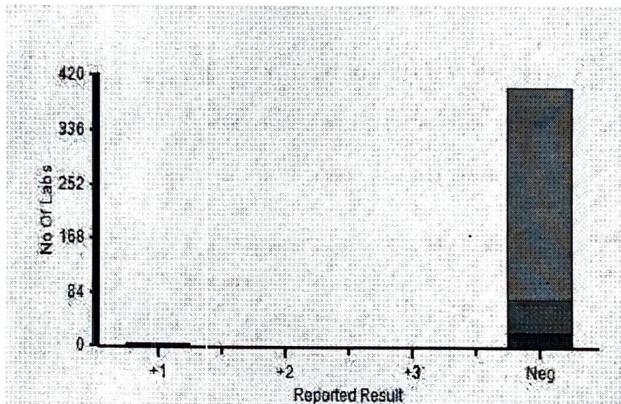

Satish Jadhav
 ✓



PC-1022

Page 1 of 18

Metropolis Healthcare Ltd., EQAS

Analyte Methodwise Result Report

Lab : 837



Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

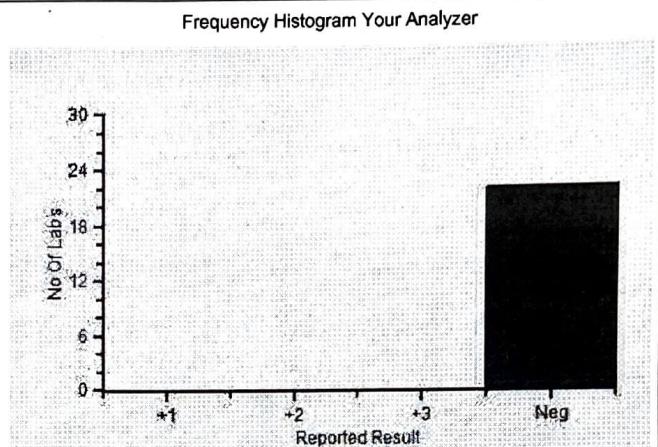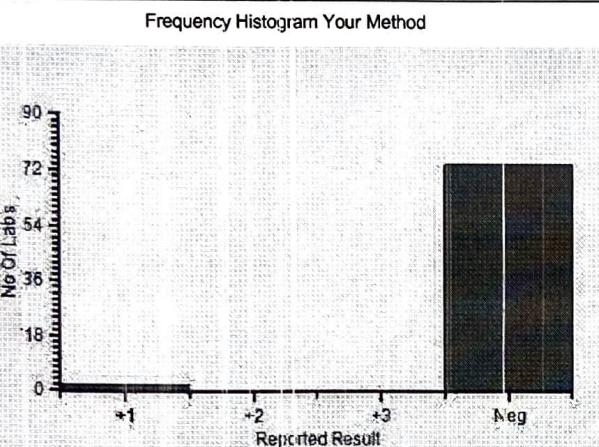

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass : Acceptable performance
- One out of two pass : Review for random error & take action if appropriate
- Both failed : Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass : Acceptable performance
- Two out of three pass : Review for random error & take action if appropriate
- One out of three pass : Unacceptable performance, Review for systematic error
- All failed : Unacceptable performance, Review for systematic error



PC-1022

Page 2 of 18

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

Clinical Path - Urine Routine Chemistry, Blood (urine), -

	N
All Methods	394
Reflectance Photometry - (Your Method)	72
TransAsia Laura urine analyser - (Your Analyzer)	21

Evaluation Based On - Method wise Peer Grouping

Your Result


1+

Result Expected

+1,+2,Tr

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

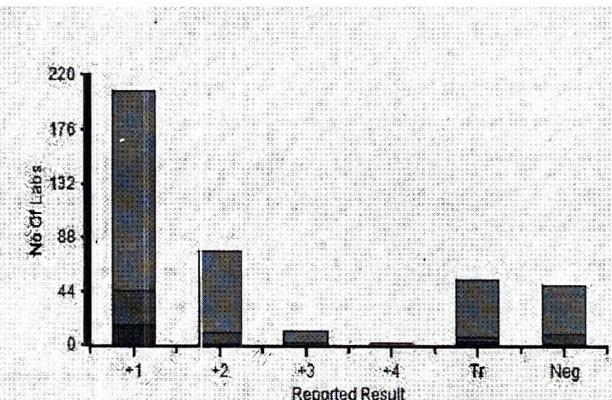

PC-1022

Page 3 of 18

Metropolis Healthcare Ltd., EQAS
Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD


Report Date : 18/02/2025

Cycle No : 240412


Sample No : 01

Round Open Date : 25/12/2024

Frequency Histogram Your Method

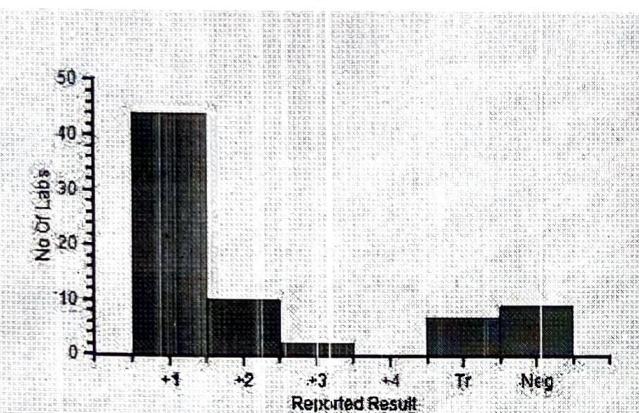

Frequency Histogram Your Analyzer

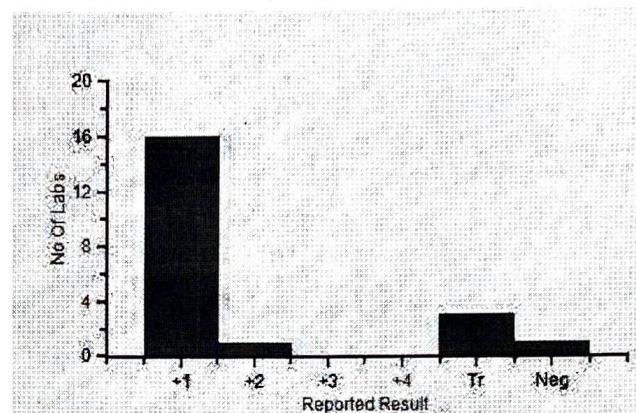

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



PC-1022

Page 4 of 18

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

Clinical Path - Urine Routine Chemistry, Glucose (urine), -

- All Methods 403
- Reflectance Photometry - (Your Method) 74
- TransAsia Laura urine analyser - (Your Analyzer) 20

Evaluation Based On - Method wise Peer Grouping


Your Result

3+

Result Expected

+2, +3, +4

Note : # is an indication that this parameter has not been evaluated

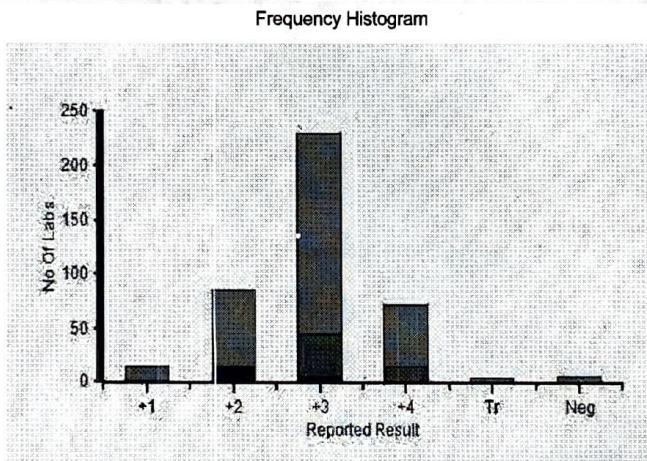

PC-1022

Page 5 of 18

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD


Report Date : 18/02/2025

Cycle No : 240412


Sample No : 01

Round Open Date : 25/12/2024

Frequency Histogram Your Method

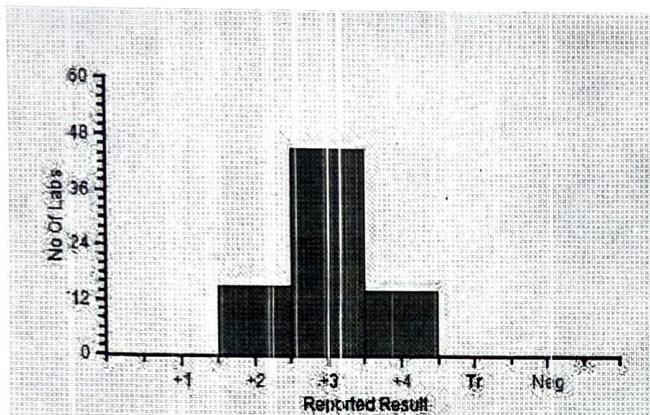

Frequency Histogram Your Analyzer

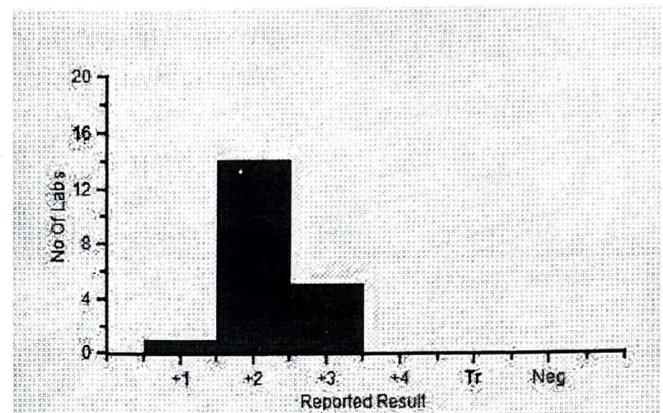

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



PC-1022

Page 6 of 18

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

Clinical Path - Urine Routine Chemistry, Ketone (urine), -


	N
All Methods	401
Reflectance Photometry - (Your Method)	71
TransAsia Laura urine analyser - (Your Analyzer)	21

Evaluation Based On - Method wise Peer Grouping

Your Result	Negative
Result Expected	Neg,Tr

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

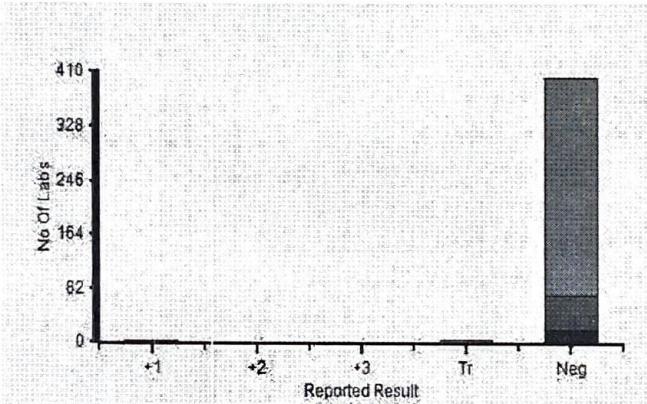

PC-1022

Page 7 of 18

Metropolis Healthcare Ltd., EQAS

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD


Report Date : 18/02/2025

Cycle No : 240412


Sample No : 01

Round Open Date : 25/12/2024

Frequency Histogram Your Method

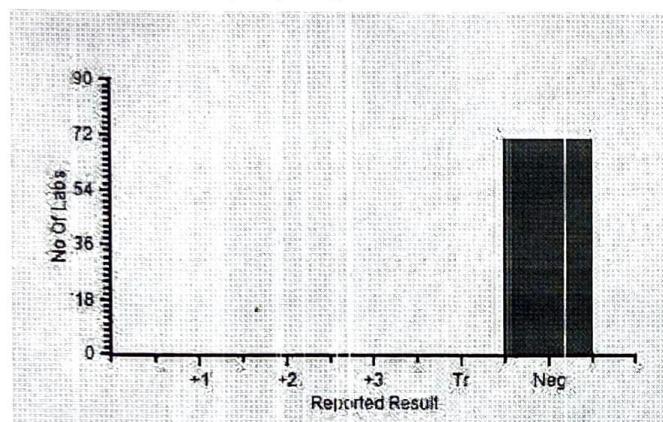

Frequency Histogram Your Analyzer

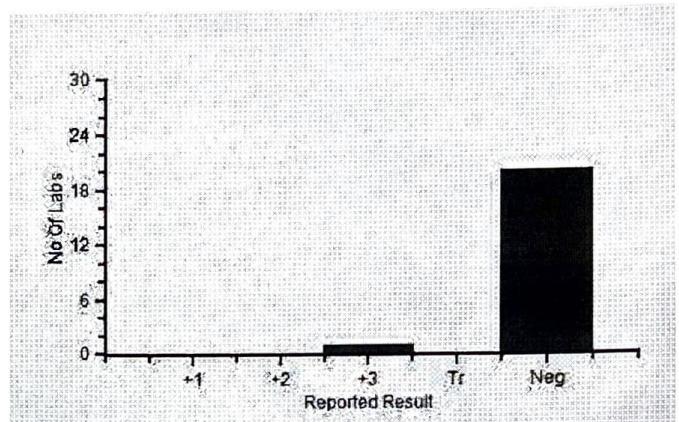

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass : Acceptable performance
- One out of two pass : Review for random error & take action if appropriate
- Both failed : Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass : Acceptable performance
- Two out of three pass : Review for random error & take action if appropriate
- One out of three pass : Unacceptable performance, Review for systematic error
- All failed : Unacceptable performance, Review for systematic error



PC-1022

Page 8 of 18

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024


Clinical Path - Urine Routine Chemistry, Nitrite (urine), -

	N
All Methods	387
Reflectance Photometry - (Your Method)	81
TransAsia Laura urine analyser - (Your Analyzer)	21

Your Result	Present
Result Expected	Pre

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

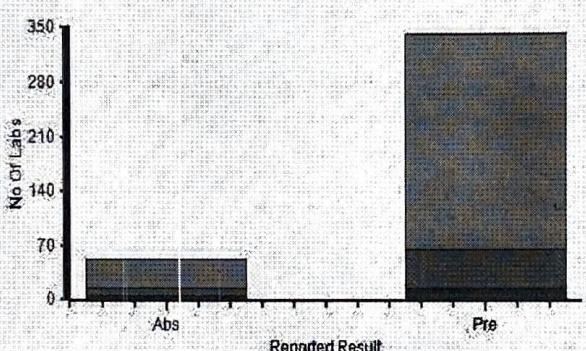

PC-1022

Page 9 of 18

Analyte Methodwise Result Report

Lab : 837


Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

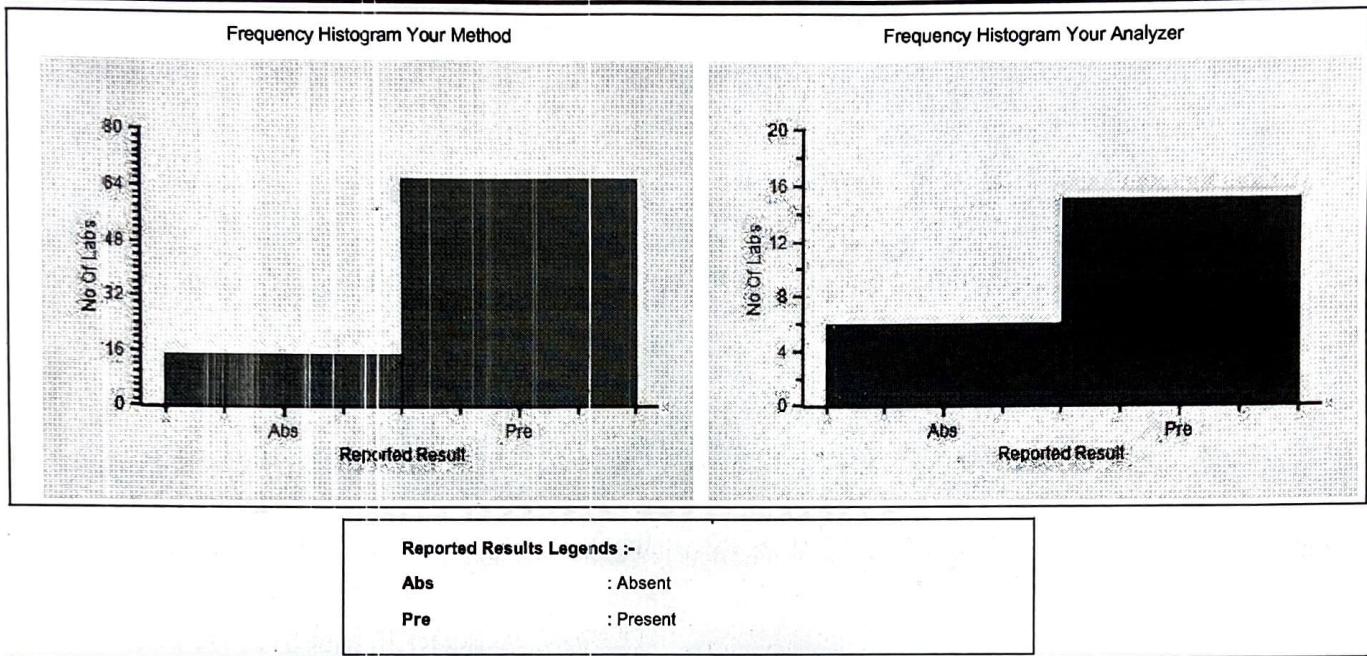

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



PC-1022

Page 10 of 18

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

Clinical Path - Urine Routine Chemistry, pH, -


	N
All Methods	405
Reflectance Photometry - (Your Method)	72
TransAsia Laura urine analyser - (Your Analyzer)	21

Evaluation Based On - Method wise Peer Grouping

Your Result	5
Result Expected	5,5,5,6

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

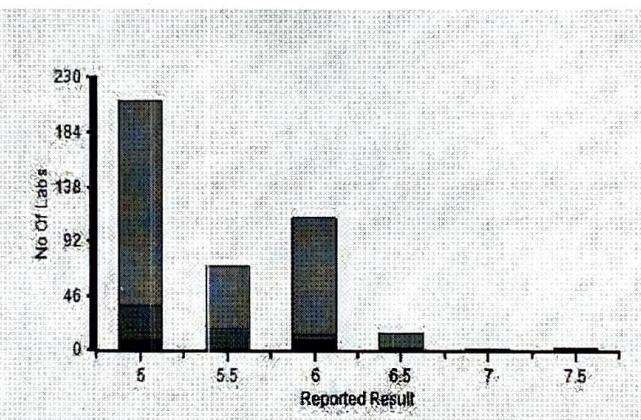

PC-1022

Page 11 of 18

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD


Report Date : 18/02/2025

Cycle No : 240412


Sample No : 01

Round Open Date : 25/12/2024

Frequency Histogram Your Method

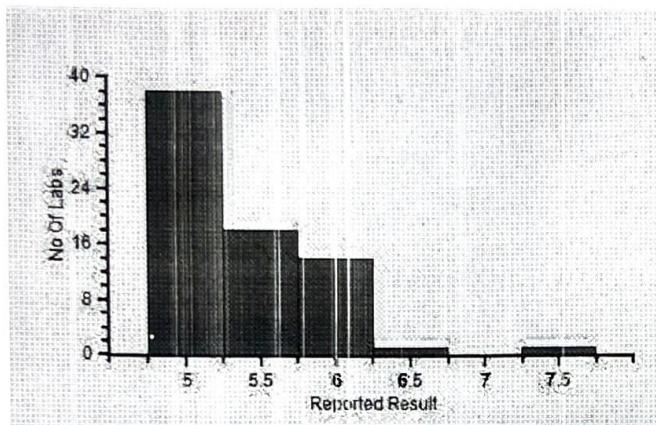

Frequency Histogram Your Analyzer

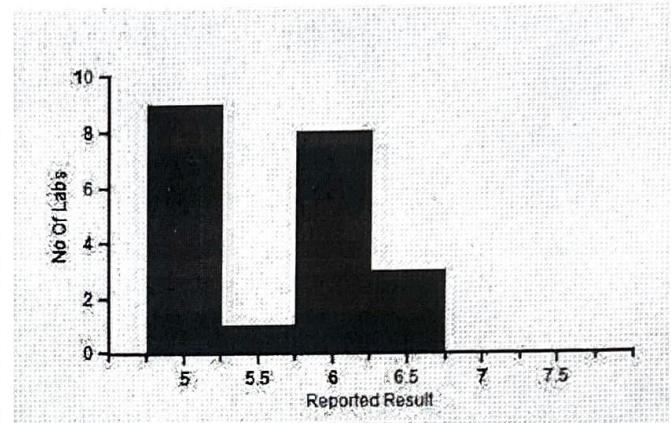

Reported Results Legends :-

5	:	5
5.5	:	5.5
6	:	6
6.5	:	6.5
7	:	7
7.5	:	7.5
8	:	8
8.5	:	8.5
9	:	9

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



PC-1022

Page 12 of 18

Metropolis Healthcare Ltd., EQAS
Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

Clinical Path - Urine Routine Chemistry, Protein (Urine), -


	N
All Methods	404
Reflectance Photometry - (Your Method)	74
TransAsia Laura urine analyser - (Your Analyzer)	21

Evaluation Based On - Method wise Peer Grouping

Your Result	1+
Result Expected	+1,+2,+3

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

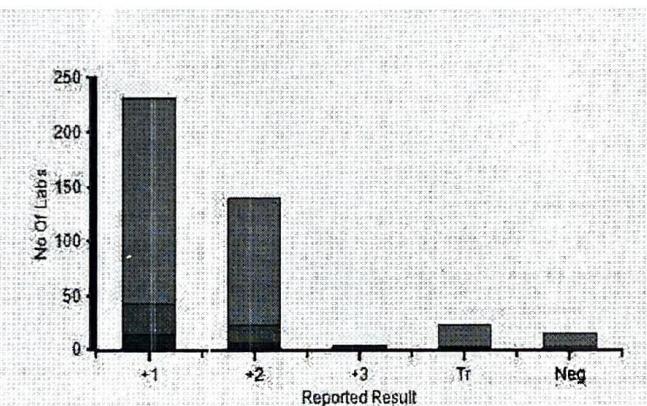

PC-1022

Page 13 of 18

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD


Report Date : 18/02/2025

Cycle No : 240412


Sample No : 01

Round Open Date : 25/12/2024

Frequency Histogram Your Method

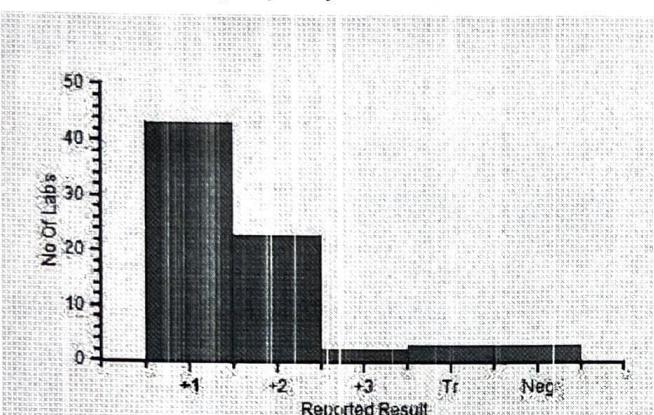

Frequency Histogram Your Analyzer

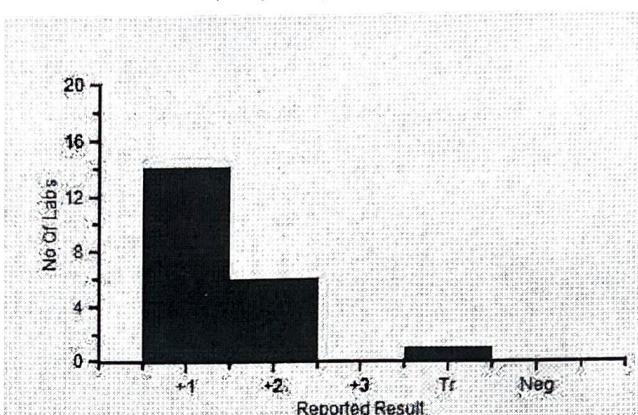

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass : Acceptable performance
- One out of two pass : Review for random error & take action if appropriate
- Both failed : Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass : Acceptable performance
- Two out of three pass : Review for random error & take action if appropriate
- One out of three pass : Unacceptable performance, Review for systematic error
- All failed : Unacceptable performance, Review for systematic error



PC-1022

Page 14 of 18



Metropolis Healthcare Ltd., EQAS

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01


Round Open Date : 25/12/2024

Clinical Path - Urine Routine Chemistry, Specific Gravity, -

	N
All Methods	402
Reflectance Photometry - (Your Method)	84
TransAsia Laura urine analyser - (Your Analyzer)	22

Evaluation Based On - Method wise Peer Grouping	
Your Result	1.025
Result Expected	1.020, 1.025, 1.030

Note : # is an indication that this parameter has not been evaluated

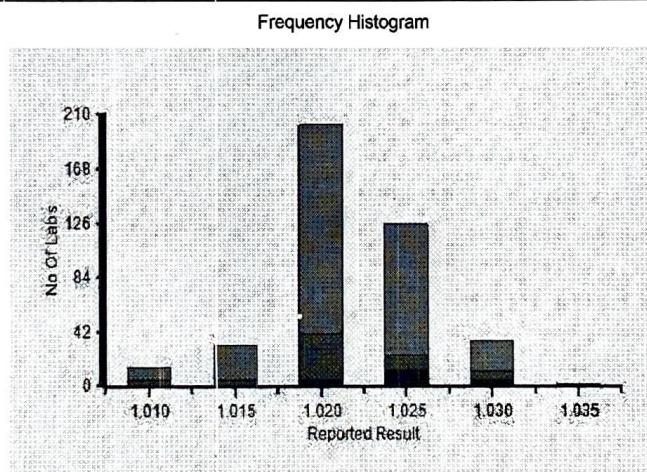

PC-1022

Page 15 of 18

Metropolis Healthcare Ltd., EQAS

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD


Report Date : 18/02/2025

Cycle No : 240412


Sample No : 01

Round Open Date : 25/12/2024

Frequency Histogram Your Method

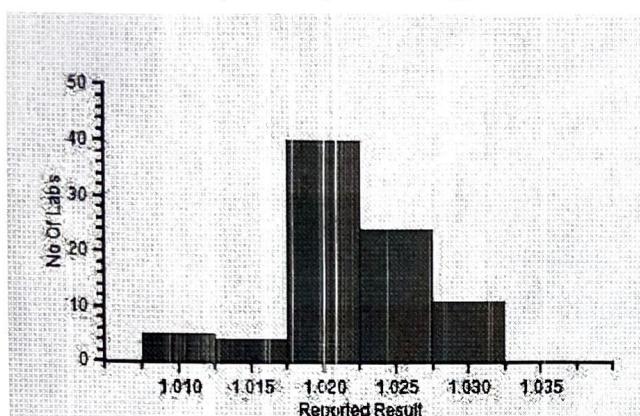

Frequency Histogram Your Analyzer

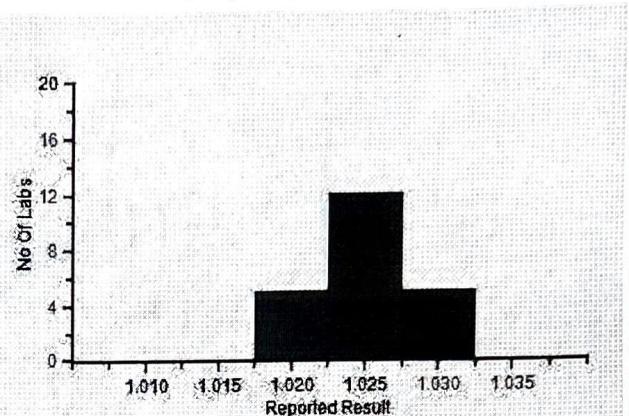

Reported Results Legends :-

1.005	: 1.005
1.010	: 1.010
1.015	: 1.015
1.020	: 1.020
1.025	: 1.025
1.030	: 1.030
1.035	: 1.035

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



PC-1022

Page 16 of 18

Metropolis Healthcare Ltd., EQAS

Analyte Methodwise Result Report

Lab : 837

Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

Clinical Path - Urine Routine Chemistry, Urobilinogen (urine), -


	N
All Methods	375
Reflectance Photometry - (Your Method)	68
TransAsia Laura urine analyser - (Your Analyzer)	21

Evaluation Based On - Method wise Peer Grouping

Your Result	Normal
Result Expected	Nor

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

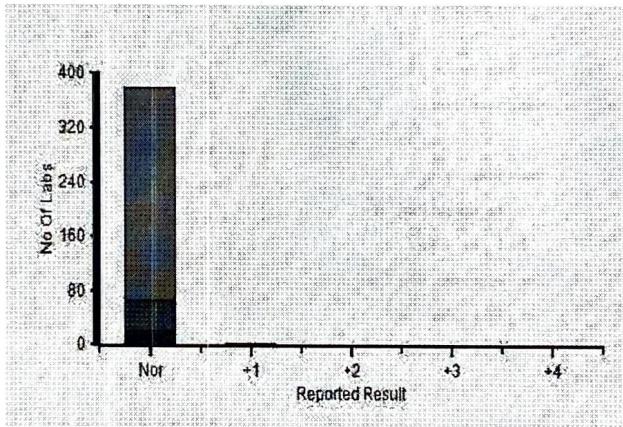

PC-1022

Page 17 of 18

Analyte Methodwise Result Report

Lab : 837


Lab Name : TRUSTLAB DIAGNOSTICS PVT LTD

Report Date : 18/02/2025

Cycle No : 240412

Sample No : 01

Round Open Date : 25/12/2024

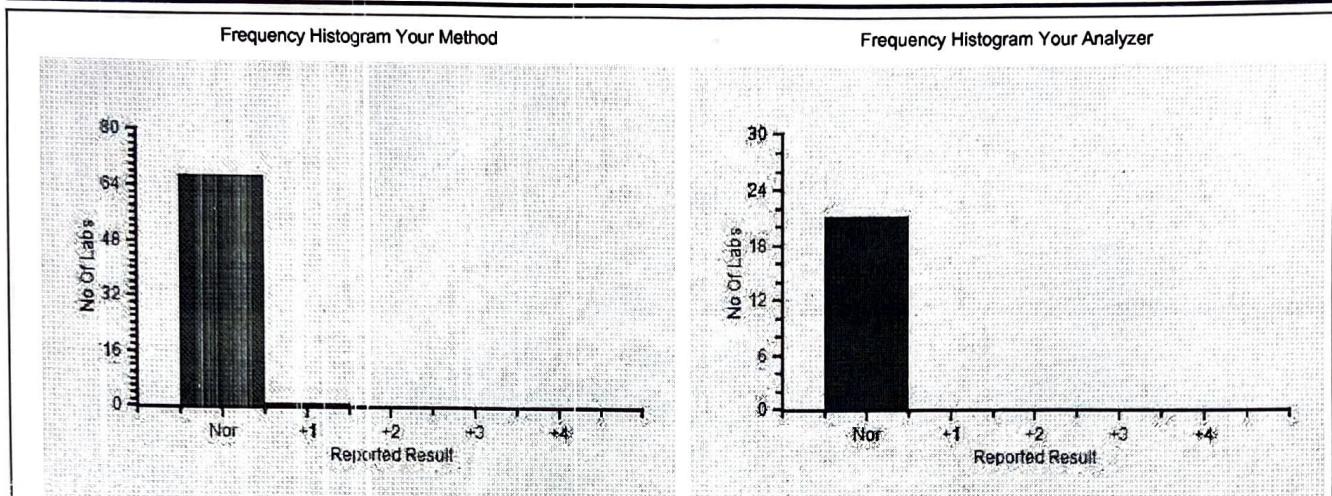

Reported Results Legends :-

Nor	: Normal
+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam
 PT Coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416, 4th Floor,
 Commercial Building - A
 Kohinoor City, Kohinoor Mall, Kurla (W),
 Mumbai - 400070, Maharashtra, India

This is a computer generated report hence signature is not required



PC-1022

End of Report

Page 18 of 18