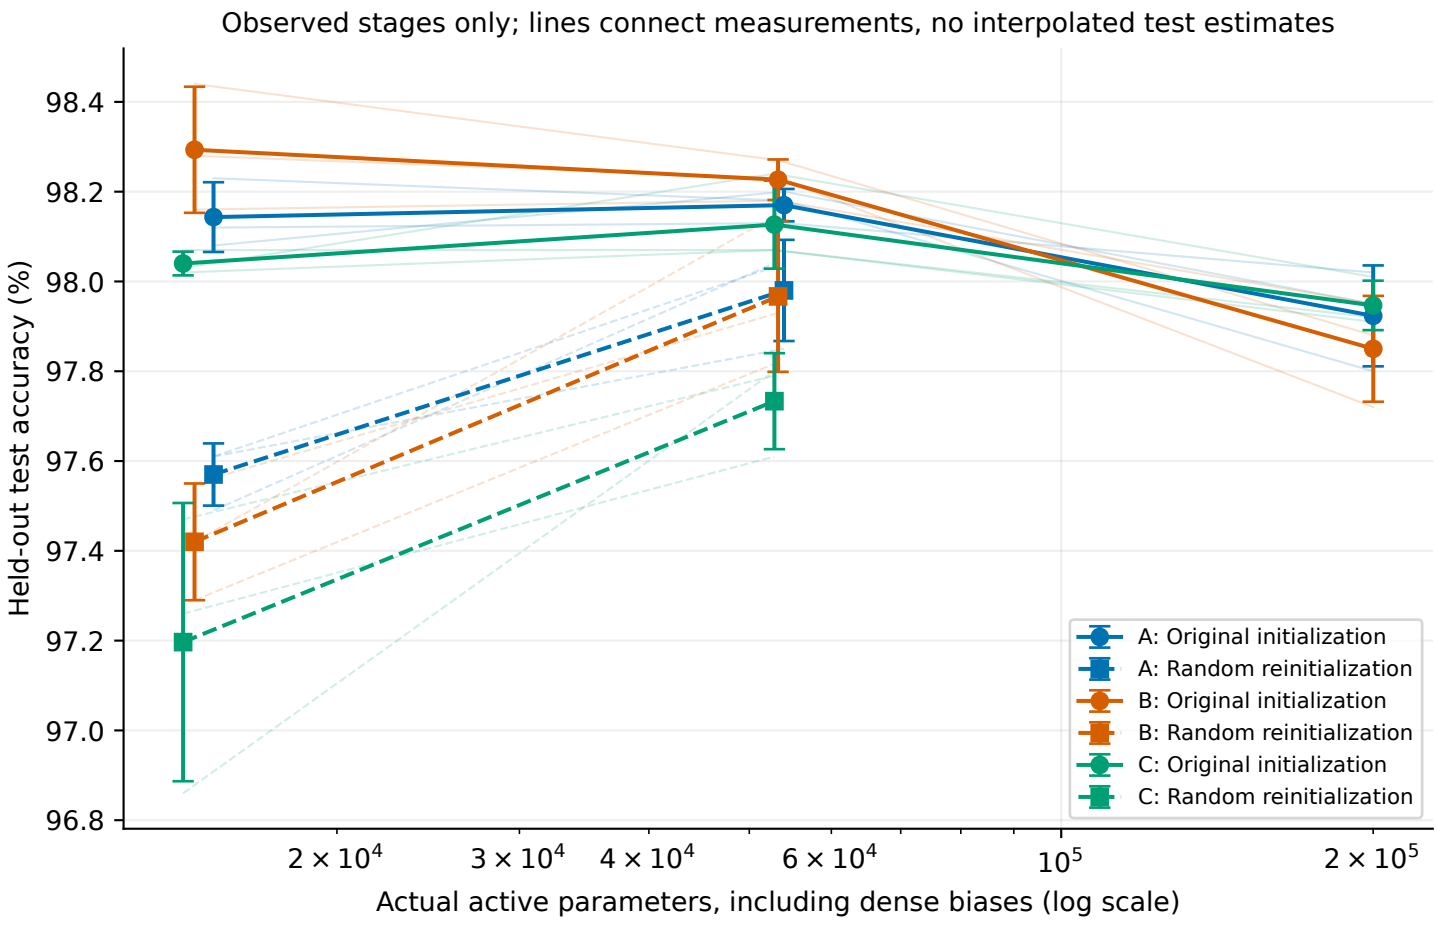
Observed stages only; lines connect measurements, no interpolated test estimates
Held-out test accuracy (%)
98.4
98.2
98.0
97.8
97.6
97.4
97.2
97.0
96.8
2×10^4
3×10^4
4×10^4
6×10^4
10^5
2×10^5
Actual active parameters, including dense biases (log scale)
A: Original initialization
A: Random reinitialization
B: Original initialization
B: Random reinitialization
C: Original initialization
C: Random reinitialization