
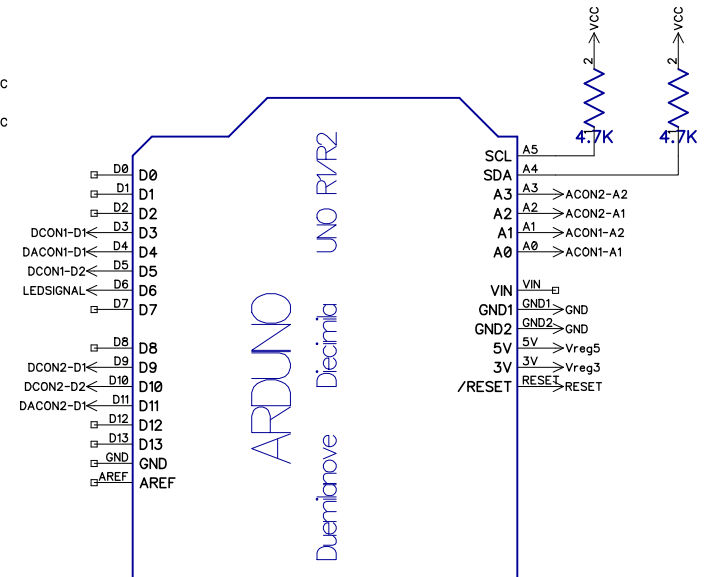
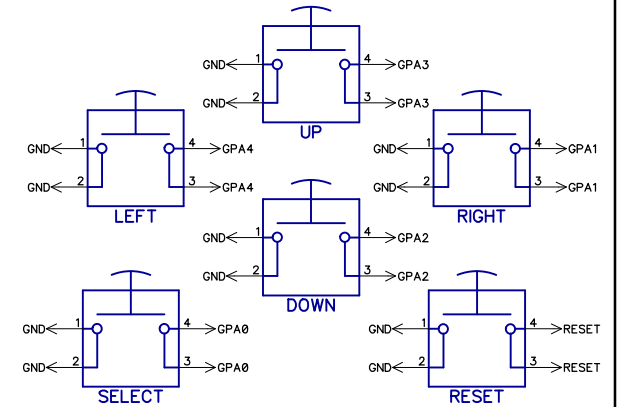
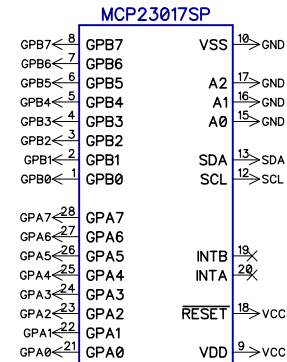
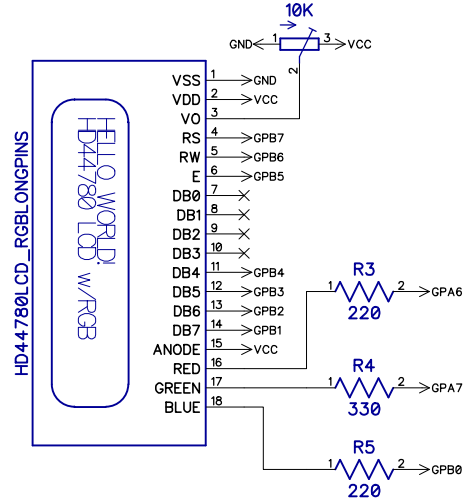




2

1



Note: ACON1/DACON1 Cannot be used at the same time.  
This also applies to ACON2/DACON2

Multi-Affector Homeostasis Device

Paul Warmuth  
10/26/2019 01:08 AM

SIZE FSCM NO.

DWG NO.

REV  
A

SCALE

Sheet 1

2

1