



Instruction Manual  
**optoNCDT 1320**

ILD 1320-10  
ILD 1320-25  
ILD 1320-50  
ILD 1320-100

Intelligent laser optical displacement measurement

MICRO-EPSILON  
MESSTECHNIK  
GmbH & Co. KG  
Königbacher Straße 15

94496 Ortenburg / Germany

Tel. +49 (0) 8542 / 168-0  
Fax +49 (0) 8542 / 168-90  
e-mail [info@micro-epsilon.de](mailto:info@micro-epsilon.de)  
[www.micro-epsilon.com](http://www.micro-epsilon.com)

---

## Contents

<b>1.</b>	<b>Safety .....</b>	<b>9</b>
1.1	Symbols Used .....	9
1.2	Warnings .....	9
1.3	Notes on CE Identification .....	10
1.4	Proper Use .....	11
1.5	Proper Environment .....	11
<b>2.</b>	<b>Laser Class .....</b>	<b>12</b>
<b>3.</b>	<b>Functional Principle, Technical Data .....</b>	<b>14</b>
3.1	Short Description .....	14
3.2	Auto Target Compensation (ATC) .....	15
3.3	Technical Data .....	16
<b>4.</b>	<b>Delivery .....</b>	<b>18</b>
4.1	Unpacking .....	18
4.2	Storage .....	18
<b>5.</b>	<b>Installation .....</b>	<b>19</b>
5.1	Instructions for Installation .....	19
5.1.1	Reflection Factor of the Target Surface .....	19
5.1.2	Error Influences .....	19
5.1.2.1	Light from other Sources .....	19
5.1.2.2	Color Differences .....	20
5.1.2.3	Surface Roughness .....	20
5.1.2.4	Temperature Influences .....	20
5.1.2.5	Mechanical Vibration .....	20
5.1.2.6	Movement Blurs .....	20
5.1.2.7	Angle Influences .....	21
5.1.3	Optimizing the Measuring Accuracy .....	21
5.2	Mounting, Dimensions .....	22
5.3	Indicator Elements at Sensor .....	24
5.4	Electrical Connections .....	25
5.4.1	Connection Possibilities .....	25
5.4.2	Pin Assignment .....	27
5.4.3	Supply Voltage .....	28

---

5.4.4	Laser on .....	28
5.4.5	RS422 Connection with USB Converter IF2001/USB .....	29
5.4.6	Analog Output .....	29
5.4.7	Multifunctional Input .....	30
5.4.8	Digital Output.....	31
5.4.9	Sensor Cable.....	32
<b>6.</b>	<b>Operation .....</b>	<b>33</b>
6.1	Getting Ready for Operation .....	33
6.2	Operation via Web Interface .....	34
6.2.1	Preconditions.....	34
6.2.2	Access via Web Interface .....	36
6.2.3	Measurement Presentation via Web Browser .....	38
6.2.4	Video Signal via Web Browser .....	40
6.3	Programming via ASCII Commands .....	42
6.4	Timing, Measurement Value Flux .....	42
<b>7.</b>	<b>Set Sensor Parameter .....</b>	<b>43</b>
7.1	Preliminary Remarks to the Adjustments .....	43
7.2	Overview Parameter.....	43
7.3	Inputs .....	44
7.4	Signal Processing.....	44
7.4.1	Preliminary Remark .....	44
7.4.2	Measurement Task .....	45
7.4.3	Measuring Rate .....	46
7.4.4	Triggering.....	47
7.4.4.1	General .....	47
7.4.4.2	Signal Processing - Value Output Trigger .....	49
7.4.5	Peak Selection.....	50
7.4.6	Error Handling .....	50
7.4.7	Zeroing and Mastering .....	51
7.4.7.1	Zeroing, Mastering with Select Key .....	52
7.4.7.2	Zeroing, Mastering with Hardware Input .....	53

---

7.5	Outputs .....	54
7.5.1	Overview .....	54
7.5.2	Digital Output, RS422 .....	55
7.5.2.1	Values, Ranges .....	55
7.5.2.2	Characteristics Digital Output .....	57
7.5.3	Analog Output Scaling .....	59
7.5.3.1	Output Scaling .....	59
7.5.3.2	Output Scaling with Key Select .....	60
7.5.3.3	Output Scaling via Hardware Input .....	61
7.5.3.4	Calculation of Measuring Value using Analog Current .....	62
7.5.3.5	Characteristics Distance Value and Analog Output .....	64
7.5.3.6	Mastering and Teaching Analog Output .....	66
7.6	System Settings .....	67
7.6.1	General .....	67
7.6.2	Unit, Language .....	67
7.6.3	Keylock .....	68
7.6.4	Load, Save .....	69
7.6.5	Import, Export .....	71
7.6.6	Access Authorization .....	72
7.6.7	Sensor Reset .....	73
<b>8.</b>	<b>Digital Interfaces RS422 .....</b>	<b>74</b>
8.1	Preliminary Remarks .....	74
8.2	Measurement Data Format .....	74
8.3	Conversion of the Binary Data Format .....	75
<b>9.</b>	<b>Cleaning .....</b>	<b>76</b>
<b>10.</b>	<b>Software Support with MEDAQLib .....</b>	<b>77</b>
<b>11.</b>	<b>Warranty .....</b>	<b>78</b>
<b>12.</b>	<b>Decommissioning, Disposal .....</b>	<b>78</b>
<b>13.</b>	<b>Service, Repair .....</b>	<b>78</b>

---

## **Appendix**

A 1	Optional Accessories .....	79
A 2	Factory Setting .....	80
A 3	ASCII Communication with Sensor .....	81
A 3.1	General .....	81
A 3.2	Overview Commands .....	83
A 3.3	General Commands .....	86
	A 3.3.1 HELP .....	86
	A 3.3.2 GETINFO, Sensor Information .....	86
	A 3.3.3 LANGUAGE, Website .....	86
	A 3.3.4 RESET, Boot Sensor .....	87
	A 3.3.5 RESETCNT, Reset Counter .....	87
	A 3.3.6 ECHO, Switching the Command Reply, ASCII Interface .....	87
	A 3.3.7 PRINT, Sensor Settings .....	88
	A 3.3.8 User Level .....	89
	A 3.3.8.1 LOGIN, Change of the User Level .....	89
	A 3.3.8.2 LOGOUT, Change into User Level .....	89
	A 3.3.8.3 GETUSERLEVEL, User Level Request .....	89
	A 3.3.8.4 STDUSER, Set Standard User .....	89
	A 3.3.8.5 PASSWD, Change Password .....	89
	A 3.3.9 Triggering .....	90
	A 3.3.9.1 TRIGGER, Selection .....	90
	A 3.3.9.2 MFLEVEL, Input Pulse Multifunctional Input .....	90
	A 3.3.9.3 TRIGGERCOUNT, Number of Displayed Measurement Values .....	90
	A 3.3.9.4 TRIGGERSW, Software Trigger Pulse .....	90
	A 3.3.10 Interfaces .....	91
	A 3.3.10.1 BAUDRATE, RS422 .....	91
	A 3.3.10.2 UNIT, Web Interface .....	91
	A 3.3.10.3 MFIFUNC, Function Selection Multifunctional Input .....	91
	A 3.3.10.4 ERRORROUT1, Activate Error Output .....	91
	A 3.3.10.5 ERRORLEVELOUT1, Output Level Digital Output .....	92
	A 3.3.10.6 ERRORLIMIT .....	92
	A 3.3.10.7 ERRORHYSTERESIS .....	92
	A 3.3.10.8 ERROROUTHOLD .....	92

---

A 3.3.11	Handling of Setups.....	93
A 3.3.11.1	IMPORT .....	93
A 3.3.11.2	EXPORT .....	93
A 3.3.11.3	MEASSETTINGS, Load / Save Measurement Settings .....	93
A 3.3.11.4	BASICSETTINGS, Load / Save Device Settings.....	94
A 3.3.11.5	SETDEFAULT, Default Settings .....	94
A 3.3.12	ANALOGSCALE, Scaling the Analog Output.....	94
A 3.3.13	Key Function.....	95
A 3.3.13.1	KEYFUNC, Choose Key Function .....	95
A 3.3.13.2	KEYLOCK, Set Keylock .....	95
A 3.4	Measurement.....	95
A 3.4.1	MEASPEAK, Choice of the Peak in the Video Signal .....	95
A 3.4.2	MEASRATE, Measuring Rate .....	95
A 3.4.3	LASERPOW, Laser Power .....	95
A 3.4.4	Measurement Value Processing.....	96
A 3.4.4.1	MASTERMV, Mastering / Zeroing.....	96
A 3.5	Data Output.....	96
A 3.5.1	OUTPUT, Selection of Measurement Value Output .....	96
A 3.5.2	OUTHOLD, Error Processing .....	96
A 3.5.3	Selection of Measurement Values to be Output .....	97
A 3.5.3.1	GETOUTINFO_RS422, Request Data Selection .....	97
A 3.5.3.2	OUTADD_RS422, Selection of Data Additional Values .....	97
A 3.6	Example Command Sequence During Selection of Measurement Value.....	97
A 3.7	Error Messages.....	98
A 4	Control Menu .....	100
A 4.1	Tab Home.....	100
A 4.2	Tab Settings .....	100
A 4.2.1	Inputs .....	100
A 4.2.2	Signal Processing.....	101
A 4.2.3	Outputs.....	103
A 4.2.4	System Settings.....	105



## 1. Safety

The handling of the sensor assumes knowledge of the instruction manual.

### 1.1 Symbols Used

The following symbols are used in this instruction manual:



#### CAUTION

Indicates a hazardous situation which, if not avoided, may result in minor or moderate injury.



#### NOTICE

Indicates a situation which, if not avoided, may lead to property damage.



Indicates a user action.



#### i

Indicates a user tip.

Measure

Indicates hardware or a button/menu in the software.

### 1.2 Warnings

Avoid unnecessary laser radiation to be exposed to the human body.

- ➡ Switch off the sensor for cleaning and maintenance.
- ➡ Switch off the sensor for system maintenance and repair if the sensor is integrated into a system.

Caution - use of controls or adjustments or performance of procedures other than those specified may cause harm.



Connect the power supply and the display/output device in accordance with the safety regulations for electrical equipment.

- > Danger of injury
- > Damage to or destruction of the sensor



Avoid shock and vibration to the sensor.

- > Damage to or destruction of the sensor

Mount the sensor only to the existing holes on a flat surface. Clamps of any kind are not permitted  
> Damage to or destruction of the sensor

The power supply may not exceed the specified limits.  
> Damage to or destruction of the sensor

Protect the sensor cable against damage. Attach the cable load-free, hold the cable after appr. 25 cm e.g. zip tie.

- > Destruction of the sensor
- > Failure of the measuring device

Avoid continuous exposure to fluids on the sensor.  
> Damage to or destruction of the sensor

Avoid exposure to aggressive materials (washing agent, penetrating liquids or similar) on the sensor.  
> Damage to or destruction of the sensor

### **1.3 Notes on CE Identification**

The following applies to the optoNCDT 1320:

- EU directive 2014/30/EU
- EU directive 2011/65/EU, "RoHS" category 9

Products which carry the CE mark satisfy the requirements of the quoted EU directives and the European standards (EN) listed therein. The EC declaration of conformity is kept available according to EC regulation, article 10 by the authorities responsible at

MICRO-EPSILON MESSTECHNIK  
GmbH & Co. KG  
Königbacher Straße 15  
94496 Ortenburg / Germany

The sensor is designed for use in industry and satisfies the requirements.

## 1.4 Proper Use

- The optoNCDT 1320 system is designed for use in industrial and laboratory areas.
- It is used
  - for measuring displacement, distance, position and thickness
  - for in-process quality control and dimensional testing
- The sensor may only be operated within the limits specified in the technical data, see Chap. [3.3](#).
- Use the sensor in such a way that in case of malfunctions or failure personnel or machinery are not endangered.
- Take additional precautions for safety and damage prevention for safety-related applications.

## 1.5 Proper Environment

- Protection class: IP 65 (applies only when the sensor cable is plugged in)

Lenses are excluded from protection class. Contamination of the lenses leads to impairment or failure of the function.

- Operating temperature: 0 °C ... 50 °C (+32 up to +104 °F)
  - Storage temperature: -20 °C ... 70 °C (-4 up to +158 °F)
  - Humidity: 5 - 95 % (non-condensing)
  - Ambient pressure: Atmospheric pressure
- The protection class is limited to water, no penetrating liquids or similar!



## 2. Laser Class

The optoNCDT 1320 sensors operate with a semiconductor laser with a wavelength of 670 nm (visible/red). The sensors fall within Laser Class 2 (II). The laser is operated on a pulsed mode, the average power is  $\leq 1 \text{ mW}$ . The pulse frequency depends on the adjusted measuring rate (0.25 ... 2 kHz). The pulse duration of the peaks is regulated depending on the measuring rate and reflectivity of the target and can be 0.3 up to 3999.6  $\mu\text{s}$ .



- Comply with all regulations on lasers!

### CAUTION

Never deliberately look into the laser beam!  
Consciously close your eyes or turn away immediately if ever the laser beam should hit your eyes.

Although the laser output is low looking directly into the laser beam must be avoided. Due to the visible light beam eye protection is ensured by the natural blink reflex. The housing of the optical sensors may only be opened by the manufacturer, see Chap. 11. For repair and service purposes the sensors must always be sent to the manufacturer.

Lasers of Class 2 (II) are not subject to notification and a laser protection officer is not required.

The following warning labels are attached to the sensor cable.




Fig. 1 Laser warning labels on the sensor cable



Fig. 2 Laser warning labels on the sensor housing

During operation of the sensor the pertinent regulations acc. to IEC 60825-1 on „radiation safety of laser equipment“ must be fully observed at all times. The sensor complies with all applicable laws for the manufacturer of laser devices.

Laser operation is indicated by LED, see Chap. [5.3](#).

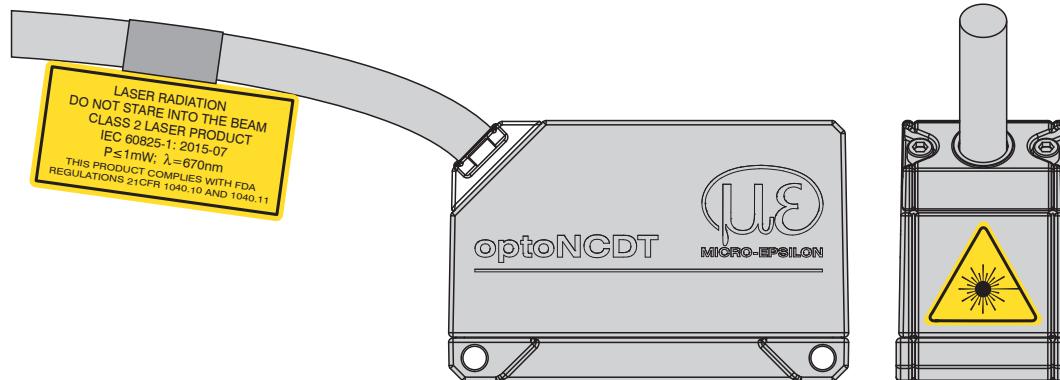

*Fig. 3 True reproduction of the sensor with its actual location of the warning labels, ILD 1320*

- If both warning labels are covered over when the unit is installed the user must ensure that supplementary labels are applied.

### 3. Functional Principle, Technical Data

#### 3.1 Short Description

The optoNCDT 1320 uses the principle of optical triangulation, that is, a visible, modulated point of light is projected onto the target surface.

The diffuse part of the reflection of this point of light is displayed depending on distance on a position-resolving element (CMOS) by an receiver optic which is arranged to the optical axis of the laser beam in a defined angle.

A signal processor in the sensor calculates the distance of the point of light on the measuring object to the sensor by means of the output signal of the CMOS elements. The distance value is linearized and output by means of the analog or RS422 interface.

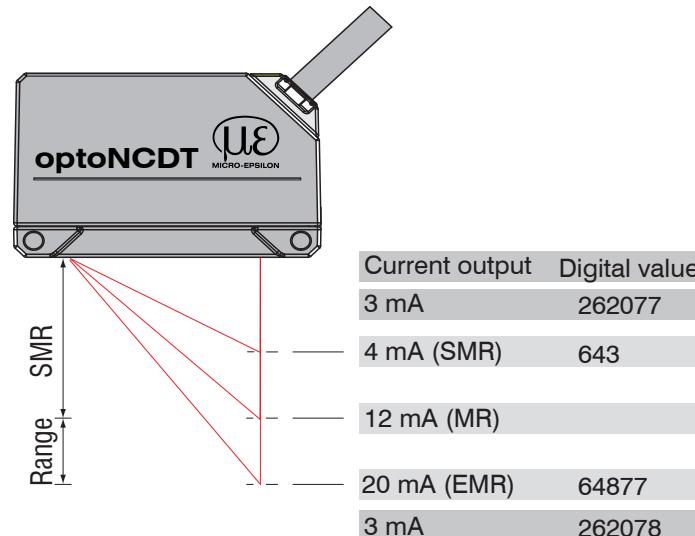


Fig. 4 Definition of terms

### **3.2      Auto Target Compensation (ATC)**

The Auto Target Compensation (ATC) enables stable compensation independent of color and brightness of the measuring object. Also small objects can be detected reliably thanks to the small measuring spot.

### 3.3 Technical Data

Model	ILD1320-10	ILD1320-25	ILD1320-50	ILD1320-100
Measuring range	10 mm	25 mm	50 mm	100 mm
Start of measuring range	20 mm	25 mm	35 mm	50 mm
Midrange	25 mm	37.5 mm	60 mm	100 mm
End of measuring range	30 mm	50 mm	85 mm	150 mm
Linearity <sup>1</sup>	12 µm ≤ 0.12 % FSO	30 µm	60 µm	120 µm
Reproducibility <sup>2</sup>	1 µm	2.5 µm	5 µm	10 µm
Measuring rate	0.25 kHz / 0.5 kHz / 1 kHz / 2 kHz			
Light source	semiconductor laser <1 mW, 670 nm (red)			
Permissible ambient light	10,000 lx			
Spot diameter ± 10 %	SMR	90 x 120 µm	100 x 140 µm	90 x 120 µm
	MMR	45 x 40 µm	120 x 130 µm	230 x 240 µm
	EMR	140 x 160 µm	390 x 500 µm	630 x 820 µm
	smallest ø	45 x 50 µm at 24 mm	55 x 50 µm at 31 mm	70 x 65 µm at 42 mm
Laser safety class		class 2 IEC 60825-1: 2015-07		
Temperature stability		± 0.03 % FSO/°C		
Operation temperature		0 ... +50 °C (non-condensing)		
Storage temperature		-20 ... +70 °C (non-condensing)		
Output	analog	4 ... 20 mA; 12 bit free scalable within the nominal range		
	digital	RS422 / 16 bit resp. 18 bit		
Vibration		20 g / 20 ... 500 Hz (acc. to IEC 60068-2-6)		
Shock		15 g / 6 ms / 3 axes (acc. to IEC 60068-2-29)		

Weight	with cable 3m	approx. 145 g
Control I/O	input <sup>3</sup>	laser on/off; functional input: trigger / zero-setting / mastering / teaching
	output <sup>4</sup>	error output, threshold
Sensor cable <sup>5</sup>		3 m, integrated, open ends
LED		2 x 3 color LEDs for power and status
Key		select key for zero / teaching / factory setting
Power supply		11-30 V DC, 24 V P< 2 W
Controller		integrated signal processor

The specified data apply for a diffusely reflecting matt white ceramic target.

FSO = Full scale output

SMR = Start of measuring range; MR = Midrange; EMR = End of measuring range

1) Values are valid from 0 to 50 % FSO resp. 51 to 100 % FSO.

2) Measuring rate 1 kHz, median 9

3) not galvanically isolated, level: HTL

4) not galvanically isolated, switching characteristics: NPN, PNP, PUSH-PULL

5) not cable carriers suitable

## 4. Delivery

### 4.1 Unpacking

- 1 Sensor ILD 1320
- 1 Assembly instruction
- 1 CD with program <ILD1320 DAQ Tool.exe> and instruction manual
- 1 Calibration protocol
- Accessories (2 pieces screw M2 and 2 pieces washer)

- ➡ Carefully remove the components of the measuring system from the packaging and ensure furthermore that the goods are forwarded in such a way that no damage will occur.
- ➡ Check the delivery for completeness and shipping damage immediately after unpacking.
- ➡ In case of damage or missing parts, please contact the manufacturer or supplier immediately.

See Appendix for further accessories, see Chap. A 1

### 4.2 Storage

Storage temperature: -20 up to +70 °C (-4 °F up to +158 °F)

Humidity: 5 - 95 % (non-condensing)

## 5. Installation

### 5.1 Instructions for Installation

#### 5.1.1 Reflection Factor of the Target Surface

In principle the sensor evaluates the diffuse part of the reflected laser light.

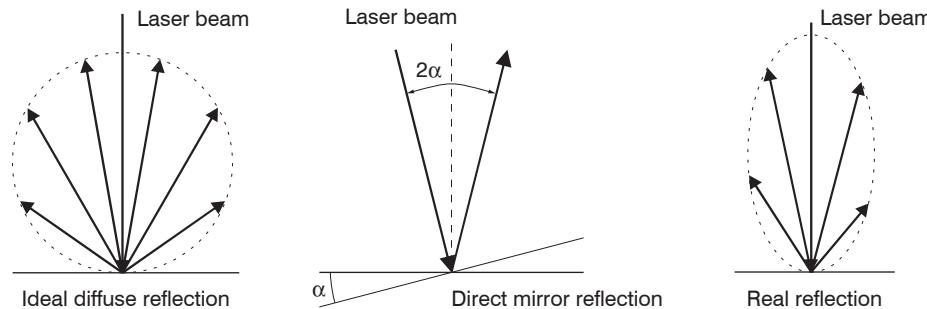


Fig. 5 Reflection factor of the target surface

A statement concerning a minimum reflectance is difficult to make because even a small diffuse fraction can be evaluated from highly reflecting surfaces. This is done by determining the intensity of the diffuse reflection from the CMOS signal in real time and subsequent compensation, see Chap. 3.2. Dark or shiny objects being measured, e.g. black rubber, may require longer exposure times. The exposure time is dependent on the measuring rate and can only be increased by reducing the sensor's measuring rate.

#### 5.1.2 Error Influences

##### 5.1.2.1 Light from other Sources

Thanks to their integrated optical interference filters the optoNCDT 1320 sensors offer outstanding performance in suppressing light from other sources. However, this does not preclude the possibility of interference from other light sources if the objects being measured are shiny and if lower measuring rates are selected. Should this be the case it is recommended to use suitable shields to screen the other light sources. This applies in particular to measurement work performed in close proximity to welding equipment.

### 5.1.2.2 Color Differences

Because of intensity compensation, color difference of targets affect the measuring result only slightly. However, such color differences are often combined with different penetration depths of the laser light into the material. Different penetration depths then result in apparent changes of the measuring spot size. Therefore color differences in combination with changes of penetration depth may lead to measuring errors.

### 5.1.2.3 Surface Roughness

In case of traversing measurements surface roughnesses of  $5 \mu\text{m}$  and more lead to an apparent distance change (also-called surface noise). However, they can be damped by averaging.

### 5.1.2.4 Temperature Influences

When the sensor is commissioned a warm-up time of at least 20 minutes is required to achieve uniform temperature distribution in the sensor. If measurement is performed in the micron accuracy range, the effect of temperature fluctuations on the sensor holder must be considered. Due to the damping effect of the heat capacity of the sensor, sudden temperature changes are only measured with delay.

### 5.1.2.5 Mechanical Vibration

If the sensor is to be used for resolutions in the  $\mu\text{m}$  to sub- $\mu\text{m}$  range, special care must be taken to ensure stable and vibration-free mounting of sensor and target.


### 5.1.2.6 Movement Blurs

If the objects being measured are fast moving and the measuring rate is low, it is possible that movement blurs may result. Always select a high measuring rate for high-speed operations, therefore, in order to prevent errors.

### 5.1.2.7 Angle Influences


Tilt angles of the target in diffuse reflection both around the X and the Y axis of less than 5 ° only have a disturbing effect with surfaces which are highly reflecting.

These influences have to be explicitly considered when scanning profiled surfaces. Basically the angle behavior of triangulation is liable to the reflectivity of the measuring object surface.

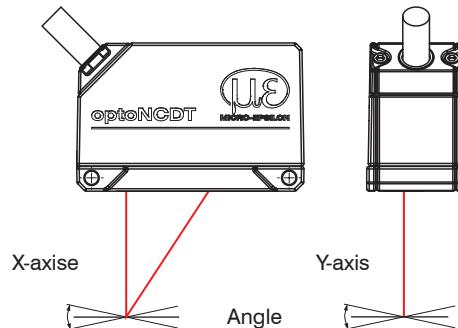


*Fig. 6 Measurement errors through tilting with diffuse reflection*

### 5.1.3 Optimizing the Measuring Accuracy

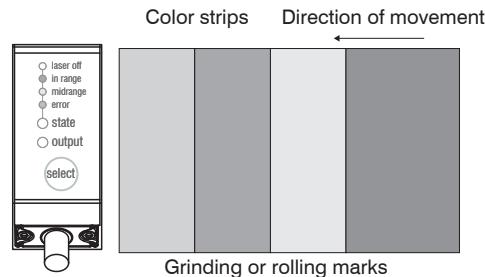

In case of rolled or polished metals that are moved past the sensor the sensor plane must be arranged in the direction of the rolling or grinding marks. The same arrangement must be used for color strips.

*Fig. 7 Sensor arrangement in case of ground or striped surfaces*

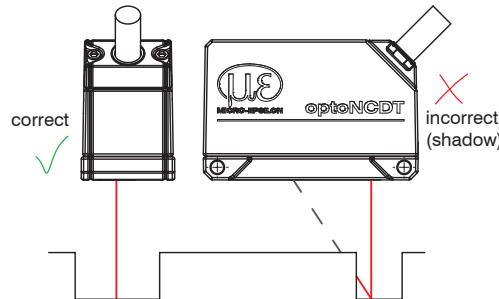

In case of bore holes, blind holes and edges in the surface of moving targets the sensor must be arranged in such a way that the edges do not obscure the laser spot.

*Fig. 8 Sensor arrangement for holes and ridges*

## 5.2 Mounting, Dimensions

The optoNCDT 1320 sensor is an optical system for measurements with micrometer accuracy. The laser beam must be directed perpendicularly onto the surface of the target. In case of misalignment it is possible that the measurement results will not always be accurate.


- Make sure it is handled carefully when installing and operating.
- i** Mount the sensor by means of 2 screws type M3 or by means of through bores for M2 with the screws from the accessories.

Bolt connection					
Through length	Screw depth	Amount	Screw	Washer	Torque
20 mm	min 5 mm	2	M2 x 25 ISO 4762-A2	A2.2 ISO 7089-A2	0.5 Nm ( $\mu = 0.2$ )
	min 4.8 mm, max 20 mm	2	M3 ISO 4762-A2		1 Nm ( $\mu = 0.12$ )
Direct fastening					

*Fig. 9 Mounting conditions*

The bearing surfaces surrounding the fastening holes (through-holes) are slightly raised.

- Mount the sensor only to the existing holes on a flat surface. Clamps of any kind are not permitted. Do not exceed torques.

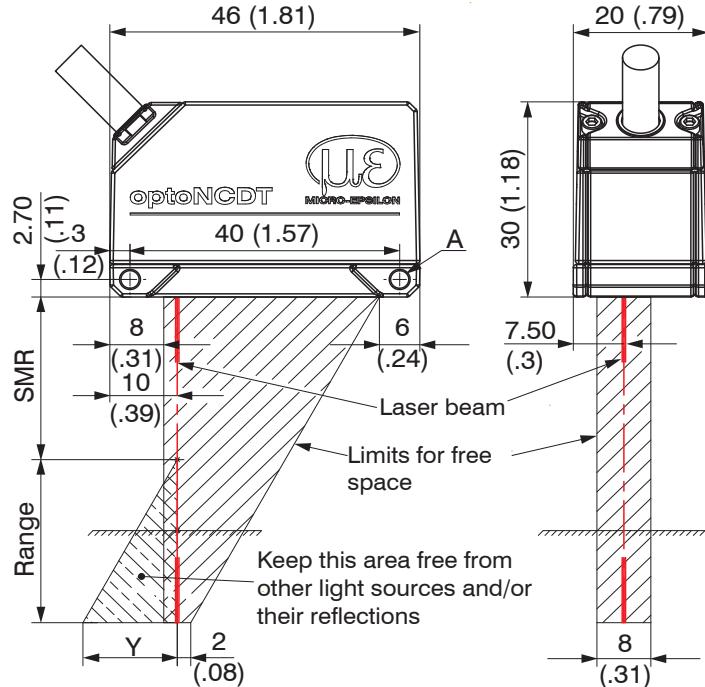


ILD 1320-		10	25	50	100
Range	mm	10	25	50	100
SMR	mm	20	25	35	50
EMR	mm	30	50	85	150
Y	mm	10	21	28	46

Fig. 10 Dimensional drawing and free space for optics and optical free space

A: 2x M3 for direct fastening or  
2x M2 for bolt connection

### 5.3 Indicator Elements at Sensor

LED State	Meaning
green	Measuring object within sensor range
yellow	Mid range
red	Error - e.g. Poor target or out of range
off	Laser off
LED Output	Meaning
green	RS422 measurement value output
yellow	RS422 and current output are switched off. The RS422 and the current output can be switched on. Web interface can also be switched on.
red	Current 4 ... 20 mA measurement value output
off	Sensor off, no supply

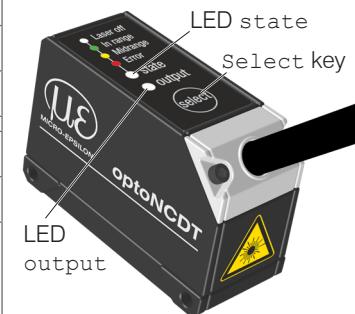

The programmable touch key `select` calls up the functions `Masters` and `Teaching`. By factory default this key is only active for the first 5 minutes after power up. After that it will be automatically locked. The keylock can be programmed via internal websites or ASCII commands.

## 5.4 Electrical Connections

### 5.4.1 Connection Possibilities

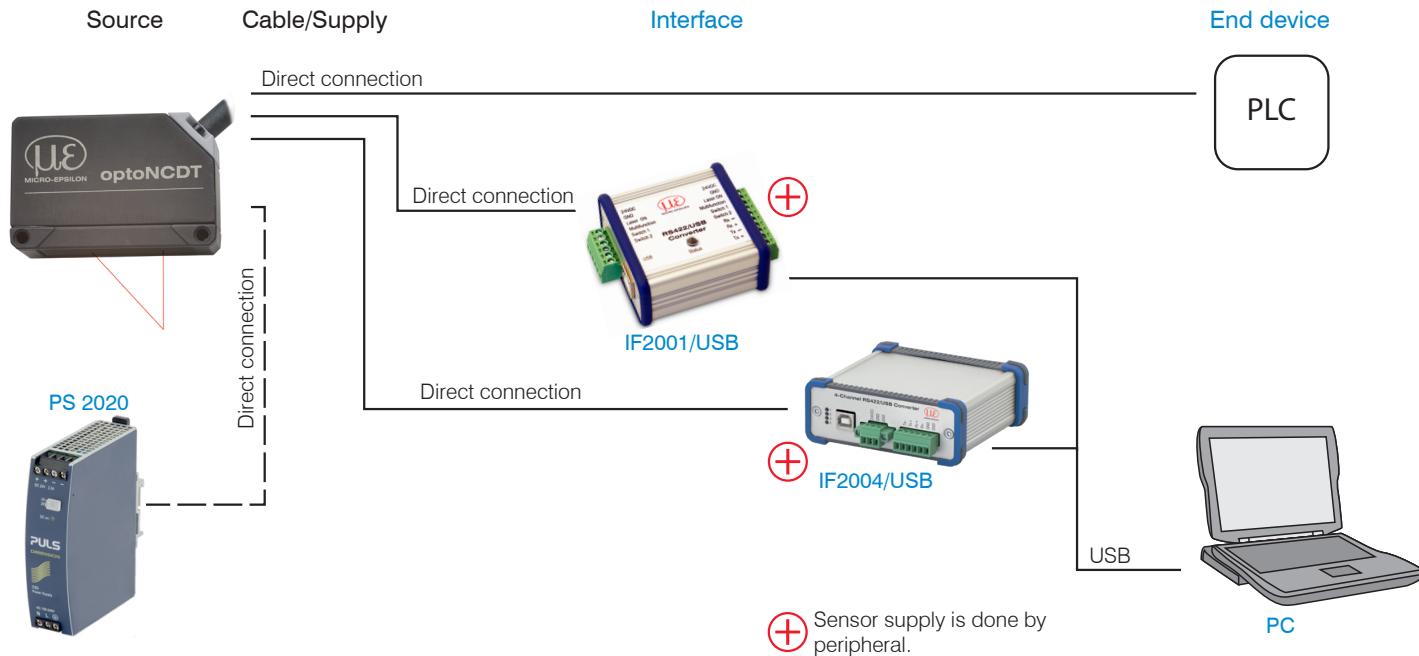



Fig. 11 Connection examples on ILD 1320

The different periphery devices can be connected to the sensor by the illustrated connections, see Fig. 11. The converters IF2001/USB and IF2004/USB also supply the operating voltage (24 V DC) of the sensor. Power to the converters is supplied e. g. by the optional power supply PS 2020.

Peripheral	Sensor channels	Interface
IF2001/USB, RS422 USB converter	one	RS422
IF2004/USB	one	
SPS, ILD 1320 or the like	---	Functional input: trigger
Switch, key, PLC or the like	---	Switching input laser On/Off

*Fig. 12 Max. sensor channels on the peripheral devices*

## 5.4.2 Pin Assignment

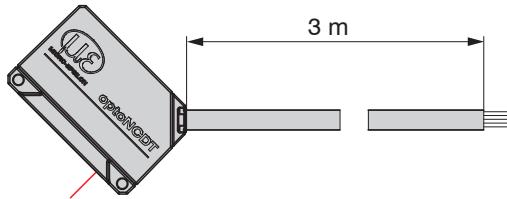

The shielding of the cable is connected to the sensor housing. The sensor cable is not cable carriers suitable. One end is molded on the sensor, the other end has free leads with ferrules.


ILD1320 with open ends

Sensor cable	Description		Specification
green	RS422 Rx+	Serial input	Internally terminated with 120 Ohm
yellow	RS422 Rx-		
gray	RS422 Tx+	Serial output	Terminate externally with 120 Ohm
pink	RS422 Tx-		
red	+U <sub>B</sub>	Supply voltage	11 ... 30 VDC, typ. 24 VDC, P < 2 W
black	Laser on/off	Switch input	Laser is active, if input is connected with GND
violet	Functional input		Trigger, Zero/Master, Teaching
brown	Error	Digital output	I <sub>max</sub> = 100 mA, U <sub>max</sub> = 30 VDC, Programmable switching characteristic: (NPN, PNP, Push-Pull)
white	I <sub>OUT</sub>	4 ... 20 mA	R <sub>Load</sub> = 250 Ohm: U <sub>OUT</sub> 1 ... 5 V with U <sub>B</sub> > 11 V R <sub>Load</sub> = 500 Ohm: U <sub>OUT</sub> 2 ... 10 V with U <sub>B</sub> > 17 V
blue	GND	Ground potential	Supply and signal ground
Shield	Connector housing	Sensor housing	Connect with potential equalization

### 5.4.3 Supply Voltage

Nominal value: 24 V DC (11 ... 30 V, P < 2 W).

- Switch on the power supply unit once wiring is completed.
- Connect the inputs "red" and "blue" at the sensor with a 24 V voltage supply.



Wire color	Supply
red	+U <sub>B</sub>
blue	Ground

Use the supply voltage for measurement instruments only and not for drive units or similar sources of pulse interference at the same time.


MICRO-EPSILON recommends using an optional available power supply unit PS2020 for the sensor.

Fig. 13 Connection of supply voltage

### 5.4.4 Laser on

The measuring laser on the sensor is activated via an HTL switch input. This is advantageous if the sensor has to be switched off for maintenance or similar. Switching can be done with a transistor (for example open collector in an optocoupler) or a relay contact.

- If the black and blue wire are not connected, the laser is off.

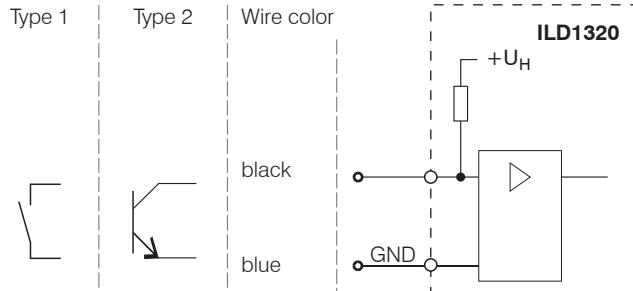

There is no external resistor for current limiting required. Connect the black wire with the blue wire for permanent „Laser on“.

Reaction Time for Laser-On: Correct measuring data are sent by the sensor approximately 1 ms after the laser was switched on.

Fig. 14 Electrical wiring for laser off

### 5.4.5 RS422 Connection with USB Converter IF2001/USB

Cross the lines for connections between sensor and PC.

- i** Disconnect or connect the D-sub connection between RS422 and USB converter when the sensor is disconnected from power supply only.

Sensor		End device (converter) Type IF2001/USB from MICRO-EPSILON
Signal	Sensor cable	
Tx +	grey	Rx + (Pin 3)
Tx -	pink	Rx -(Pin 4)
Rx +	green	Tx + (Pin 1)
Rx -	yellow	Tx -(Pin 2)
GND	blue	GND (Pin 9)



Symmetric differential signals acc. to EIA-422, not galvanically isolated from supply voltage.

Use a shielded cable with twisted cores.

Fig. 15 Pin assignment IF2001/USB


### 5.4.6 Analog Output

The sensor provides a current output 4 ... 20 mA.

- i** The output may not be continuously operated in short circuit operation without load resistor. The short circuit operation leads to durable thermal overload and thus for automatic overload shutdown of the output.

- Connect the white wire and the blue wire on the sensor to a measuring device.

Sensor	
Signal	Sensor cable
I <sub>OUT</sub>	white
GND	blue

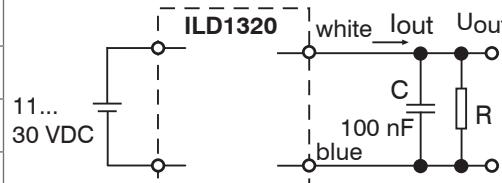

With the adjacent circuit you will get an analog voltage output in the range of 1 ... 5 V. R = 250 Ohm:  
 $U_{OUT} 1 \dots 5 \text{ V at } U_B > 11 \text{ V}$   
 $R = 500 \text{ Ohm: }$   
 $U_{OUT} 2 \dots 10 \text{ V at } U_B > 17 \text{ V}$

Fig. 16 Wiring for voltage output

### 5.4.7 Multifunctional Input

The multifunctional input enables the functions Triggering, Zeroing/Mastering, Teaching. The function is dependent on the programming of the input and of the time behavior of the input signal.

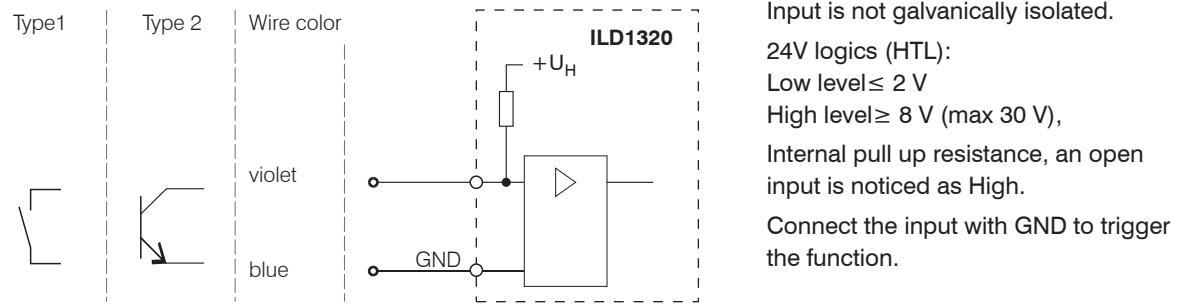


Fig. 17 Electrical wiring for multifunctional input

### 5.4.8 Digital Output

The switching characteristic (NPN, PNP, Push-Pull, Push-Pull negated) of the digital output (Error) depends on the programming.

The NPN output is e.g. suitable for adjustment to TTL logics with an auxiliary voltage  $U_H = +5$  V. The digital output is protected against reverse polarity, overloading (< 100 mA) and over temperature.

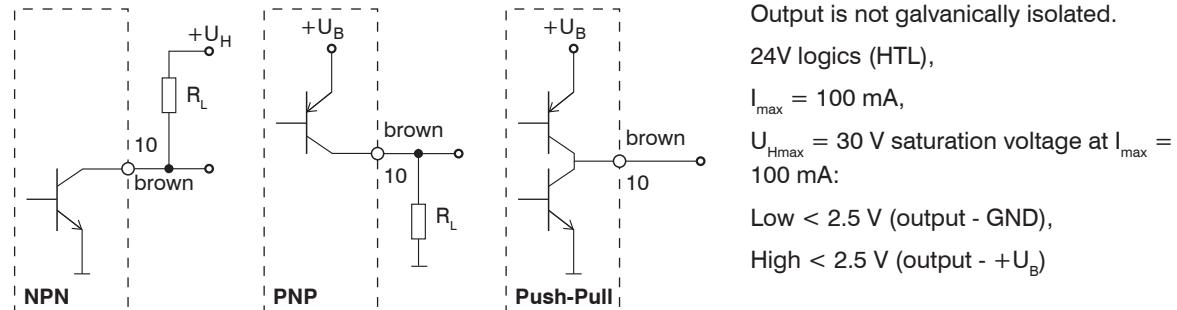



Fig. 18 Electrical wiring digital output

Switching characteristic		
Description	Output active (error)	Output passive (no error)
NPN (Low side)	GND	appr. $+U_H$
PNP (High side)	$+U_B$	appr. GND
Push-Pull	$+U_B$	GND
Push-Pull, negated	GND	$+U_B$

Fig. 19 Switching characteristic digital output

The digital output is activated when measuring object is missing, measuring object too close/too far or when no valid measurement value can be determined.

#### 5.4.9 Sensor Cable

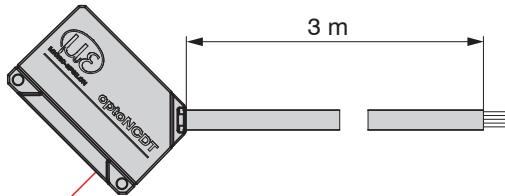

ILD 1320 with open ends

- ▶ Never fall below the bending radius for the sensor cable of 30 mm (fixed) resp. 60 mm (dynamic).
  - i The fixed connected sensor cables are not cable carriers suitable.
  - i Unused open cable ends must be insulated to protect against short circuits or malfunction of the sensor.
- 
- ▶ Avoid excessive pulling to the cables. Provide strain relieves near the connectors when cables > 5 m are vertically free hanging.
  - ▶ Connect the cable shield to the potential equalization (PE, protective earth conductor) on the evaluator (control cabinet, PC housing) and avoid ground loops.
  - ▶ Never lay signal leads next to or together with power cables or pulse-loaded cables (e.g. for drive units and solenoid valves) in a bundle or in cable ducts. Always use separate ducts.

Recommended strand cross-section for self-made connection cables:  $\geq 0.14 \text{ mm}^2$  (AWG 25).

## 6. Operation

### 6.1 Getting Ready for Operation

- ➡ Install and assemble the optoNCDT 1320 in accordance with the instructions set out, see Chap. 5.
- ➡ Connect the sensor with the indicator or monitoring unit and the power supply.

The laser diode in the sensor can only be activated if at the input Laser on/off Pin 8 is connected with Pin 12, see Chap. 5.4.4.

Once the operating voltage has been switched on the sensor runs through an initialization sequence. This is indicated by the momentary activation of all the LEDs. Once initialization has been completed, the sensor transmits a „->“ via the RS422 interface. The initialization takes up to 10 seconds. Within this period, the sensor executes the `Reset` resp. the `Bootloader` command through the key `select` only.

To be able to produce reproducible measurements the sensor typically requires a start-up time of 20 minutes.

If the LED output is off, this means that there is no supply voltage.

If the LED state is off, this means that the laser light source has been switched off.

## 6.2 Operation via Web Interface

### 6.2.1 Preconditions

In the sensor, dynamic Web pages are created that contain the current settings of the sensor and the periphery. The operation is only possible as long as an RS422 connection to the sensor exists.

The sensor is connected to a PC/notebook via a RS422 converter, supply voltage persists.

► Start the program ILD1320 DAQ Tool Vx.x.x.

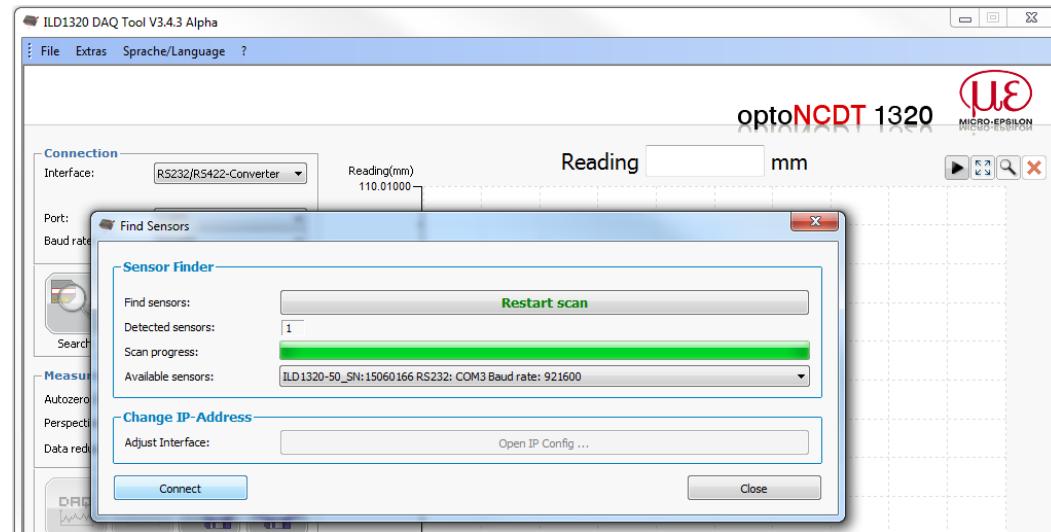


Fig. 20 Auxiliary program for sensor search and to start web interface

The ILD 1320 DAQ tool searches for connected ILD 1320 sensors by means of an internal auxiliary program on available interfaces.

You need a web browser (e.g. Mozilla Firefox or Internet Explorer) on a PC/notebook.

► Choose the desired sensor. Click on the button Connect.

► Choose Configuration in the menu Extras.

► Choose the browser type in dialog Configuration and click on the button .

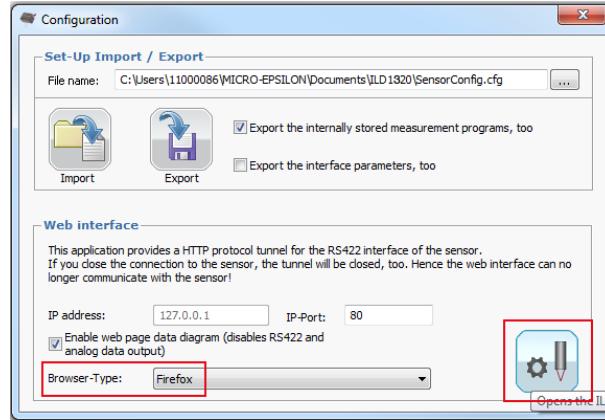


Fig. 21 Dialog configuration web interface

## 6.2.2 Access via Web Interface

► Start the web interface of the sensor, see Chap. 6.2.1

Interactive websites for programming the sensor now appear in the web browser.



In the top navigation bar other auxiliary functions (settings, measurement chart etc.) are available.

The appearance of the websites can change dependent of the functions. Each page contains descriptions of parameters and so tips for filling the website.

*Fig. 22 First interactive website after selection of the web interface*

The sensor is active and supplies measurement values. The ongoing measurement can be operated by means of function buttons in the area Measurement.

By clicking the button in the area Measurement configuration, the change between the saved configurations (presets) for different measuring object surfaces (targets) is done. Choosing a target causes a predefined configuration of the settings which achieves the best results for the chosen material.

Presets	Standard	Ceramics, metal
 Standard		
 Multi-Surface <sup>1)</sup>		Printed circuit boards (PCB), hybrid material
 Light Penetration <sup>1)</sup>		Plastics (Teflon, POM), materials with large penetration depth of the laser
Signal quality	Averaging	Description
	static balanced moving, 128 values balanced moving, 64 values dynamic Median, 9 values no averaging	In the area Signal quality you can switch between four given basic settings (static, balanced, dynamic and no averaging). You can instantly see the reaction in the diagram and system configuration.

The area System configuration displays the current settings for measuring rate and RS422 in blue lettering. Changes to the settings are possible by means of the slide Signal quality or by means of the tab Settings.

The area Diagram type enables the change between graphical display of the measurement value or the video signal, each as value time diagram.

- After programming all the settings are to be stored permanently in a set of parameters. The next time you turn on the sensor they are available again. Therefore use the button Save settings.
- If the sensor starts with user defined measurement setting (setup), see Chap. 7.6.4, changing the signal quality is not possible.

1) Available for the sensor models ILD1320-10/25/50.

### 6.2.3 Measurement Presentation via Web Browser

► Start the measurement value display (Measurement chart) in the horizontal navigation bar.

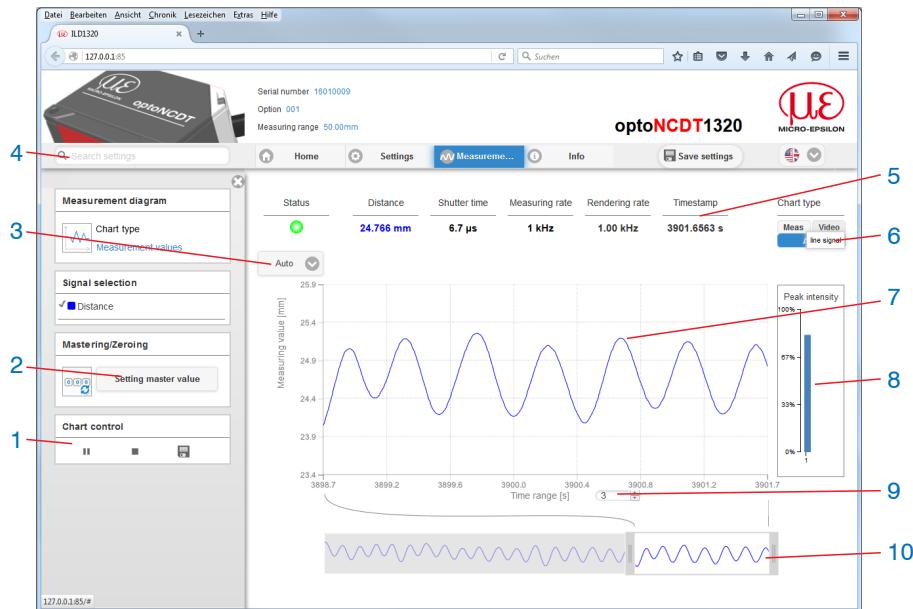


Fig. 23 Website measurement (distance measurement)

- 1 Stop stops the diagram; data selection and zoom function are still possible. Pause interrupts recording. Save opens the Windows selection dialog for file name and storage location to save the last 10,000 values in a CSV file (separation with semicolon).
- 2 This function starts resp. stops a relative measurement. The master value can also be defined in a submenu here.

- 3 For scaling the measurement value axis (y-axis) of the graphics you can either choose **Auto** (= auto-scaling) or **Manual** (= manual setting).
  - 4 The search function enables time-saving access to functions and parameters.
  - 5 In the text boxes above the graphics current values for distance, exposure time, current measuring and display rate and timestamp are displayed.
  - 6 Choice of a diagram type. In the setting **Auto** the diagram type matching the setting is chosen automatically.
  - 7 Mouse over function. When moving the mouse over the graphic in stopped state curve points are marked with a circle symbol and the related values are displayed in text boxes above the graphic. Peak intensity is also updated.
  - 8 The peak intensity is displayed as bar chart.
  - 9 Scaling of the x-axis can be defined by means of a input field below the time axis.
  - 10 Scaling of the x-axis: you can enlarge (zoom) the overall signal by means of the left slider during ongoing measurement. If the diagram is stopped, you can also use the right slider. The zoom window can also be moved by means of the mouse in the middle of the zoom window (arrow cross).
- i** If you leave the diagram display in a separate tab or window of the browser running, you do not have to restart the description each time.
- Click the button **Start**, for starting the display of the measurement results.

### 6.2.4 Video Signal via Web Browser

► Start the video signal display with the function Video in the area Diagram type.

The diagram in the big graphic window on the right displays the video signal of the recipient filed. The video signal in the graphic window displays the intensity distribution above the pixels of the recipient field. 0 % (distance small) on the left and 100 % (distance big) on the right. The related measurement value is marked by means of a vertical line (peak marking).

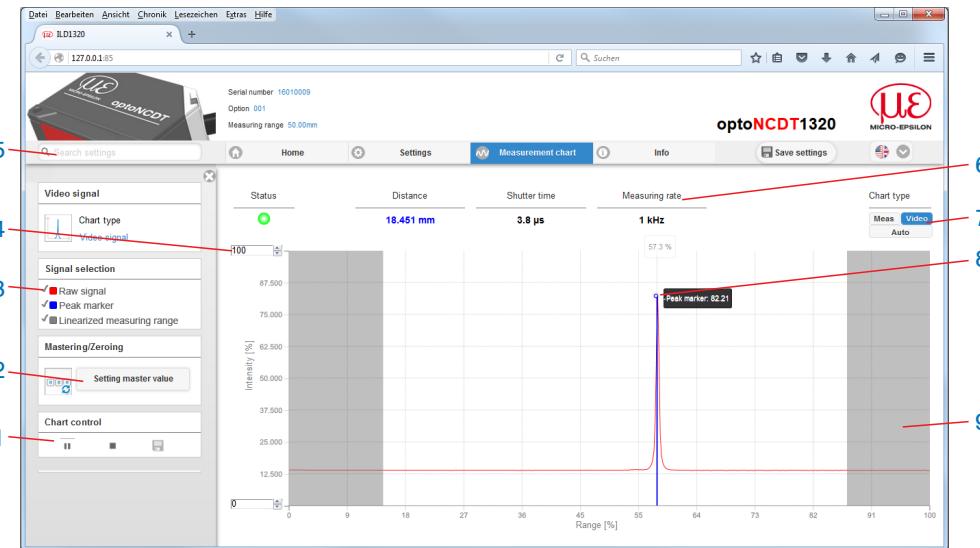


Fig. 24 Display of video signals

- 1 Stop stops the diagram; data selection and zoom function are still possible. Pause interrupts recording. Save opens the Windows selection dialog for file name and storage location to save the last 10,000 values in a CSV file (separation with semicolon).
- 2 This function starts resp. stops a relative measurement. The master value can also be defined in a submenu here.

- 3 The video curves to be displayed while or after measurement can be switched on or off in addition in the left window. Non active curves are highlighted in gray and can be added by clicking the hook. If you only want to see a single signal, then click on its name.
  - Raw signal (uncorrected CMOS signal, red)
  - Peak marking (vertical blue line), corresponds to the calculated measurement value
  - Linearized measuring range (limited by means of gray shading), cannot be changed
- 4 For scaling the measurement value axis (y-axis) of the graphics you can either choose `Auto` (= auto scaling) or `Manual` (= manual setting).
- 5 The search function enables time-saving access to functions and parameters.
  - **i** ASCII commands to the sensor can also be sent via the search function.
- 6 In the text boxes above the graphics current values for distance, exposure time, current measuring and display rate and timestamp are displayed.
- 7 Choice of a diagram type. In the setting `Auto` the diagram type matching the setting is chosen automatically.
- 8 Mouse over function. When moving the mouse over the graphic in stopped state curve points are marked with a circle symbol and the related intensity is displayed. The related x position in % appears above the graphic field.
- 9 The linearized range is between the gray shading in the diagram and cannot be changed. Only peaks which centers are within this range can be calculated as measurement value. The masked range can be limited on request and is additionally limited by means of a light blue shading on the right and on the left. The remaining peaks in the resulting range are used for evaluation.

By displaying the video signal, you can detect effect of the adjustable measurement task (target material), choice of peak and possible interfering signals by means of reflections.

There is no linear relationship between the position of the peaks in the video signal and the output measurement value.

### **6.3 Programming via ASCII Commands**

As an added feature you can program the sensor via an ASCII interface, physically the RS422. This requires, that the sensor must be connected to a serial RS422 interface via a suitable interface converter, see Chap. A 1, to a PC / PLC.

Pay attention in the programs used to the correct RS422 default setting.

Once connected, you can transmit the commands from the appendix, see Chap. A 3, via the terminal to the sensor.

### **6.4 Timing, Measurement Value Flux**

The sensor requires three cycles for measurement and calculation without triggering:

Each cycle takes  $500 \mu\text{s}$  at a measuring rate of 2 kHz. The measured value N is available at the output after three cycles. The delay between acquisition and output is therefore  $1500 \mu\text{s}$ . As the processing in the cycles occurs parallel, after another  $500 \mu\text{s}$ , the next measured value ( $N+1$ ) is output.

## 7. Set Sensor Parameter

### 7.1 Preliminary Remarks to the Adjustments

You can program the optoNCDT 1320 simultaneously in two different ways:

- using a web browser via the ILD 1320 DAQ Tool and the Web interface
- ASCII command set and a terminal program via RS422.

- If you do not save the programming permanently in the sensor, you lost the settings after turning off the sensor.

### 7.2 Overview Parameter

The following parameters can be set or changed in the optoNCDT 1320, see tab Settings.

Inputs	Laser on/off, Multifunctional input, Key function
Signal processing	Measurement task, Measuring rate, Reset counter, Triggering (Data recording, Data output), Evaluation range (ROI), Peak selection, Error handling, Averaging, Zeroing/ Mastering, Data reduction
Outputs	RS422, Analog output, Digital output
System settings	Unit on website, Keylock, Setup management, Import & Export, Access authorization, Reset controller (factory settings)

## 7.3 Inputs

► Go to the menu **Inputs** in the menu **Settings**.

Laser on/off	<i>On / Off</i>		<i>Laser on/off is only effective when pin 8 is connected to GND.</i>	
Multifunctional input	<i>Zeroing (Mastering)</i>	<i>High / Low</i>	<i>Sets the function of the switching input. The Trigger influences capture and export of a measurement value. Zeroing/Mastering sets the current measurement value to the entered master value. Teaching scales the analog output. HTL is defined as active input level.</i>	
	<i>Trigger In</i>	<i>High / Low</i>		
	<i>Teaching</i>			
	<i>Inactive</i>			
Key function	<i>Zeroing (Mastering)</i>		<i>Sets the function of the sensor key. Inactive means keylock.</i>	
	<i>Teaching</i>			
	<i>Inactive</i>			

## 7.4 Signal Processing

### 7.4.1 Preliminary Remark


► Go to the menu **Signal processing** in the tab **Settings**.

A diagram appears according to the prior settings in the area **Diagram type** in the right part of the display. The diagram is active and various settings can be seen immediately. You can find references to the chosen setting below.

The menus for the area **Signal processing** are located in the left part.



Grey shaded fields require a selection.




Value  
Dark-bordered fields require you to specify a value.


### 7.4.2 Measurement Task

The measurement task contains choice of the measuring object (target). The choice of a target loads a pre-defined sensor configuration which achieves the best results for the chosen material.

Measurement task	<i>Standard</i>	<i>Suitable for materials made of ceramics, metal or filled plastics</i>
	<i>Changing surfaces<sup>1</sup></i>	<i>Suitable e.g. for Printed circuit boards (PCB) or hybrid materials</i>
	<i>Material with penetration<sup>1</sup></i>	<i>Suitable for plastics (POM, Teflon), materials with large penetration depth of the laser</i>

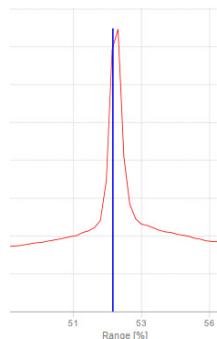

Setting: Standard

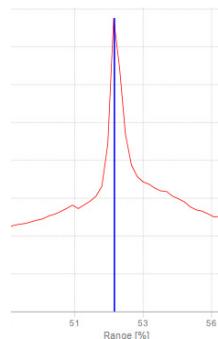

Material with penetration

The choice of measuring object preferences can be observed in the diagram [Video signal](#) on the right by means of the position of the blue peak marking in relation to the video signal (raw signal). It should preferably hit in the area of the highest point (peak) of the video signal.

Fig. 25 Example: Video signals (extract) with measuring object material POM

In the setting **Standard** the peak marking (measurement value) of the plastics example POM does not hit the focus of the real peak as its base is distorted asymmetrically by means of penetration of the laser light. This is possible only if the measurement task was set to **Material with penetration**.

In the setting **Changing surfaces** a compromise between penetration and standard finish is chosen which achieves optimum results for both materials. This can also be seen in the diagram distance values (**Meas**) by means of the different distance values for the respective measurement tasks.

- 1) Available for the sensor models ILD1320-10/25/50.

Grey shaded fields require a selection.

Value  
Dark-bordered fields require you to specify a value.

### 7.4.3 Measuring Rate

The measuring rate indicates the amount of measurements per second.

► Choose the desired measuring rate.


Measuring rate	250 Hz / 500 Hz / 1 kHz / 2 kHz	<i>Use a high measuring rate with light and matt measuring objects. Use a low measuring rate with dark and shiny measuring objects (e.g. black lacquered surfaces) to improve the measuring result.</i>
----------------	---------------------------------	---

With a maximum measuring rate of 2 kHz the CMOS element is exposed 2,000 times per second. The lower the measuring rate, the higher maximum exposure time.

Measuring rate is set to 1 kHz ex works.



Grey shaded fields require a selection.



Value  
Dark-bordered fields require you to specify a value.

## 7.4.4 Triggering

### 7.4.4.1 General


The optoNCDT 1320 measurement output is controllable through an external trigger signal or a command. Triggering affects the analog and digital output. The measurement value at the time of triggering is output delayed, see Chap. 6.4.

- Triggering does not influence the measuring rate resp. the timing so that between the trigger event (level change) and the start of output always lie 3 cycles + 1 cycle (Jitter).
- The multifunctional input is used as external trigger input, see Chap. 5.4.7.
- Factory setting: no triggering, the sensor starts data transmission right after start-up.
- Pulse duration of the “Trigger in“ signal must be at least 50 µs.

<i>Output trigger</i>	<i>Level</i>			<i>A continuous measurement task is following as long as the chosen level remains the same. Choice of level, see Chap. 7.3. Pulse duration must be at least a cycle time. The following pause must be at least a cycle time..</i>
	<i>Edge</i>	<i>infinite</i>		<i>Edge selection, see Chap. 7.3. “0“ end trigger, “1 ... 16382“ values per trigger, “16383“ endless trigger</i>
		<i>manual</i>	<i>Number</i>	<i>Value</i>
	<i>Software</i>	<i>infinite</i>		<i>A software triggering is started by clicking the button Release trigger. “0“ end trigger “1 ... 16382“ values per trigger, “16383“ endless trigger</i>
		<i>manual</i>	<i>Number</i>	<i>Value</i>
<i>Inactive</i>			<i>No triggering</i>	



Grey shaded fields require a selection.



Dark-bordered fields require you to specify a value.

## Implemented trigger conditions:

**Level triggering** with high level / low level.

Continuous measurement input resp. output, as long as the selected level is applied. Then stops the data output.

The pulse duration must be at least one cycle time. The subsequent break must also be at least one cycle time.

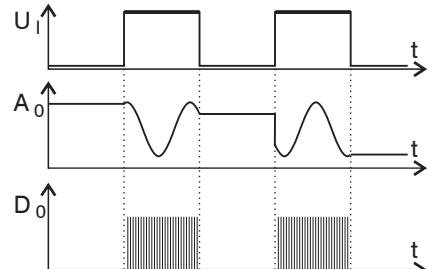


Fig. 26 High trigger level (above) with analog output  $A_o$  and digital output signal  $D_o$  (below)

**Edge triggering** with rising or falling edge.

Starts measured value acquisition resp. output as soon as the chosen edge is applied to the trigger input. The sensor outputs a fixed number of measurement values when trigger conditions have been met. Value range from 1 ... 16383. After termination of data output the analog output sticks to the last value (sample & hold).

Pulse duration must be at least 50  $\mu$ s.

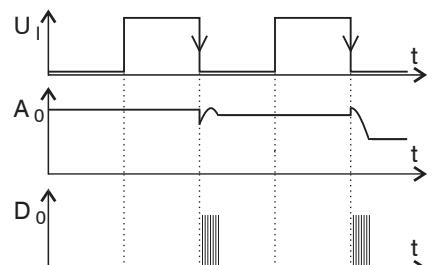


Fig. 27 Trigger edge HL (above) with analog output  $A_o$  and digital output signal  $D_o$  (below)

**Software triggering.** Starts the measurement value output, when a software command comes. The trigger time is defined more inaccurately. After the trigger event the sensor outputs the preset number of measurement values or starts a continuous measurement value output. If "0" is selected for the number of measurement values, the sensor stops the triggering and the continuous value output.

Measurement output can also be stopped by means of a command.

#### **7.4.4.2 Signal Processing - Value Output Trigger**

Measurement values are calculated continuously and independently of the trigger event. A trigger event simply triggers the value output via a digital interface. Therefore, any values measured immediately before the trigger event are included in calculating mean values (averages).

#### 7.4.5 Peak Selection

Peak selection	<i>First peak / highest peak / last peak</i>	<p>Defines, which signal is used for the evaluation in the line signal.</p> <p>First peak: nearest peak to the sensor.</p> <p>Highest peak: standard, peak with the highest intensity.</p> <p>Last Peak: widest peak to the sensor.</p>	
----------------	--	---	--

A correct measuring result can be determined only for the first peak when a measuring object which consists of several transparent layers.

#### 7.4.6 Error Handling

Error handling adjusts the behavior of the analog output and the RS422 interface in the event of an error.

Error handling	Error output, no value	<i>Analog output supplies 3 mA instead of the measurement value. The RS422 interface outputs an error value.</i>	
	Retain last value infinitely	<i>Analog output and RS422 interface stick to the latest valid value.</i>	
	Retain last value	1 ... 1024	Value

If no valid measurement value can be detected, an error is output. If this disrupts further processing, you can alternatively hold the last valid value over a specific period of time i.e. it can be output again. After expiry of the chosen number an error value is output.



Grey shaded fields require a selection.



Value  
Dark-bordered fields require you to specify a value.

#### 7.4.7 Zeroing and Mastering

By zeroing and mastering you can set the measurement value to a set point in the measuring range. The output range is moved thereby. This function makes sense, for example, for several adjacent measuring sensors or in the case of the thickness and planarity measurement.

Master value in mm	<b>Value</b>	<i>Data, for example of the thickness, of a master piece. Value range max. 0 up to + 2 x measuring range</i>
--------------------	--------------	--

Setting masters is used to compensate mechanical tolerances in the measurement setup of the sensors or to adjust the temporal (thermal) changes in the measurement system. The masters measurement, also known as the calibration measurement, is given a set point.

The value which is given during measurement on the sensor output of the “mastering object” is the **master value**. The zero-setting is a characteristic of the mastering, because here the master value is 0.

When mastering the sensor's characteristic is parallel displaced. The displacement of the characteristic curve reduces the usable measurement range of the sensor the further the master value is away from the master position.

##### Sequence for Mastering / Zeroing:

- Bring target and sensor in the desired position together.
- Send the master command.

The master command waits for 2 seconds on the next measurement value and masters it. If no measurement value is received within this time, for example by external triggering, the command returns with the error E220 Timeout back.

After the mastering, the sensor gives new measurement values, related to the master value. The non-mastered condition applies by means of a reset with the button **Inactive**.



Grey shaded fields require a selection.



Value  
Dark-bordered fields require you to specify a value.

- **i** Zeroing/Mastering requires that a target is within the measurement range. Zeroing/Mastering has an influence on the digital and the analog output.

An invalid master value, e. g. no peak available, will be acknowledged with the **E602 Master value is out of range** error.

### 7.4.7.1 Zeroing, Mastering with Select Key



Fig. 28 Flow chart for zeroing, mastering (key select)

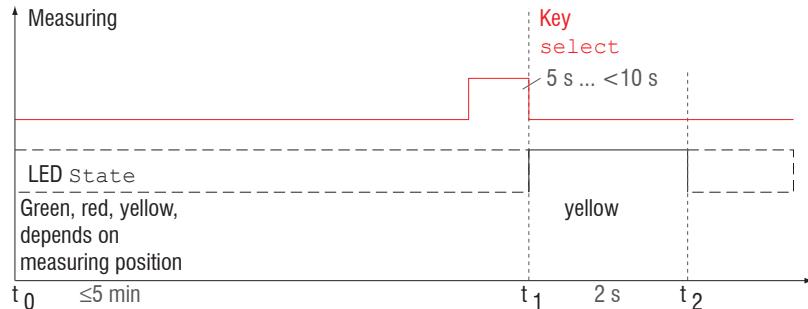


Fig. 29 Flow chart for the return of zero setting and mastering

- 1) The key Select remains without effect since key lock is active.
- 2) The master value is not applied when LED State is red, flash frequency 3 Hz for 2 s.

**i** The key Select is locked according to factory settings after expiry of 5 min. You can unlock the keylock e.g. via the web interface, see Chap. 7.6.3.

The function Zeroing/Mastering can be used several times in succession. Between repetition of the function Zeroing/Mastering a brake of 1 s is necessary. The function Zeroing/Mastering can also be combined with the multifunctional input.

#### 7.4.7.2 Zeroing, Mastering with Hardware Input

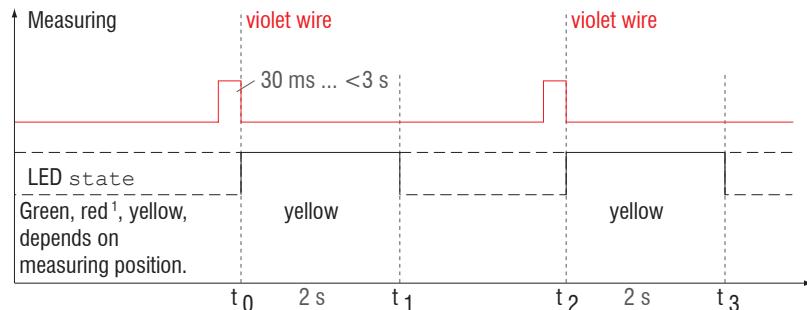


Fig. 30 Flow chart for zeroing, mastering (hardware input)

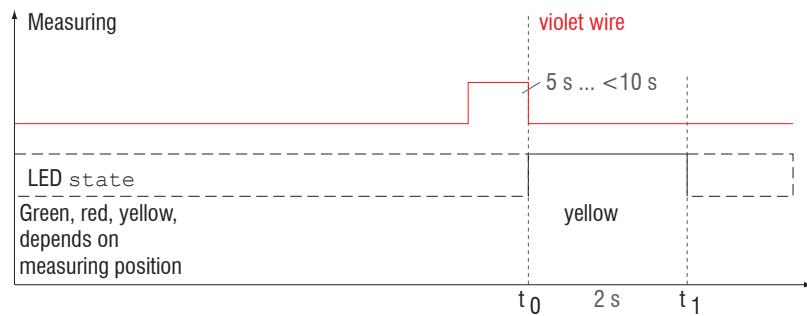


Fig. 31 Flow chart for the return of zero setting and mastering

The function zeroing/mastering can be applied successive in several times. Between repeating the zeroing/mastering function a pause of 1 s is required. The zeroing/mastering function can also be combined with the select key.

- 1) With red State LED, the master value is not accepted, flashes with 8 Hz for 2 s.

**i** A pulse can be made via the functional input (violet wire sensor cable).

Details of the hardware input can be found in the electrical connections, see Chap. 5.4.7.


## 7.5 Outputs

### 7.5.1 Overview

RS422	Baud rate	9.6 / 19.2 / 56.0 / 115.2 / 230.4 ... / 1000 kBps		Transmission rate with binary data format.
	Output data	<i>Distance / Shutter time / Intensity / Sensor state / Measurement counter / Non-linearized focal point / Time stamp / Video raw signal</i>		The data which are provided for the transmission are to activate with the checkbox.
Analog output	<i>Standard scale</i>			Start of measuring range 4 mA, end of measuring range 20 mA
	<i>Two-point scale</i>	Minimum value	Value	Always 2 points which mark the start and end of a new measuring range are taught. Reversal of the output signal is possible with two-point scaling.
		Maximum value	Value	
Error output	Inactive			Adjusts the switching characteristic of the error output (error), see Chap. 5.4.8.
	Full scale error	NPN / PNP / PushPull / PushPullNeg		
Output Interface	Web interface / Analog / RS422			Decides via the used interface for measurement output. A parallel measurement output via multiple channels is not possible. When choosing web interface measurement values are not output via RS422 or current output.



Grey shaded fields require a selection.



Value  
Dark-bordered fields require you to specify a value.

## 7.5.2 Digital Output, RS422

### 7.5.2.1 Values, Ranges

The digital measuring values are being output as unsigned digital values (raw values). 16 resp. 18 bits per value are being transmitted. Subsequently you can find a compilation of output values and the conversion of the digital value.

Value	Length	Variables	Value range	Formula
Distance (without Mastering)	16 bits	x = digital value	[0; <643] SMR reserve [643; 64877] measuring range [>64877; 65520] EMR reserve	$d \text{ [mm]} = \frac{1}{100} \left( \frac{102}{65520} x - 1 \right) * \text{MR} \text{ [mm]}$
		MR = measuring range [mm]	{10/25/50/100}	
		d = distance [mm]	[-0,01MR; 1,01MR]	
Distance (with Mastering)	18 bits	x = digital value	[0; 229320]	The output range is also coded with 64235 values at 18 bit and shifted with the master value, see Fig. 33. The reserves at SMR and EMR are coded with 643 values each.
		MR = measuring range [mm]	{10/25/50/100}	
		MP = master position [mm]	[0; MR]	
		MV = master value [mm]	[0; 2MR]	
		d = distance [mm]		
		MV < MP - 0.5MR:	[-0.5MR + MV; MR - MP + MV]	
		MV ≥ MP - 0.5MR:	[-MP + MV; MR - MP + MV]	
Exposure time	18 bits	x = digital value	[1; 262143]	$\text{ET} \text{ [\mu s]} = \frac{1}{10} x$
		ET = exposure time [\mu s]	[0.1; 26214.3]	
Intensity	16 bits	x = digital value	[0; 65472]	$I \text{ [%]} = \frac{25}{16368} x$
		I = intensity [%]	[0; 100]	

Sensor status	18 bits	x = digital value	[0; 242143]	Bit 0 (LSB): peak starts before ROI
		Bit encoding	[0; 1]	Bit 1: peak ends after ROI
				Bit 2: no peak found
		SMR = Start of measuring range		Bit 5: distance before SMR (extended)
		EMR = End of measuring range		Bit 6: distance after EMR (extended)
				Bit 15: measuring value is triggered
				Bit 16, 17: status LED; - 00 – off            10 – red - 01 – green        11 – yellow
Measurement counter	18 bits	x = digital value	[0; 262143]	
Time stamp	2 words, at 16 bit	x = digital value Lo	[0; 65535]	$t \text{ [ms]} = \frac{1}{100} (65536y + x)$
		y = digital value Hi	[0; 65535]	
Non-linearized focus	18 bits	t = time stamp [ms]	[0; 11h55m49.67s]	$NF \text{ [%]} = \frac{100}{262143} x$
		x = digital value	[0; 262143]	
Video raw signal	16 bits	NF = focus	[0; 100]	
		512 pixel	[0; 65535]	


Additional information transmitted in the distance value

Distance value	Description
262075	data amount to big for selected baud rate
262076	no peak available
262077	peak before the measurement range (MR)
262078	peak behind the measurement range (MR)
262080	measurement value can not be calculated
262081	peak is to large
262082	Laser is off


### 7.5.2.2 Characteristics Digital Output

Measurements are coded with 18 bit, if based on zero setting or mastering. The master value itself can accept the double measuring range. The examples below show the digital output behavior of an ILD1320-50 with 50 mm measuring range.


Target at 16 % measuring range

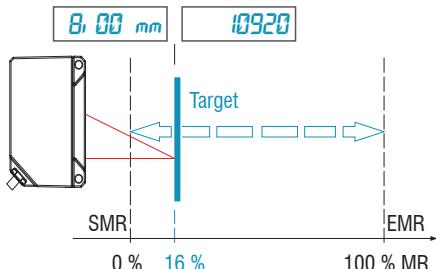


Target at 60 % measuring range

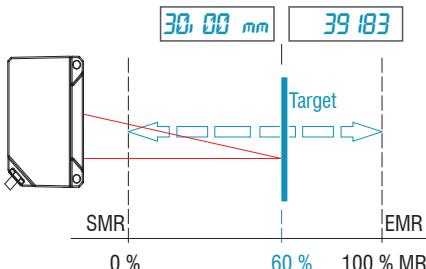


Target at 60 % measuring range

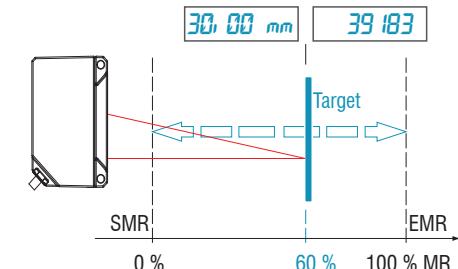


➡ Zero setting (master value = 0 mm)

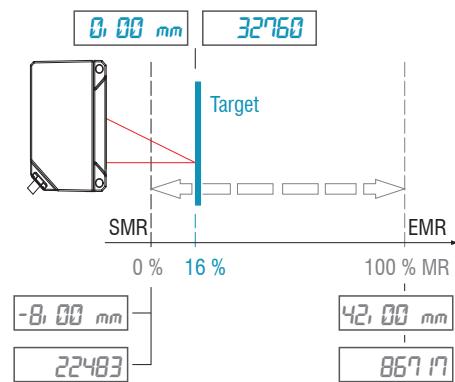

➡ Zero setting (master value = 0 mm)

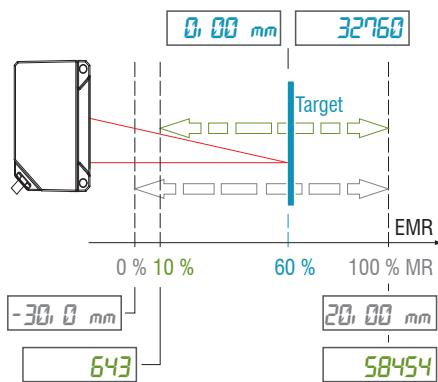

➡ Set master value 10 mm

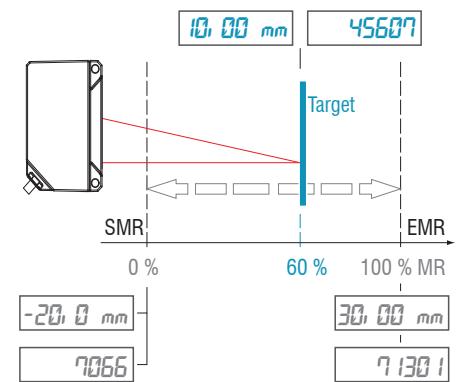

Digital minimum reached at 10 % MR

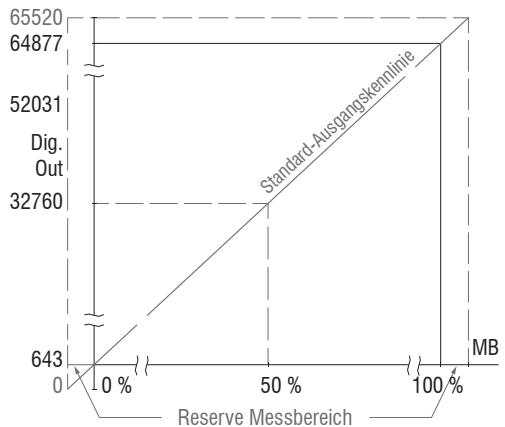


Fig. 32 Digital values without zero setting resp.  
mastering

➡ Set target at 80 % measuring range (40 mm), set master value 100 mm

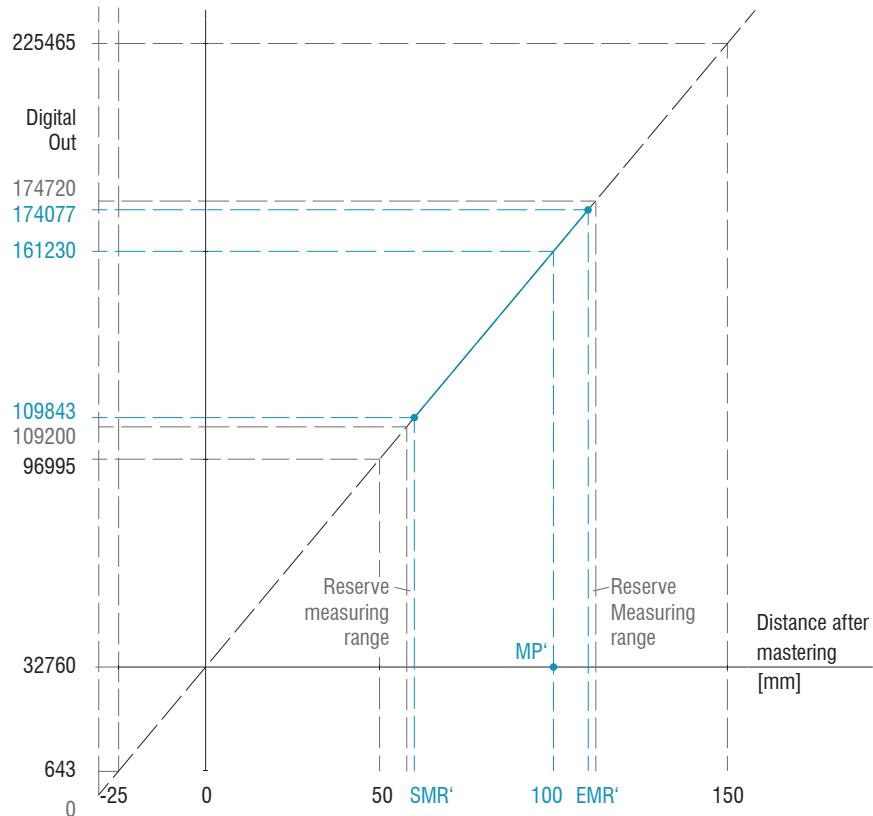


Fig. 33 Digital values of an ILD1320-50 with mastering, master value 100 mm

## 7.5.3 Analog Output Scaling

### 7.5.3.1 Output Scaling

- Max. output range: 4 mA ... 20 mA
- Output gain  $\Delta I_{OUT}$ : 16 mA = 100 % MR
- Error value: 3.0 mA ( $\pm 10 \mu A$ )

The teaching scales the analog output (4 to 20 mA) for a part of the measuring range. This allows you to optimize the resolution for the analog measurement range. Only the current and error output will be affected by the 2 point calibration. Therefore you define a new start and end for the measurement range. This teaching procedure can be performed live via the select key, the multifunctional input or via the webinterface.

- With a user defined output scaling you can use the error output, see Chap. 5.4.8, as a programmable limit switch.

The measurement object positions for Teach 1 and Teach 2 have to differ from each other.

The teaching process requires a valid measuring signal. The teaching process is terminated at

- no target,
- target not evaluated,
- to close to the sensor - beyond SMR or
- to far from the sensor - beyond EMR.

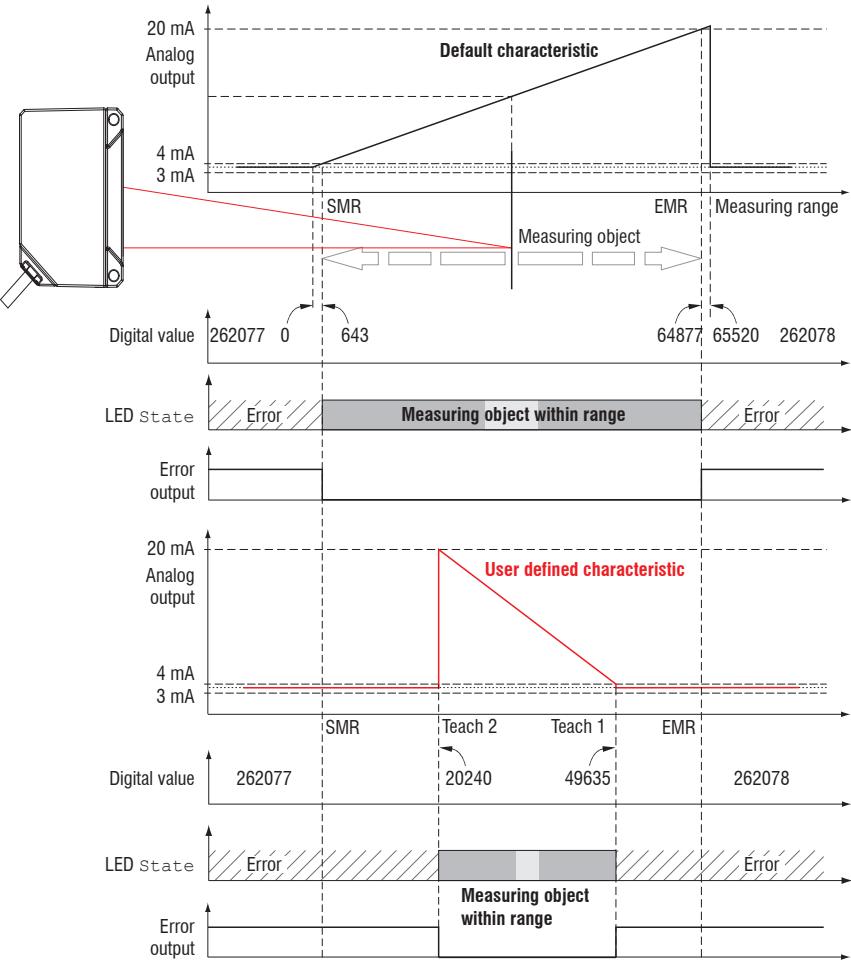


Fig. 34 Default characteristic (black), reverse, user defined characteristic (red)

### 7.5.3.2 Output Scaling with Key Select

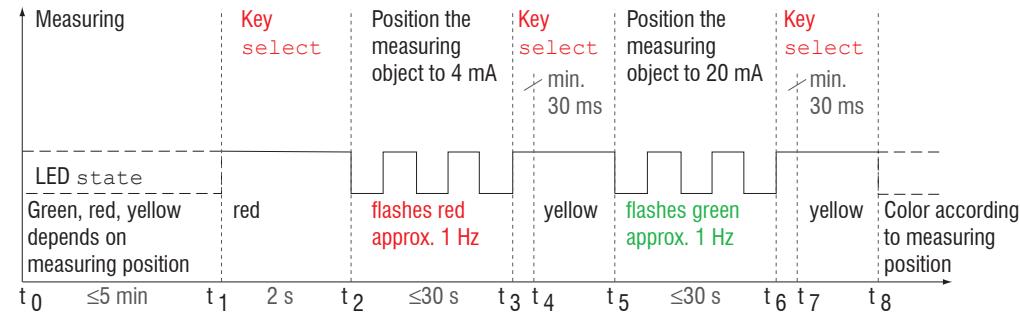


Fig. 35 Flow chart for output scaling

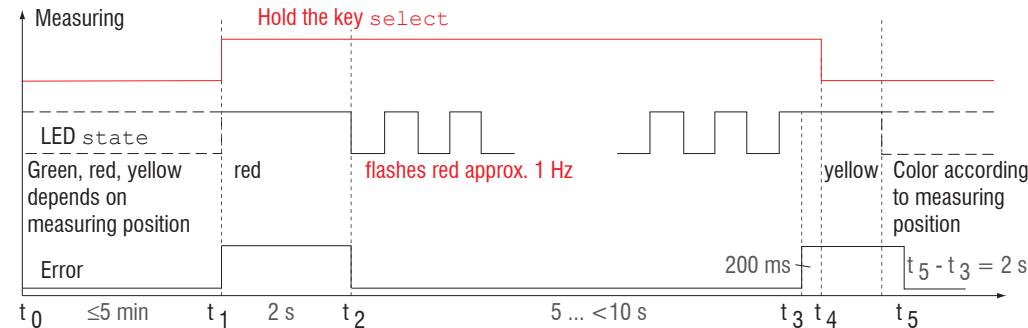


Fig. 36 Flow chart for the return of output scaling

If the key Select is pressed longer than 10 s or not within the timeframe while doing the return of the output scaling, an error is shown via State LED. In this case the State LED is blinking red with 8 Hz for 2 s.

### 7.5.3.3 Output Scaling via Hardware Input

Scaling of the analog output can be made via an impulse at the functional input, the violet wire on the sensor cable.

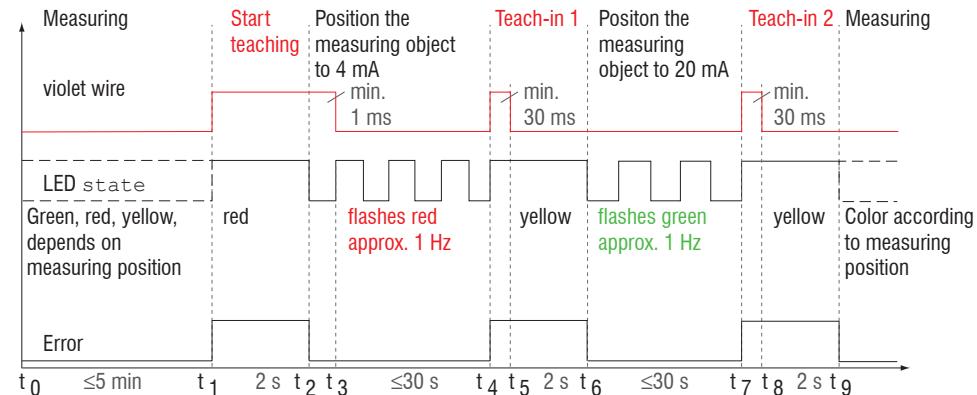


Fig. 37 Flow chart for output scaling

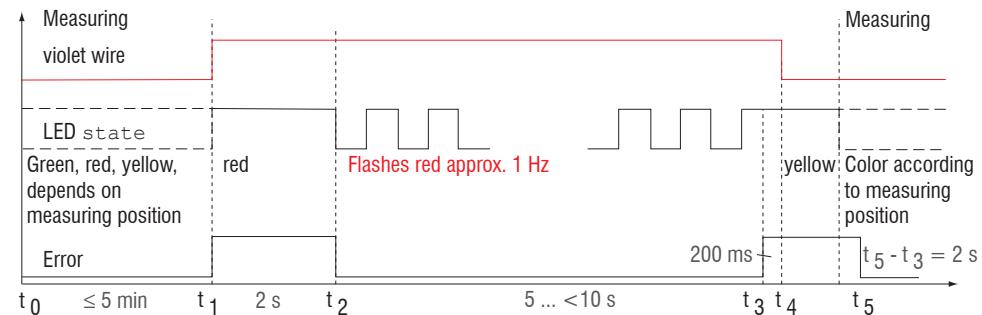


Fig. 38 Flow chart for the return of output scaling

#### 7.5.3.4 Calculation of Measuring Value using Analog Current

Current output (without mastering, without teaching)

Variables	Value range	Formula
$I_{OUT}$ = current [mA]	[3,8; <4] SMR reserve [4; 20] measuring range [>20; 20,2] EMR reserve	$d \text{ [mm]} = \frac{(I_{OUT} \text{ [mA]} - 4)}{16} * MR \text{ [mm]}$
MR = measuring range [mm]	{10/25/50/100}	
d = distance [mm]	[-0,01MR; 1,01MR]	

Current output (with mastering), reference value is midrange

Variables	Value range	Formula
$I_{OUT}$ = current [mA]	[3,8; <4] SMR reserve [4; 20] measuring range [>20; 20,2] EMR reserve	$d \text{ [mm]} = \frac{(I_{OUT} \text{ [mA]} - 12)}{16} * MR \text{ [mm]}$
MR = measuring range [mm]	{10/25/50/100}	
MP = master position [mm]	[0; MR]	
d = distance [mm]	for $MP \leq 0.5MR$ : [-MP; 0.5MR] for $MP > 0.5MR$ : [-0.5MR; MR - MP]	

## Current output (with teaching)

Variables	Value range	Formula
$I_{OUT}$ = current [mA]	[3,8; <4] SMR reserve [4; 20] measuring range [>20; 20,2] EMR reserve	
MR = measuring range [mm]	{10/25/50/100}	
m, n = teaching area [mm]	[0; MR]	
d = distance [mm]	[m; n]	


## Current output (with mastering and teaching)

Variables	Value range	Formula
$I_{OUT}$ = current [mA]	[3,8; <4] SMR reserve [4; 20] measuring range [>20; 20,2] EMR reserve	
MR = measuring range [mm]	{10/25/50/100}	
MP = position object [mm]	[0; MR]	
m, n = teaching area [mm]	for $MP \leq 0.5MR$ : [-MP; 0.5MR] for $MP > 0.5MR$ : [-0,5MR; MR - MP]	
d = distance [mm]	[m; n]	



### 7.5.3.5 Characteristics Distance Value and Analog Output

The mastering and zero setting function set the analog output on half of the output range independent on the master value, thus 12 mA. The examples below show the current output and the distance value behavior of an ILD1320-50 with 50 mm measuring range.


Target at 16 % measuring range

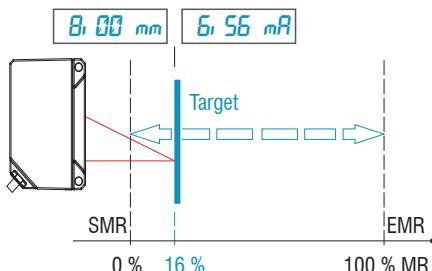


➡ Zero setting (master value = 0 mm)

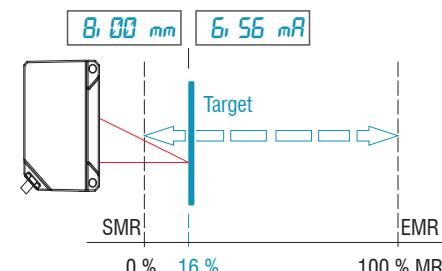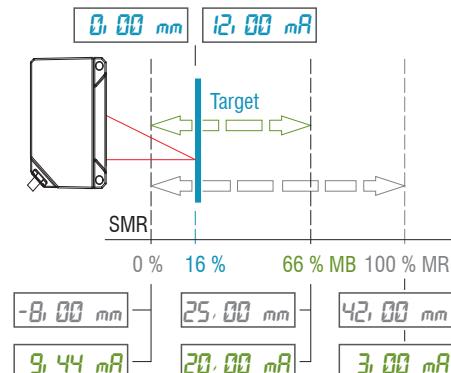


➡ Set master value 5 mm

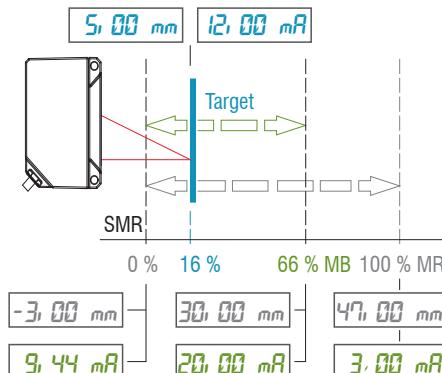

Target at 60 % measuring range

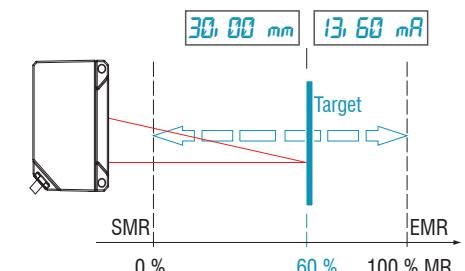


➡ Set master value 10 mm

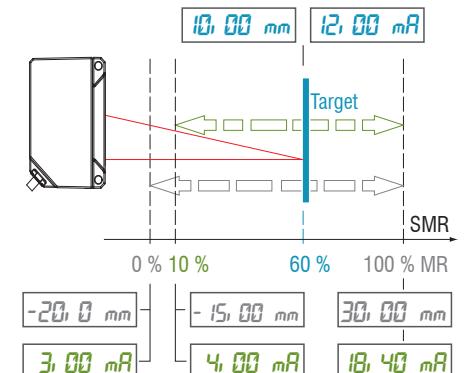

Analog maximum reached at 66 % MR

MR = measuring range, SMR = start of measuring range, EMR = end of measuring range

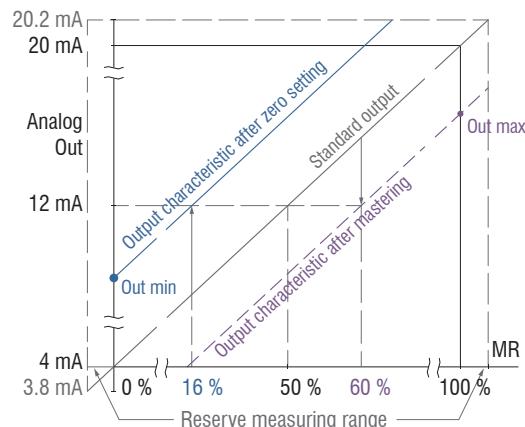

Master point	Master value	Out min	Out max
16 % (8 mm)	0 mm	9.44 mA (-8 mm)	20.0 mA (33 mm)
60 % (30 mm)	10 mm	4.00 mA (-15 mm)	18.40 mA (30 mm)

Fig. 39 Analog output with zero setting resp. mastering



### 7.5.3.6 Mastering and Teaching Analog Output

Proceed as follows:

1. Mastering or zero setting, menu signal processing

2. Teach output, menu Outputs

The mastering and zero setting function set the analog output on half of the output range, see Chap. 7.5.3.5.

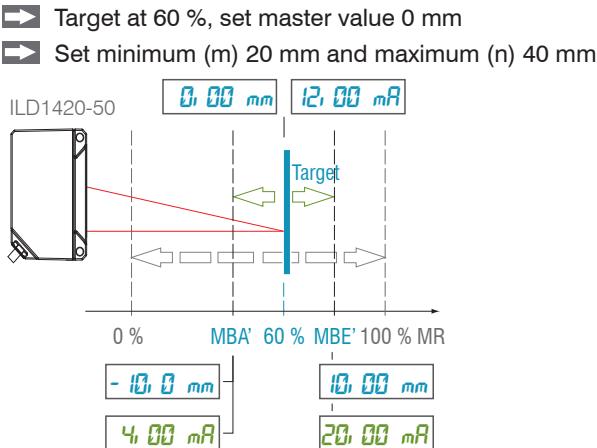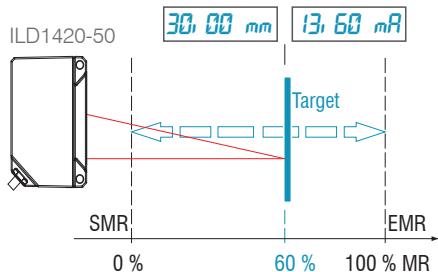

- i With  $n < m$  generates an inverse characteristic.

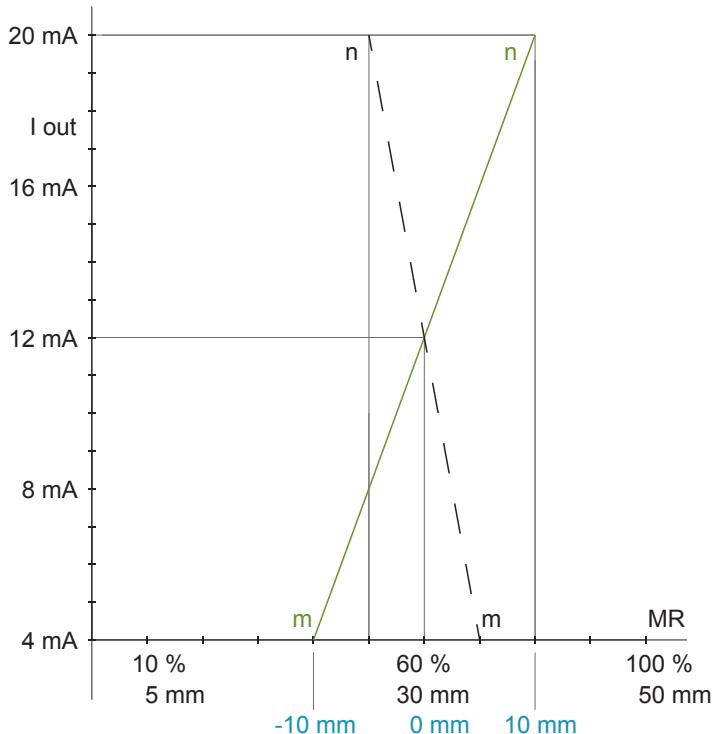


Fig. 40 Analog output characteristic after mastering and scaling with an ILD1320-50

## 7.6 System Settings

### 7.6.1 General

After programming all the settings are to be stored permanently in a set of parameters. The next time you turn on the sensor they are available again.

### 7.6.2 Unit, Language

The web interface promotes the units millimeter (mm) and inch when displaying measuring results.

You can choose German, English or Chinese in the web interface. You can change language in the menu bar.



Fig. 41 Language selection in the menu bar


### 7.6.3 Keylock

The function keylock for the key *Select*, see Chap. 5.3 prevents unauthorized / unintended performing of the key functions. Keylock is always activated when user level *User* is chosen. Keylock can only be deactivated in user level *Expert*. If an expert logs in the system, keylock on the sensor is automatically unlocked.

Key lock	Automatic	Range from 1 ... 60 [min]	Value	<i>Keylock starts after expiry of defined time. Clicking the button Refresh prolongs the timeframe until keylock starts.</i>
<i>Active</i>				<i>The key Select is deactivated independent of the user level.</i>
<i>Inactive</i>				<i>The key Select is active independent of the user level.</i>



Grey shaded fields require a selection.



Value  
Dark-bordered fields require you to specify a value.

## 7.6.4 Load, Save

All settings to the sensor can be saved permanently in one application program, a so called setup.

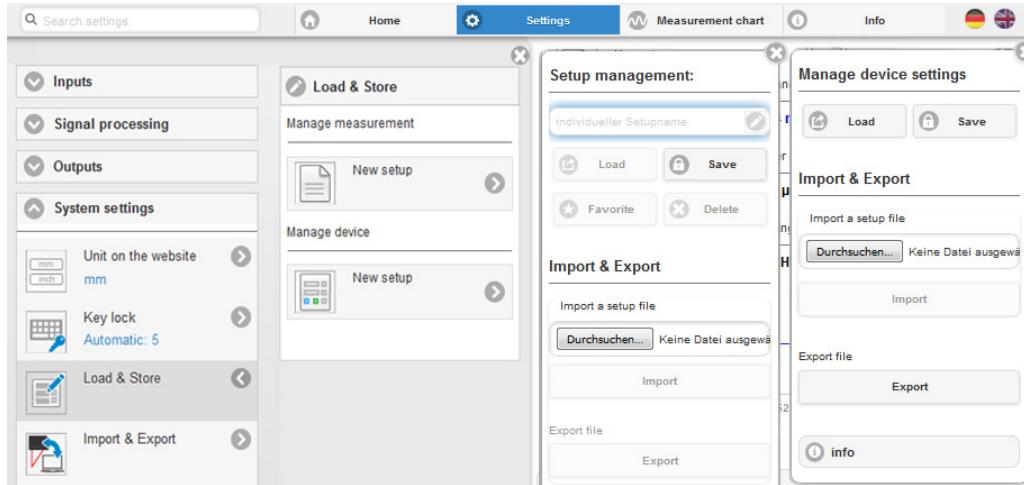



Fig. 42 Administration of application programs

### Administer setups in the sensor, possibilities and procedure

Save settings	Activate existing setup	Save changes in active setup	Define setup after booting
Menu New setup	Menu Load & Save	Menu bar	Menu Load & Save
<p>► Enter the name for the setup into the field <input type="text" value="Individual setup name"/> , e.g. rubber 1.05 and click the button Save.</p>	<p>► Click on the setup with the left mouse button. The dialog Setup management opens. ► Click on the button Load.</p>	<p>► Click on the button  Save settings</p>	<p>► Click on the setup with the left mouse button. The dialog Setup management opens. ► Click on the button Favorite.</p>


Exchange setup with PC/notebook, possibilities	
Save setup on PC	Load setup from PC
<p>Menu Load &amp; Save</p> <p>► Click on the setup with the left mouse button, area A.</p> <p>The dialog Setup management opens.</p> <p>► Click on the button Export.</p>	<p>Menu Load &amp; Save</p> <p>► Click on Create setup with the left mouse button.</p> <p>The dialog Setup management opens.</p> <p>► Click on the button Search.</p> <p>A Windows dialog for file selections opens.</p> <p>► Choose the desired file and click on the button Open.</p> <p>► Click the button Import in the setup management.</p>

## 7.6.5 Import, Export

A set of parameters covers current settings, setup(s) and the initial setup when booting the sensor. The menu Import & Export enables easy exchange of sets of parameters with a PC/notebook.

Exchange set of parameters with PC/notebook, possibilities	
Save set of parameters on PC	Load set of parameters from PC
Menu Import & Export	Menu Import & Export
<ul style="list-style-type: none"> <li>➡ Click on the button New set of parameters with the left mouse button..</li> </ul> <p>The dialog Choose setups for export opens.</p> <ul style="list-style-type: none"> <li>➡ You arrange a set of parameters by selecting/deselecting the check boxes.</li> <li>➡ Click on the button Transmit file.</li> </ul> <p>A Windows dialog for file transmission opens.</p> <ul style="list-style-type: none"> <li>➡ Confirm the dialog with OK.</li> </ul> <p>The operating system stores the set of parameters in the area Download.</p> <p>File name for the following example is &lt;...\\Downloads\\ILD1320_50BASICSETTINGS-MEASSETTINGS_SCHALE_T1...SETTING_Rubber 1.05.JSON&gt;</p>	<ul style="list-style-type: none"> <li>➡ Click on the button Search.</li> </ul> <p>A Windows dialog for file selection opens.</p> <ul style="list-style-type: none"> <li>➡ Choose the desired file and click on the button Open.</li> </ul> <p>The dialog Choose setups for export opens.</p> <ul style="list-style-type: none"> <li>➡ You define actions to be made by selecting/deselecting the check boxes.</li> <li>➡ Click on the button Transmit file.</li> </ul>

A security query, see adjacent figure, helps to avoid that an existing setup is inadvertently overwritten during import.

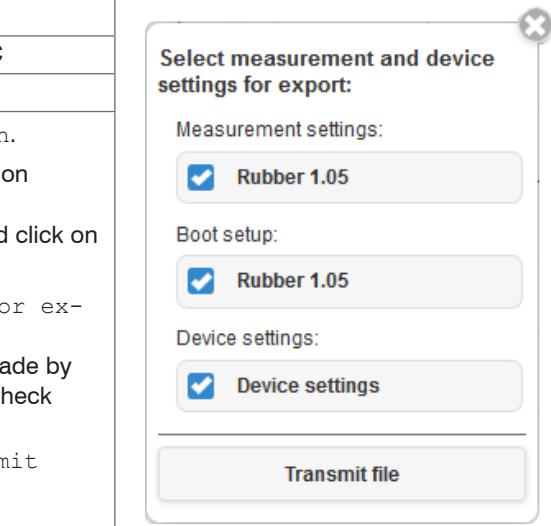

### Options during import:

- Overwrite existing setups (with the same name)
- Apply settings of the imported boot setup

### 7.6.6 Access Authorization


The assignment of a password prevents unauthorized changing of settings on the sensor. When delivered, the password protection is not enabled. The sensor operates in the user level **Professional**. The password protection should be enabled after configuration of the sensor. The default password for the expert level is 000.

- i** The default password or a user-defined password is not changed by a software update. The professional password is independent of the setup and is therefore not together loaded or saved with the setup.

The following functions are available for the user:

	User	Professional
Password required	no	yes
Viewing settings, signal processing, outputs, system settings	yes	yes
Changing settings, signal processing, outputs, system settings	no	yes
Changing password	no	yes
Changing between the measurement and video signal chart types	no	yes
Scaling diagrams	yes	yes
Setting factory setting	no	yes

*Fig. 43 Rights in the user hierarchy*

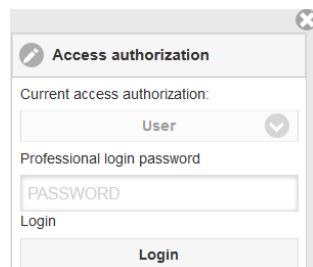

Type in the default password 000 or a user-defined password in the Password field and confirm with Login.

Change with a click on the Logout button in the mode user.

*Fig. 44 Change in the professional user level*

The user management allows you to assign a custom password in the Professional mode.

Password	Value	Case-sensitive rules are observed for all passwords. Numbers are allowed. Special characters are not allowed. Maximum length is set to 31 characters.
User level when restarting	User / Professional	Specifies the user level, with which the sensor starts after the restarting. For this purpose, MICRO-EPSILON recommends the selection user.


After configuration of the sensor the password protection is to be activated. Please note the password for later reference.

#### 7.6.7 Sensor Reset

Sensor reset	Sensor settings	Button	Settings for baud rate, language, unit, keylock and echo mode are deleted and the default parameters are loaded.
	Measurement settings	Button	Settings for measuring rate, trigger, evaluation range, peak selection, error handling, averaging, zeroing/mastering, data reduction and the setups are deleted. The 1 <sup>st</sup> preset will be loaded.
	Reset all	Button	When clicking this button settings for sensor, measuring preferences, access authorization, password and the setups are deleted. The 1 <sup>st</sup> preset will be loaded.
	Restart sensor	Button	When clicking this button the sensor is rebooted with the settings from the setup Favorite, see Chap. 7.6.4.



Grey shaded fields require a selection.



Value  
Dark-bordered fields require you to specify a value.

## 8. Digital Interfaces RS422

### 8.1 Preliminary Remarks

The interface RS422 has a maximum baud rate of 1 MBaud. The factory-set baud rate is 921.6 kBaud. The maximum measuring rate is 4 kHz.

Data format: Measurement values in binary format, commands as an ASCII string.

Interface parameter: 8 Data bits, no parity, one stop bit (8N1).

- **i** Disconnect or connect the D-sub connection between RS422 and USB converter when the sensor is disconnected from power supply only.

### 8.2 Measurement Data Format

16<sup>1</sup> resp. 18 bits are transmitted per output value, see Chap. 7.5.2. An output value is divided into three bytes that differ in the two most significant bits. The transmission of additional output values is optional.

Output value 1 / additional:

L-Byte	0	0	D5	D4	D3	D2	D1	D0
M-Byte	0	1	D11	D10	D9	D8	D7	D6
H-Byte	1	0 <sup>2</sup>	0 <sup>3</sup>	0 <sup>3</sup>	D15	D14	D13	D12

Output sequence: L-Byte, M-Byte, H-Byte.

1, 3) Error values are coded with 18 Bit.

2) To decide between the 1<sup>st</sup> output value and additional output values, bit 7 in the H-Byte is set to 1. Bit 7 in the H-Byte is set to 0 for the 1<sup>st</sup> output value. This simultaneously represents the identifier of a new block. Depending on the measuring rate, baud rate and output data rate output all data can be output in one block. If data output is not possible, a run-time error will be output. Use the command GETOUTINFO\_RS422 to query for data selection and output sequence.

### 8.3 Conversion of the Binary Data Format

For conversion purposes the H-Byte, M-Byte and L-Byte must be identified on the basis of the two first bits (flag bits), the flag bits deleted and the remaining bits compiled into a 16 or 18 bit data word.

Result of conversion:



Conversion must be done in the application program. D16 and D17 are among others used for interpretation of error codes or e.g. for the measurement counter.

- **i** The sensor continues to deliver measurement values to the RS422 output even while communicating with the sensor.

For the data transmission with a PC the MICRO-EPSILON IF2001/USB is suitable. The IF2001/USB combines the three bytes for the data word and saves them in the FIFO. The 18 bits are used for measurement values and error values. For further information, please refer to the descriptions of the IF2001/USB interface card and associated MEDAQlib driver program.

You will find the latest program routine at: [www.micro-epsilon.com/link/software/medaqlip](http://www.micro-epsilon.com/link/software/medaqlip).

## **9. Cleaning**

Cleaning of the protective screens is recommended periodically.

### **Dry Cleaning**

Therefore an optics anti-static brush is suitable or bleeding the screen with dehumidified, clean and oil-free compressed air.

### **Wet Cleaning**

For cleaning the protective screen use a clean, soft, lint-free cloth or lens cleaning paper with pure alcohol (isopropyl).

Never use standard glass cleaner or other cleaning agents.

## 10. Software Support with MEDAQLib

MEDAQLib offers you a documented driver DLL. Therewith you embed optoNCDT laser sensors, in combination with a RS422/USB converter, e. g. IF2001/USB, into an existing or a customized PC software.

MEDAQLib

- contains a DLL, which can be imported into C, C++, VB, Delphi and many additional programs,
- makes data conversion for you,
- works independent of the used interface type,
- features by identical functions for the communication (commands),
- provides a consistent transmission format for all MICRO-EPSILON sensors.

For C/C++ programmers MEDAQLib contains an additional header file and a library file. You will find the latest driver / program routine at:

[www.micro-epsilon.de/download](http://www.micro-epsilon.de/download)

[www.micro-epsilon.de/link/software/medaqlib](http://www.micro-epsilon.de/link/software/medaqlib)

## 11.      **Warranty**

All components of the device have been checked and tested for perfect function in the factory. In the unlikely event that errors should occur despite our thorough quality control, this should be reported immediately to MICRO-EPSILON.

The warranty period lasts 12 months following the day of shipment. Defective parts, except wear parts, will be repaired or replaced free of charge within this period if you return the device free of cost to MICRO-EPSILON. This warranty does not apply to damage resulting from abuse of the equipment and devices, from forceful handling or installation of the devices or from repair or modifications performed by third parties.

No other claims, except as warranted, are accepted. The terms of the purchasing contract apply in full.

MICRO-EPSILON will specifically not be responsible for eventual consequential damages. MICRO-EPSILON always strives to supply the customers with the finest and most advanced equipment. Development and refinement is therefore performed continuously and the right to design changes without prior notice is accordingly reserved. For translations in other languages, the data and statements in the German language operation manual are to be taken as authoritative.

## 12.      **Decommissioning, Disposal**

► Disconnect the power supply and output cable on the sensor.

Incorrect disposal may cause harm to the environment.

► Dispose of the device, its components and accessories, as well as the packaging materials in compliance with the applicable country-specific waste treatment and disposal regulations of the region of use.

## 13.      **Service, Repair**

In the event of a defect on the sensor or the sensor cable:

- If possible, save the current sensor settings in a parameter set, see Chap. [7.6.4](#), in order to load again the settings back into the sensor after the repair.
- Please send us the effected parts for repair or exchange.

In the case of faults the cause of which is not clearly identifiable, the whole measuring system must be sent back to

MICRO-EPSILON Optronic GmbH

Lessingstraße 14

01465 Langebrück / Germany

Tel. +49 (0) 35201 / 729-0

Fax +49 (0) 35201 / 729-90

[optronic@micro-epsilon.de](mailto:optronic@micro-epsilon.de)

[www.micro-epsilon.com](http://www.micro-epsilon.com)

## Appendix

### A 1      Optional Accessories

IF2001/USB



Converter RS422 to USB, type IF2001/USB,  
inclusive driver,  
connections: 1x female connector 10-pin  
(cable clamp) type Würth 691361100010,  
1x female connector 6-pin (cable clamp) type  
Würth 691361100006

IF2004/USB



1 channel<sup>1</sup> converter RS422 to USB inclusive  
driver, connections: 1x terminal block

PS2020



Power supply for mounting on DIN rail, input  
230 VAC, output 24 VDC/2.5 A

1) One channel with ILD 1320 possible only.

## A 2      Factory Setting

Password	„000“
Measuring rate	1 kHz
Measuring range	100 % FSO: $I = 20 \text{ mA}$ , digital 64877
	0 % FSO: $I = 4 \text{ mA}$ , digital 643
Peak selection	Highest peak
Error handling	Error output, no measurement

Measurement averaging	Median 9
Output	Analog current
RS422	921.6 kBaud
Trigger mode	No trigger
Language	German

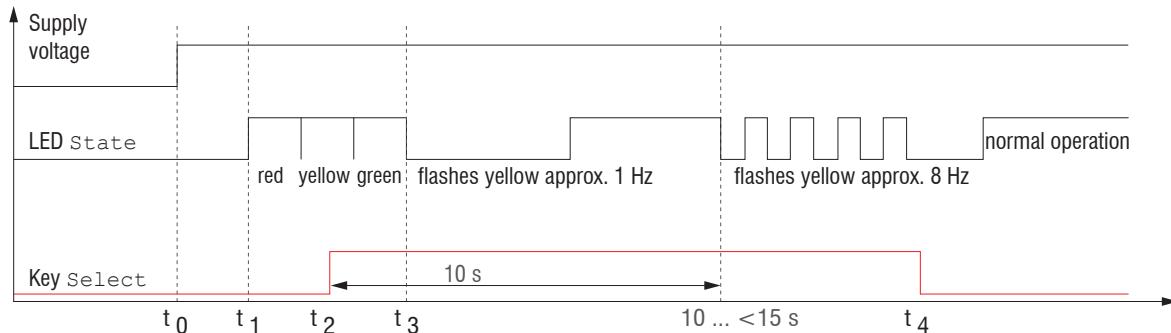


Fig. 45 Flow chart to start a sensor with factory setting

$t_0$ : power supply is on

$t_1 \dots t_3$ : both LEDs signalize the start sequence (red-yellow-green for 1 sec. each)

$t_2$ : key is pressed during start sequence ( $t_1 \dots t_3$ )

$t_4$ : key is released while the LED State is flashing red

$\Delta t = t_4 - t_2$ ;  $\Delta t$  (key press period) must be at least 10 sec., max. 15 sec.

## A 3        ASCII Communication with Sensor

### A 3.1      General

The ASCII commands can be sent to the sensor via the RS422 interface. All commands, inputs and error messages are effected in English.

One command always consists of a command name and zero or several parameters, which are separated by blanks and are completed with LF. If blanks are used in parameters, the parameter must be set in quotation marks.

Example: Switch on the output via RS422

OUTPUT RS422 ↴

Advice:      ↴ must include LF, but may also be CR LF.

Declaration: LF    Line feed (line feed, hex 0A)

CR    Carriage return (carriage return, hex 0D)

↳ Enter (depending on the system System hex 0A or hex 0D0A)

The currently set parameter value is returned, if a command is activated without parameters.

The input formats are:

<Command name> <Parameter1> [<Parameter2> [...] ]

<Command name> <Parameter1> <Parameter2> ... <Parameter...>

or a combination thereof.

Parameters in []-brackets are optional and require the input of the parameter standing in front. Sequent parameters without []-brackets are to input compulsory, that is, it must not be omitted a parameter.

Alternative inputs of parameter values are displayed separately by „|“, for example the values „a“, „b“ or „c“ can be set for „a|b|c“. Parameter values in <> brackets are selectable from a value range.

Declarations on format:

„a   b“	Value of the parameter can be set to the value “a“ or “b“.
„ P1 P2“	It requires that both parameters “P1“ and “P2“ are set.
„ P1 [P2 [P3]]“	The parameters “P1“, “P2“ and “P3“ can be set, whereby “P2“ may only be set, if “P1“ is set and “P3“ only if “P1“ and “P2“ are set.

„<a>“	The value of the parameter lies in a value range of „... to ...“, see parameter description.
-------	--

Parameter values without peak brackets can only assume discrete values, see parameter description.

Parantheses are to be understood as a grouping, that is, for a better articulation „P1 P2 | P3“ is written as „(P1 P2)|P3“.

Example without []:

„PASSWD <Old password> <New password> <New password>“

- To change the password, all three parameters are to be input.

The output format is:

<Command name> <Parameter1> [<Parameter2> [...]]

The reply can be used again as command for the parameter setting without changes. Optional parameters are only returned, if the returning is necessary. For example, the activated output values are returned by command Data selection additional values. After processing a command always a return and a prompt (“->”) is returned. In the case of an error an error message is before the prompt, that begins with „Exxx“, where xxx is a unique error number. Also warnings („Wxxx“) can be output instead of error messages.

These are analogous to the error messages. In case of warnings the command is executed.

The replies to the commands GETINFO and PRINT are useful for support requests to the sensor, because they contain sensor settings.

**A 3.2 Overview Commands**

Group	Chapter	Command	Short description
<b>General</b>			
	Chap. A 3.3.1	HELP	Help on commands
	Chap. A 3.3.2	GETINFO	Request sensor information
	Chap. A 3.3.3	LANGUAGE	Determine language of website
	Chap. A 3.3.4	RESET	Reboot sensor
	Chap. A 3.3.5	RESETCNT	Reset counter
	Chap. A 3.3.6	ECHO	Switching the command reply, ASCII interface
	Chap. A 3.3.7	PRINT	Output of all sensor settings
<b>User level</b>			
	Chap. A 3.3.8.1	LOGIN	Change of user level
	Chap. A 3.3.8.2	LOGOUT	Change to user in the user level
	Chap. A 3.3.8.3	GETUSERLEVEL	User level request
	Chap. A 3.3.8.4	STDUSER	Setting the standard user
	Chap. A 3.3.8.5	PASSWD	Change password
<b>Triggering</b>			
	Chap. A 3.3.9.1	TRIGGER	Selection of trigger mode
	Chap. A 3.3.9.2	MFILEVEL	Selection of level for multifunctional input
	Chap. A 3.3.9.3	TRIGGERCOUNT	Number of measurement values displayed
	Chap. A 3.3.9.4	TRIGGERSW	Software - trigger pulse

Interfaces	Chap. A 3.3.10.1	BAUDRATE	RS422 setting
	Chap. A 3.3.10.2	UNIT	Selection of measuring unit web interface
	Chap. A 3.3.10.3	MFIFUNC	Selection of function multifunctional input
	Chap. A 3.3.10.4	ERRORROUT1	Activate digital output
	Chap. A 3.3.10.5	ERRORLEVELOUT1	Output level digital output
	Kap. A 3.3.10.6	ERRORLIMIT	Limit to activate digital output
	Kap. A 3.3.10.7	ERRORHYSTERESIS	Stable digital output
	Kap. A 3.3.10.8	ERROROUTHOLD	Minimum duration active digital output
	Handling of setups		
Handling of setups	Chap. A 3.3.11.1	IMPORT	Load parameter
	Chap. A 3.3.11.2	EXPORT	Export sensor settings
	Chap. A 3.3.11.3	MEASSETTINGS	Load/save measurement settings
	Chap. A 3.3.11.4	BASICSETTINGS	Load/save device settings
	Chap. A 3.3.11.5	SETDEFAULT	Factory settings
Scaling of analog output			
Chap. A 3.3.12 ANALOGSCALE Scaling analog output			
Key function			
Key function	Chap. A 3.3.13.1	KEYFUNC	Selection of key function
	Chap. A 3.3.13.2	KEYLOC	Selection of keylock

Measurement		
General		
Chap. A 3.4.1	MEASPEAK	Choice of the peak in the video signal
Chap. A 3.4.2	MEASRATE	Selection of measuring rate
Chap. A 3.4.3	LASERPOW	Selection of laser power
Measurement Value Processing		
Chap. A 3.4.4.1	MASTERMV	Mastering / Zeroing
Data Output		
General		
Chap. A 3.5.1	OUTPUT	Selection measuring value output
Chap. A 3.5.2	OUTHOLD	Setting of error processing
Select measurement values to be output		
Chap. A 3.5.3.1	GETOIUTINFO_RS422	Request data selection
Chap. A 3.5.3.2	OUTADD_RS422	Selection of additional values

**A 3.3 General Commands****A 3.3.1 HELP**

```
HELP [<Command>]
```

Issues a help for every command. If no command is specified, a general help is output.

**A 3.3.2 GETINFO, Sensor Information**

```
GETINFO
```

Request of sensor information. Output see example below:

```
->GETINFO
Name: ILD1320-10 //Model name sensor, sensor series
Serial: 15030002 //Serial number
Option: 000 //Option number of sensor
Article: 4120209 //Article number of sensor
Cable head: Wire
Measuring range: 10.00mm //Measuring range of sensor
Version: 001.010 //Version of software
Hardware-rev: 00
Boot-version: 001.000
->
```

**A 3.3.3 LANGUAGE, Website**

```
LANGUAGE DE | EN
```

Determines the language for the web interface.

- DE: set language to German
- EN: set language to English
- CN: set language to Chinese

The chosen language setting applies to the website.

#### A 3.3.4     RESET, Boot Sensor

RESET

The sensor is rebooted.

#### A 3.3.5     RESETCNT, Reset Counter

RESETCNT [TIMESTAMP] [MEASCNT]

Sets back internal counters in the sensor.

- TIMESTAMP: sets back timestamp
- MEASCNT: sets back measurement counter

#### A 3.3.6     ECHO, Switching the Command Reply, ASCII Interface

ECHO ON|OFF

Setting the command reply with a ASCII command:

- ON: command reply on, for example <Kdo> ok (or notice of error)  
->
- OFF: command reply off, for example ->

### A 3.3.7 PRINT, Sensor Settings

PRINT

Print serves the output of all sensor settings.

Example of an answer:

GETUSERLEVEL PROFESSIONAL	OUTPUT ANALOG
STDUSER PROFESSIONAL	OUTADD_RS422 NONE
BAUDRATE 921600	GETOUTINFO_RS422 DIST1
UNIT MM	OUTHOLD NONE
LANGUAGE DE	ERROROUT1 DIST
MFIFUNC NONE	ERRORLEVELOUT1 NPN
MFILEVEL HTL_HIGH	ANALOGSCALE STANDARD
KEYFUNC NONE	
KEYLOCK AUTO 5 (IS_ACTIVE)	
MEASRATE 1.000	
MEASPEAK DISTA	
TRIGGER NONE	
TRIGGERCOUNT INFINITE	
LASERPOW FULL	
MASTERMV NONE	

**A 3.3.8 User Level****A 3.3.8.1 LOGIN, Change of the User Level**

LOGIN <Password>

Enter the password to change user level. The following user levels are available:

- USER (standard user): “read-only” access to all elements and graphical display of output values of web surface
- PROFESSIONAL (expert): “read-only” and “write” access to all elements

**A 3.3.8.2 LOGOUT, Change into User Level**

LOGOUT

Set user level to USER.

**A 3.3.8.3 GETUSERLEVEL, User Level Request**

GETUSERLEVEL

Request current user level

**A 3.3.8.4 STDUSER, Set Standard User**

STDUSER USER | PROFESSIONAL

Set standard user who is automatically logged in after system start. Standard user does not change with LOGOUT which means login as standard user is done automatically after the command RESET or power supply of sensor is switched on.

**A 3.3.8.5 PASSWD, Change Password**

PASSWD <Old Password> <New password> <New password>

Change password for user level PROFESSIONAL.

Type in the old password followed by the new password (2x). In case the new password is not typed in correctly, an error message will be displayed. Password may only contain letters from A to Z, no numbers 0 to 9. Watch upper and lower case lettering. The maximum length is limited to 31 characters.

### A 3.3.9 Triggering

The multifunctional input also serves as trigger input for measurement output.

#### A 3.3.9.1 TRIGGER, Selection

TRIGGER NONE | EDGE | PULSE | SOFTWARE

- NONE: no triggering
- PULSE: level triggering
- EDGE: edge triggering
- SOFTWARE: software triggering

#### A 3.3.9.2 MFILEVEL, Input Pulse Multifunctional Input

MFILEVEL HTL\_HIGH | HTL\_LOW

Selection of switching or trigger level for the multifunctional input.

- HTL\_HIGH: high active (edge triggering: rising edge, pulse triggering: high active)
- HTL\_LOW: low active (edge triggering: falling edge, pulse triggering: low active)

#### A 3.3.9.3 TRIGGERCOUNT, Number of Displayed Measurement Values

TRIGGERCOUNT NONE | INFINITE | <n>

<1...16382>

Number of displayed measurement values while triggering

- NONE: stop triggering and start continuous output
- INFINITE: start continuous output after first trigger impulse
- <n>: number of displayed measurement values after each trigger impulse n = 1 ... 16382

#### A 3.3.9.4 TRIGGERSW, Software Trigger Pulse

TRIGGERSW

Creates a trigger pulse. Error message is displayed if "SOFTWARE" is not selected in trigger selection.

**A 3.3.10 Interfaces****A 3.3.10.1 BAUDRATE, RS422**

```
BAUDRATE 9600|19200|56000|115200|128000|230400|256000|460800|691200|921600|  
1000000
```

Set the baud rate for the RS422 interface.

**A 3.3.10.2 UNIT, Web Interface**

```
UNIT MM|INCH
```

Change the measurement display on the websites. The command has no effect on the ASCII interface.

- MM representation in mm
- INCH representation in customs

**A 3.3.10.3 MFIFUNC, Function Selection Multifunctional Input**

```
MFIFUNC NONE | MASTER | TEACH | TRIGGER
```

Choose function of the multifunctional input.

- NONE: multifunctional input has no function
- MASTER: multifunctional input is master impulse input
- TEACH: multifunctional input is teach input for analog output
- TRIGGER: multifunctional input is trigger input

**A 3.3.10.4 ERROROUT1, Activate Error Output**

```
ERROROUT1 NONE|DIST|TEACH|LI1
```

Choose error signal of the digital output ERROR.

- NONE: digital output deactivated
- DIST: no peak found or beyond measuring range (out of range)
- TEACH: Distance is out of scaled analog range
- LI1: Distance is greater than the limit value (ERRORLIMIT)

#### A 3.3.10.5 ERRORLEVELOUT1, Output Level Digital Output

ERRORLEVELOUT1 NPN | PNP | PUSHPULL | PUSHPULLNEG

Choice of output level for ERROROUT1.

- NPN: digital output is active in case of an error
- PNP: digital output is active in case of an error
- PUSHPULL: digital output with high level in case of an error
- PUSHPULLNEG: digital output with low level in case of an error

Wiring of digital output ERROR1, see Chap. [5.4.8](#).

#### A 3.3.10.6 ERRORLIMIT

ERRORLIMIT DIST1 <upper threshold>

Digital output is activated, if the defined value for a measurement is exceeded.

Range: 0 ... 2 \* measuring range [mm].

#### A 3.3.10.7 ERRORHYSTERESIS

ERRORHYSTERESIS <hysteresis>

Digital output is deactivated, if the defined value for a measurement falls below the limit value.

Range: 0 ... 2 \* measuring range [mm].

#### A 3.3.10.8 ERROROUTHOLD

ERROROUTHOLD <hold period>

Indicates in ms how long the digital output must be active at least when the limit value is exceeded. This time period starts when the limit value is exceeded. Range: 0 ... 1000 [ms].

### A 3.3.11 Handling of Setups

#### A 3.3.11.1 IMPORT

```
IMPORT [FORCE] [APPLY] <Data>
```

Import of data in JSON format<sup>1</sup> to the sensor.

First, the import command returns a prompt (->). Afterwards, data can be sent.

After importing a prompt (->) is returned.

- FORCE: overwriting of measurement settings (= MEASSETTINGS) with the same name (otherwise an error message is returned when using the same name). When importing all measurement settings or device settings (= BASICSETTINGS) FORCE must always be stated.
- APPLY: applying the settings after importing / reading of initial settings.

1) JSON format, see [https://de.wikipedia.org/wiki/JavaScript\\_Object\\_Notation](https://de.wikipedia.org/wiki/JavaScript_Object_Notation)

#### A 3.3.11.2 EXPORT

```
EXPORT ALL | MEASSETTINGS_ALL | (MEASSETTINGS <SetupName>) | BASICSETTINGS
```

Exporting sensor settings. As a response data is transmitted in JSON format. Finally a prompt occurs.

#### A 3.3.11.3 MEASSETTINGS, Load / Save Measurement Settings

```
MEASSETTINGS <Subcommands> [Name]
```

Settings of the measurement task.

Loads proprietary presets and one user-specific setting from the sensor or stores one user-specific setup in the sensor.

Subcommands:

- CURRENT: Output of the name of current measurement setting
- PRESETLIST: Listing of all existing presets (names): „Standard“, „Multi-Surface“, „Light Penetration“.
- LIST: Listing of all saved measurement settings (names) „Name1“ „Name2“ „...“.
- READ <Name>: Loads a preset or a measurement setting from the sensor.
- STORE <Name>: Saves the current measurement setting in the sensor.
- DELETE <Name>: Deletes a measurement setting
- RENAME <NameOld> <NameNew> [FORCE]: Renaming a measurement setting. An existing measurement setting can be overwritten with FORCE.

- INITIAL <name> | AUTO: Loads a named or last saved measurement setting at the start of the sensor. Presets can not be specified.
- PRESETMODE: Returns the set signal quality
- PRESETMODE <Mode>: Setting the signal quality. Setting the signal quality is possible only, if a preset was loaded.
  - <mode> = STATIC|BALANCED|DYNAMIC|NOAVERAGING|NONE

#### A 3.3.11.4 BASICSETTINGS, Load / Save Device Settings

BASICSETTINGS READ | STORE

- READ: Loads the stored device settings from the sensor.
- STORE: Saves the current device settings in the sensor.

#### A 3.3.11.5 SETDEFAULT, Default Settings

SETDEFAULT ALL | MEASSETTINGS | BASICSETTINGS

Sets sensor back to default settings.

- ALL: Measurement and device settings are being deleted. The standard preset for the measurement setting resp. the the default parameter for the device settings are being loaded.
- MEASSETTINGS: Measurement settings are being deleted and the standard preset is being loaded.
- BASICSETTINGS: Device settings are being deleted and the default parameters are being loaded.

#### A 3.3.12 ANALOGSCALE, Scaling the Analog Output

ANALOGSCALE STANDARD | (TWOPOINT <Minimum value> <Maximum value>)

Setting the two point scaling of the analog output.

- STANDARD: using the measuring range of the sensor
  - TWOPOINT: two point scaling within the analog range (4 - 20 mA)
    - Minimum value: measurement value in mm which is matched to the lower analog value (4 mA)
    - Maximum value: measurement value in mm which is matched to the upper analog value (20 mA)
- I** The minimum value (in mm) can be higher than the maximum value (in mm), see Chap. 7.5.3.

**A 3.3.13 Key Function****A 3.3.13.1 KEYFUNC, Choose Key Function**

```
KEYFUNC NONE | MASTER | TEACH
```

Choice of key function.

- NONE: key has no function
- MASTER: key is used for mastering
- TEACH: key is used for teaching

**A 3.3.13.2 KEYLOCK, Set Keylock**

```
KEYLOCK NONE|ACTIVE|AUTO <time>
```

Choice of keylock.

- NONE: key works permanently, no keylock
- ACTIVE: keylock is activated right after reboot
- AUTO: keylock is only activated <time> minutes after reboot

**A 3.4 Measurement****A 3.4.1 MEASPEAK, Choice of the Peak in the Video Signal**

```
MEASPEAK DISTA|DIST1|DISTL
```

- DISTA: output of peak with highest amplitude (standard)
- DIST1: output of first peak
- DISTL: output of last peak

**A 3.4.2 MEASRATE, Measuring Rate**

```
MEASRATE 0.25|0.5|1|2
```

Choice of measuring rate in kHz.

**A 3.4.3 LASERPOW, Laser Power**

```
LASERPOW FULL|OFF
```

- FULL: laser power is set to 100 %
- OFF: laser is switched off

#### A 3.4.4 Measurement Value Processing

##### A 3.4.4.1 MASTERMV, Mastering / Zeroing

MASTERMV NONE | MASTER <MV>

- NONE: completes mastering
- MASTER: sets the current measurement value as a master value
- MV: master value in millimeters; MV = (0 ... 2) \* measuring range, i.e. master value must be within measuring range

In case of master value is 0, the mastering has the same functionality as the zeroing. The parameter MV always operates independently from an input as zeroing during mastering the analog output.

The master command awaits the next measurement value, a maximum of 2 seconds, and masters it. If no measurement value is received within this time, for example, by external triggering, the command returns with the error "E104 Timeout".

The master value is processed with six decimal places.

Note that the output value is limited to 18 bits.

#### A 3.5 Data Output

##### A 3.5.1 OUTPUT, Selection of Measurement Value Output

OUTPUT NONE | RS422 | ANALOG

- NONE: no measurement value
- RS422: output of measurement value via RS422
- ANALOG: analog output of measurement values

##### A 3.5.2 OUTHOLD, Error Processing

OUTHOLD NONE | INFINITE | <n>

Setting the behavior of the measurement value output in case of error.

- NONE: no holding of the last measurement value, output of error value
- INFINITE: infinite holding of the last measurement value
- <n>: holding of the last measurement value on the number of measurement cycles; then an error value is output, n = (1 ... 1024)

### A 3.5.3 Selection of Measurement Values to be Output

#### A 3.5.3.1 GETOUTINFO\_RS422, Request Data Selection

GETOUTINFO\_RS422

The command lists all selected output data for the RS422 interface. The sequence shown corresponds to the output sequence.

#### A 3.5.3.2 OUTADD\_RS422, Selection of Data Additional Values

OUTADD\_RS422 NONE | ([SHUTTER] [COUNTER] [TIMESTAMP] [INTENSITY] [STATE]  
[DIST\_RAW])

Selection of additional values to be transmitted.

- NONE: no output of additional values
- SHUTTER: output of exposure time
- COUNTER: output of measurement value counter
- TIMESTAMP: output of timestamp
- INTENSITY: output of intensity parallel to each distance value
- STATE: output of status word
- DIST\_RAW: output of uncalibrated distance value (raw value)

### A 3.6 Example Command Sequence During Selection of Measurement Value

Command	Content
MEASPEAK	Peak selection for displacement measurement
MEASRATE	Measuring rate (under consideration of reflectivity and movement of the target)
OUTPUT	Selection of the output channel
OUTHOLD	Output characteristic during measurement errors
OUTADD_RS422	Selection of the additional values to be output for RS422 interface
BAUDRATE	Baud rate settings RS422 interface

### A 3.7 Error Messages

If an error occurs with a command, the error message is listed.

Error message	Description
E100 Internal error	Internal error code
E104 Timeout	Timeout while mastering.
E200 I/O operation failed	Cannot write data to the output channel.
E202 Access denied	Access denied: Login as expert is necessary.
E204 Received unsupported character	An unsupported character was received
E210 Unknown command	Unknown command rights to small to read).
E214 Entered command is too long to be processed	The entered command with the parameters is too long (greater than 255 bytes).
E220 Timeout, command aborted	Timeout during mastering.
E232 Wrong parameter count	Too high or too small number of parameters.
E234 Wrong or unknown parameter type	A transmitted parameter has a wrong type or a wrong number of parameters were transmitted.
E236 Value is out of range or the format is invalid	The parameter value is out of range of the value range.
E262 Active signal transmission, please stop before	A measurement value transmission is active. Stop the data transmission in order to execute the command.
E320 Wrong info-data of the update	For update only: the header of update data contains an error.
E321 Update file is too large	For update only: update data is too large.
E322 Error during data transmission of the update	For update only: error during update data transmission.
E323 Timeout during the update	For update only: Timeout during the transmission of update data.
E331 Validation of import file failed	The import file is not valid.

E332 Error during import	Error during processing the import data
E333 No overwrite during import allowed	No overwrite of measurement and device settings allowed through import, set the checkbox.
E350 The new passwords are not identical	Password and verification password do not match.
E360 Name already exists or not allowed	The measurement setting name already exists or is not allowed.
E361 Name begins or ends with spaces or is empty	Name for the measurement setting begins or ends with spaces or is empty.
E362 Storage region is full	Number of storable measurement settings is reached.
E363 Setting name not found	Name of the measurement setting to be loaded not found
E364 Setting is invalid	Measurement resp. device setting is invalid
E602 Master value is out of range	Master value is out of valid range
E616 Software triggering is not active	Software triggering is not active.

Warning	Description
W320 The measuring output has been adapted automatically.	The measuring output has been adapted automatically.

**A 4 Control Menu****A 4.1 Tab Home**

Measurement task	Presets	Standard	<i>Suitable for materials made of ceramics, metal or filled plastics</i>
		Multi surface <sup>1</sup>	<i>Suitable for e.g. PCB or hybrid materials</i>
		Light penetration <sup>1</sup>	<i>Suitable for plastics (POM, Teflon), materials with strong penetration of the laser</i>
	Setup	Setup 1	<i>A setup contains user-specific measurement settings. Unlike the presets it can be changed anytime.</i>
Signal quality		Static / balanced / dynamic	<i>The signal quality affects averaging of measurement values.</i>

**A 4.2 Tab Settings****A 4.2.1 Inputs**


Laser on/off	On / Off		<i>Laser on/off is only effective when pin 8 is connected to GND.</i>	
Multifunctional input	Zeroing (Mastering)	High / Low	<i>Sets the function of the switching input. The trigger affects recording and output of a measurement value. Zeroing/Mastering sets the current measurement value to the entered master value. Teaching scales the analog output. HTL is defined as active input level.</i>	
	Trigger In	High / Low		
	Teaching			
	Inactive			
Key function	Zeroing (Mastering)		<i>Sets the function of the sensor key. Inactive means keylock.</i>	
	Teaching			
	Inactive			

1) Available for the sensor models ILD1320-10/25/50.

### A 4.2.2 Signal Processing

Measurement task	<i>Standard</i>			<i>Suitable for materials made of ceramics, metal or filled plastics</i>
	<i>Changing surface<sup>1</sup></i>			<i>Suitable for e.g. Printed circuit boards (PCB) or hybrid materials</i>
	<i>Material with penetration<sup>1</sup></i>			<i>Suitable for plastics (POM, Teflon), materials with strong penetration of the laser</i>
Measuring rates	250 Hz / 500 Hz / 1 kHz / 2 kHz			<i>For light and matt measuring objects a high measuring rate may be required. For dark or bright measuring objects a slower measuring rate may be required (e.g. black lacquered surface) to improve the measuring result.</i>
Output trigger	<i>Level</i>			<i>Continuous measurement output takes place as long as the selected level is applied. Level selection, see Chap. 7.3. Pulse duration must at least be one cycle time. The subsequent break must also be at least one cycle time.</i>
	<i>Edge</i>	<i>infinite</i>		<i>Edge selection. „0“ end trigger, „1 ... 16382“ values per trigger, „16383“ infinite trigger</i>
		<i>manual</i>	<i>Number</i>	
	<i>Software</i>	<i>infinite</i>		<i>Software triggering is started by clicking the button <i>Release trigger</i>. „0“ end trigger, „1 ... 16382“ values per trigger, „16383“ infinite trigger</i>
		<i>manual</i>	<i>Number</i>	
<i>Inactive</i>			<i>No triggering</i>	

1) Available for the sensor models ILD1320-10/25/50.

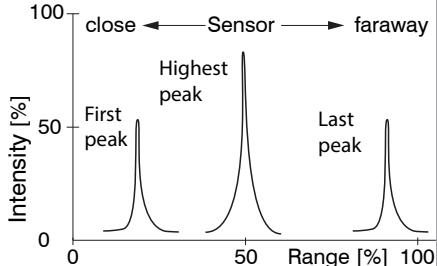Selection of peak	<i>First peak / Highest peak / Last peak</i>	<i>Defines which signal is used for the evaluation in the line signal.</i> <i>First peak: Nearest peak to sensor.</i> <i>Highest peak: standard, peak with the highest intensity.</i> <i>Last peak: widest peak to sensor.</i>	
Error handling	Error output, no measurement value	<i>The analog output supplies 3 mA instead of measurement value. The RS422 interface outputs an error value.</i>	
	Hold last value infinite	<i>Analog output and RS422 interface stop at the last valid value.</i>	
	Hold last value	1 ... 1024	<b>Value</b>
Zeroing/ Mastering	Inactive	<i>Normal measurement value resp. Zeroing/Mastering is undone.</i>	
	Active	<b>Value</b>	<i>Indication e.g. of thickness of a master part.</i> <i>Value range 0 up to max. + 2 x measuring range</i>

**A 4.2.3 Outputs**

RS422	Baud rate	9.6 / 19.2 / 56.0 / 115.2 / 230.4 ... / 1000 kBps		Transmission speed, binary data format
	Output data	<i>Distance / Exposure time / Intensity / Sensor status / Measurement value counter / non-linearized focus / Timestamp</i>		<i>Date to be transmitted are to be activated via the checkbox.</i>
Analog output	Standard scaling			<i>Start of measuring range 4 mA, at end of measuring range 20 mA</i>
	Two point scaling	Start of range	Value	<i>Always 2 points are taught which mark start and end of new measuring range. With two point scaling reversal of the output signal is possible.</i>
Digital output		End of range	Value	
Inactive			<i>Regulates the switching performance of the digital output (Error), see Chap. 5.4.8.</i>	
Analog range / Measuring range	NPN / PNP / PushPull / PushPullNeg			
Limit monitoring	NPN / PNP / PushPull / PushPullNeg			
	Limit	Value	<i>Measuring range: The digital output is switched when the peak is not (entirely) in evaluation range (ROI).</i>	
	Hysteresis	Value		
	Minimum holding period	Value		
Data output	Web interface / Analog / RS422			<i>Decides on the used interface for measurement value output. A parallel physical measurement value output via RS422 and analog is not possible. If web interface was selected, no measurement values are output via RS422 or current output.</i>

	LED Output	Web interface		RS422	Current output
		Parametrization	Measurement chart		
Selected output interface	Web interface	yellow	•	•	
	RS422	green	•		•
	Analog	red	•	•	•

**A 4.2.4 System Settings**

Unit on website	mm / inch		Unit in measurement value display	
Keylock	Automati-cally	Range 1 ... 60 [min]	Value <input type="text"/>	The keylock starts after expiry of the defined time. Clicking the button Refresh extends the interval until keylock starts.
		Refresh		
	Active			The key Select does not respond to entries, independent of user level.
Load & Save	Measure-ment set-tings	Create setup / Setup	Load	Activates a saved measurement setting setup.
			Save	Saves changed measurement settings to an existing setup.
			Favorite	Selects a setup which is used after reboot of the sensor.
			Delete	Deletes a setup.
			Search	You load an existing setup from a PC or the like to the ILD 1320 with both buttons.
			Import	
			Export	Saves the setup on a connected PC or the like.
	Device set-tings	Create setup	Load	Activates the saved device settings.
			Save	Saves changed device settings.
			Search	You load the device settings from a PC or the like to the ILD 1320 with both buttons.
			Import	
			Export	Saves the device settings on a connected PC or the like.

Import & Export	Create file	<i>Measurement settings</i>	<i>The measurement setting setups, the file with device settings and the boot file can be combined in one parameter set and exchanged with a PC or the like.</i>	
		<i>Boot setup</i>		
		<i>Device settings</i>		
	Search			
	Check file	<i>Overwrite existing setups (with the same name)</i>		
		<i>Apply settings of the imported boot setup</i>		
		<i>Transmit data</i>		

Access permission	Current access permission	<input type="text"/> Value	<i>Read only</i>	
	Logout / Login			
	User level reboot	<i>Professional / User</i>		
		<i>Sets the user level the sensor starts with after reboot. In this case MICRO-EPSILON recommends the selection user.</i>		
	Change password	Old password	<input type="text"/> Value	
		New password	<input type="text"/> Value	
		Repeat new password	<input type="text"/> Value	
		Change password		
		<i>Case-sensitive rules are observed for all passwords. Numbers are allowed. Special characters are not allowed. Maximum length is limited to 31 characters.</i>		
		<i>Button causes change of password.</i>		

Reset sensor	Measurement settings	<i>The settings for measuring rate, trigger, evaluation range, selection of peak, error handling, averaging, Zeroing/Mastering, reduction of data and setups are deleted. The 1st preset is loaded.</i>
	Device settings	<i>The settings baud rate, language, unit, keylock and echo mode are deleted and the default parameters are loaded.</i>
	Reset all	<i>By clicking the button the settings for the sensor, measurement settings, access permission, password and setups are deleted. The 1st preset is loaded.</i>
	Restart sensor	<i>By clicking the button the sensor is rebooted with the settings made in the favorite setup, see Chap. 7.6.4.</i>



Selection required or checkbox



Specification of a value required

- **i** The settings will be effective, if you click on the button **Apply**. After the programming all settings must be permanently stored under a parameter set so that they are available again when the sensor is switched on the next time.



MICRO-EPSILON MESSTECHNIK GmbH & Co. KG  
Königbacher Str. 15 · 94496 Ortenburg / Germany  
Tel. +49 (0) 8542 / 168-0 · Fax +49 (0) 8542 / 168-90  
[info@micro-epsilon.de](mailto:info@micro-epsilon.de) · [www.micro-epsilon.com](http://www.micro-epsilon.com)

X9751350-A041087MSC

© MICRO-EPSILON MESSTECHNIK

