


Reporte Biomédico MAX30102

Reporte generado automáticamente desde la sesión actual de monitoreo.

Inicio	2026-05-30T20:19:03	Fin	2026-05-30T23:23:25
Lecturas	1190	Eventos críticos	364
BPM	prom 108.0 min 16.0 max 300.0		
Temperatura	prom 31.6 min 26.5 max 34.4		
	SpO2	prom 96.3 min 4.3 max 99.9	
	Raw IR	prom 80662.9 min 423.0 max 119158.0	

Tendencias de la sesión

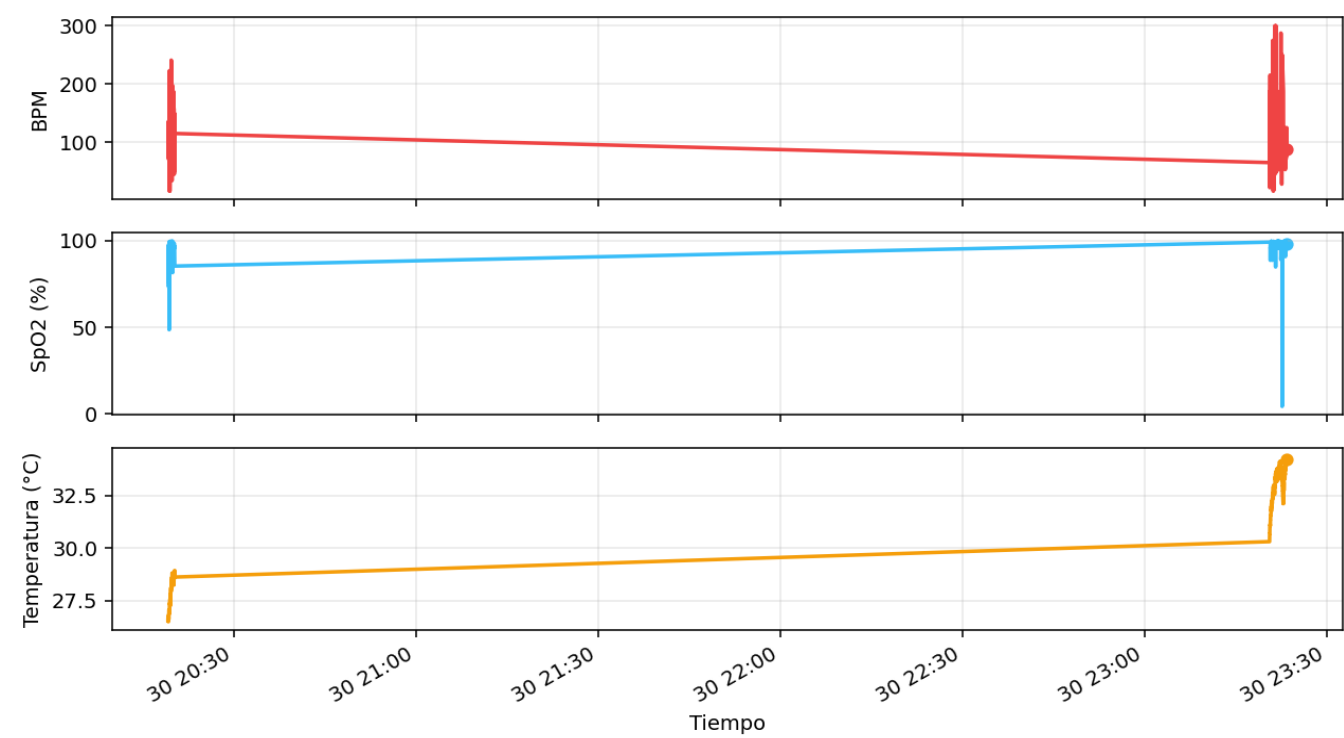

Últimas lecturas registradas

Fecha_Hora	BPM	SpO2	Temp	Raw_IR
23:23:21	78.0	97.0	34.1	93176
23:23:21	78.0	97.2	34.1	92211
23:23:21	78.0	97.2	34.1	92347
23:23:21	89.2	97.2	34.1	92544
23:23:22	83.0	97.2	34.4	92749
23:23:22	78.0	97.4	34.4	91804
23:23:22	80.5	97.4	34.4	91935
23:23:22	88.0	97.4	34.4	92218

23:23:22	83.0	97.8	34.4	92277
23:23:23	77.2	97.6	34.1	91653
23:23:23	88.0	97.8	34.1	91860
23:23:23	88.0	97.8	34.1	92343
23:23:23	83.0	97.8	34.1	91537
23:23:23	78.0	97.2	34.1	91765
23:23:24	100.0	97.2	34.4	91957
23:23:24	115.0	97.2	34.4	92258
23:23:24	115.0	97.6	34.4	91110
23:23:24	107.0	97.6	34.4	91112
23:23:24	125.0	97.6	34.4	91376
23:23:24	115.0	97.6	34.4	91550
23:23:25	100.0	97.2	34.2	90726
23:23:25	122.5	97.2	34.2	90972
23:23:25	93.0	97.2	34.2	91378
23:23:25	88.0	98.3	34.2	91502

Nota: la temperatura corresponde al sensor/chip MAX30102 y requiere calibración si se desea interpretar como temperatura corporal clínica.