


Reporte Biomédico MAX30102

Reporte generado automáticamente desde la sesión actual de monitoreo.

Inicio	2026-05-31T09:48:47	Fin	2026-05-31T09:54:30
Lecturas	1708	Eventos críticos	242
BPM	prom 89.2 min 20.0 max 271.8		
Temperatura	prom 30.1 min 28.5 max 30.6		
	SpO2	prom 98.2 min 54.2 max 99.9	
	Raw IR	prom 113804.1 min 4613.0 max 117301.0	

Tendencias de la sesión

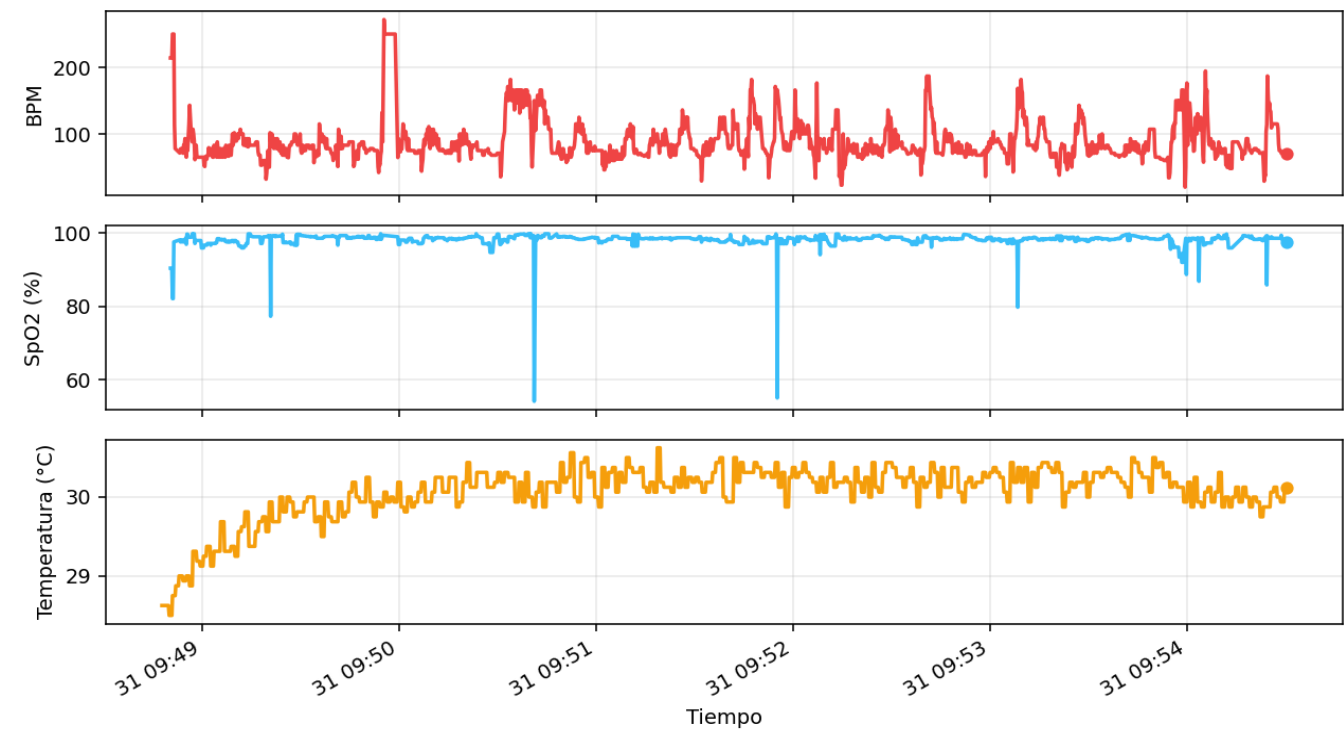

Últimas lecturas registradas

Fecha_Hora	BPM	SpO2	Temp	Raw_IR
09:54:25	109.0	99.0	30.1	113539
09:54:25	115.0	98.6	30.1	113670
09:54:26	115.0	98.6	30.1	113859
09:54:26	115.0	98.6	30.1	113815
09:54:26	115.0	98.6	30.1	113731
09:54:26	115.0	98.6	30.1	113847
09:54:26	115.0	98.6	30.1	114128
09:54:27	115.0	98.6	30.1	113957

09:54:27	115.0	98.6	30.1	113902
09:54:27	115.0	98.6	30.0	114002
09:54:27	108.2	98.6	30.0	114241
09:54:27	84.8	98.6	30.0	114396
09:54:28	75.0	98.6	30.0	114087
09:54:28	75.0	98.6	30.0	114149
09:54:28	75.0	98.6	29.9	114298
09:54:28	71.0	99.4	29.9	114552
09:54:28	71.0	98.3	29.9	114286
09:54:29	71.0	98.3	29.9	114380
09:54:29	71.0	98.3	29.9	114454
09:54:29	71.0	98.3	29.9	114640
09:54:29	71.0	97.5	30.1	114451
09:54:29	71.0	97.5	30.1	114458
09:54:30	71.0	97.5	30.1	114485
09:54:30	71.0	97.5	30.1	114633

Nota: la temperatura corresponde al sensor/chip MAX30102 y requiere calibración si se desea interpretar como temperatura corporal clínica.