

CE Diameter Report - Number Distribution



Measurement Details

Sample Name: Formiato Neuwendis

SOP Name: 5X.vsop

Edited: False

User Name: Morphologi

Edited On: 28 August 2015 10:52:26

Date: 28 August 2015 10:52:26

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 5x

Particles Counted: 42917

Result

CE Diameter Minimum (μm): 2.16

CE Diameter D[n, 0.1] (μm): 3.23

CE Diameter Maximum (μm): 599.11


CE Diameter D[n, 0.5] (μm): 9.30

CE Diameter Mean (μm): 18.15

CE Diameter D[n, 0.9] (μm): 43.04

CE Diameter STDV (μm): 26.11

CE Diameter RSD (%): 143.88

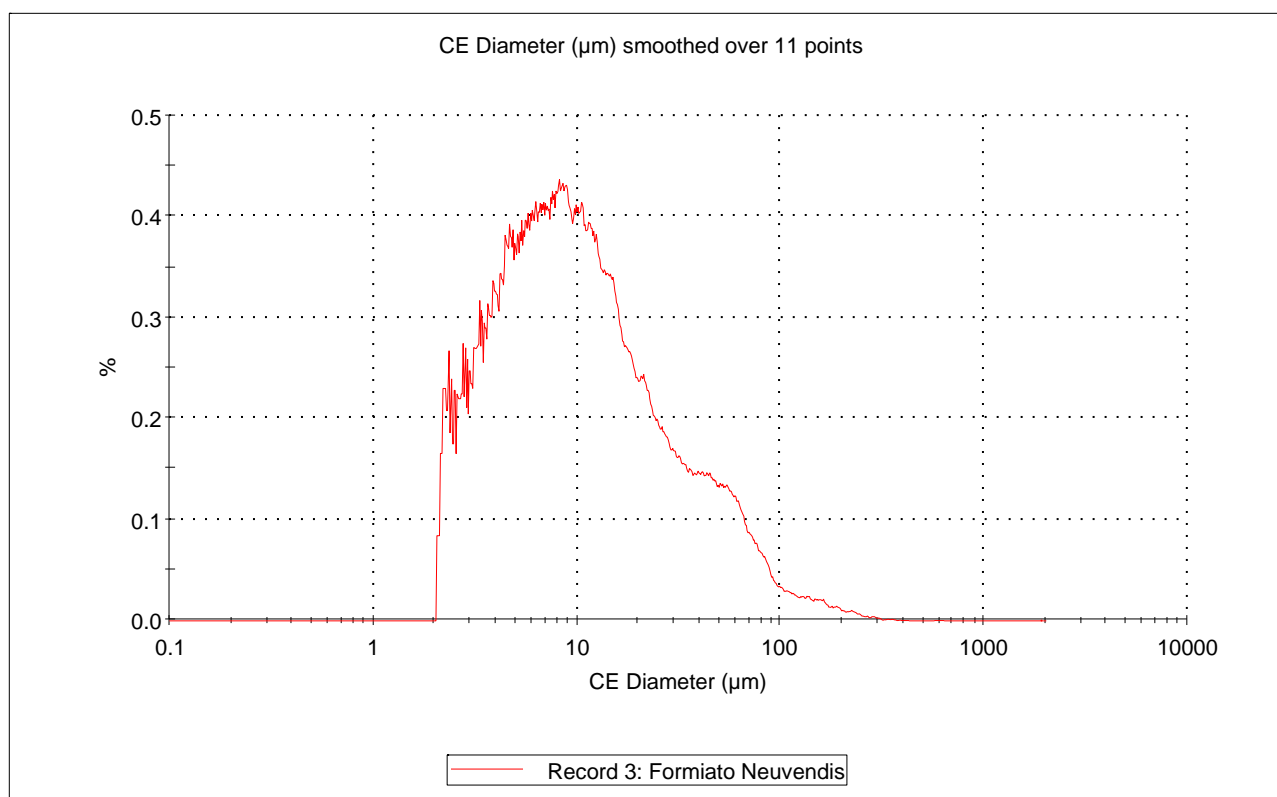

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com