

# Scattergram CE Diameter VS HS Circularity



## Measurement Details

**Sample Name:** Microsfere ESPHERES SL 300

**SOP Name:** MATERIE PRIME.vsop

**Edited:** False

**User Name:** Monphologi

**Edited On:** 24 April 2014 14:09:12

**Date:** 24 April 2014 14:09:12

## Analysis


**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 20x

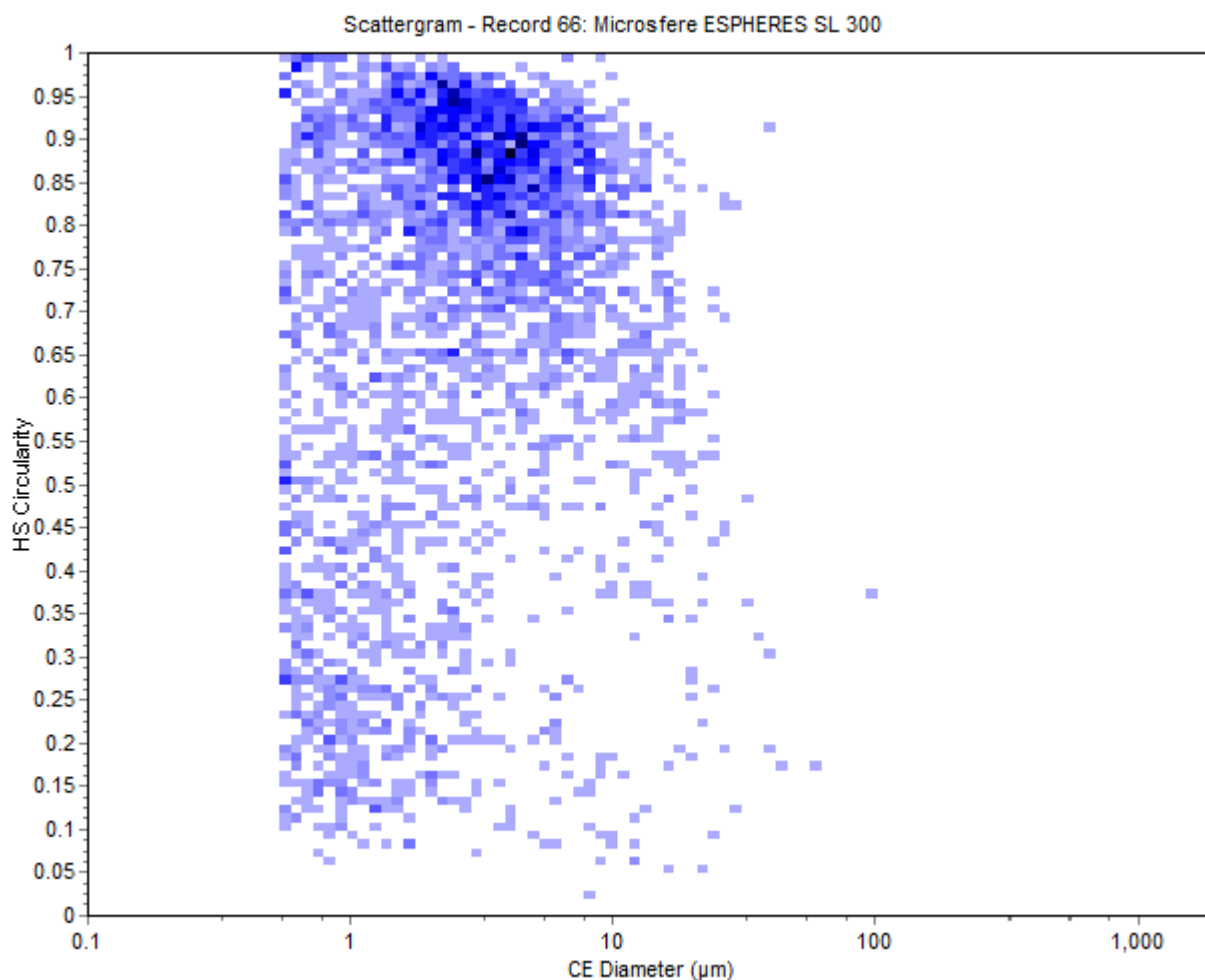

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)