

# CE Diameter Report - Number Distribution



## Measurement Details

**Sample Name:** MP4011

**SOP Name:** MATERIE PRIME.vsop

**Edited:** False

**User Name:** Morphologi

**Edited On:** 14 April 2014 19:17:26

**Date:** 14 April 2014 19:17:26

## Analysis

**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 20x

**Particles Counted:** 4368

## Result

**CE Diameter Minimum ( $\mu\text{m}$ ):** 0.54

**CE Diameter D[n, 0.1] ( $\mu\text{m}$ ):** 1.24

**CE Diameter Maximum ( $\mu\text{m}$ ):** 154.93

**CE Diameter D[n, 0.5] ( $\mu\text{m}$ ):** 7.59


**CE Diameter Mean ( $\mu\text{m}$ ):** 12.70

**CE Diameter D[n, 0.9] ( $\mu\text{m}$ ):** 30.54

**CE Diameter STDV ( $\mu\text{m}$ ):** 13.80

**CE Diameter RSD (%):** 108.67

CE Diameter ( $\mu\text{m}$ ) smoothed over 11 points

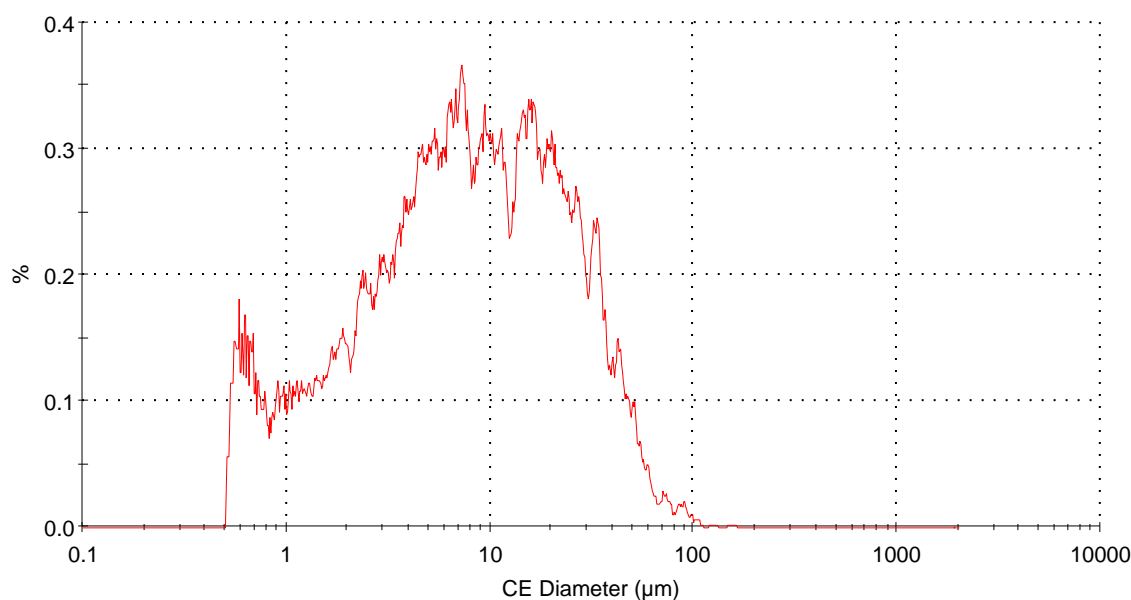

Record 602: MP4011

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)