

# Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: CRM

SOP Name: AnalyseFromFile.cfg

User Name: MDavies

Date: 19 July 2005 8:51:02 AM

Edited: False

Edited On: 14 October 2005 13:51:33

Analysis


SOP Analysis: 2.0

SOP Segmentation: Watershed

SOP Optic(s) used: 20x

SOP Fill Holes: True

SOP Trash Size: 100

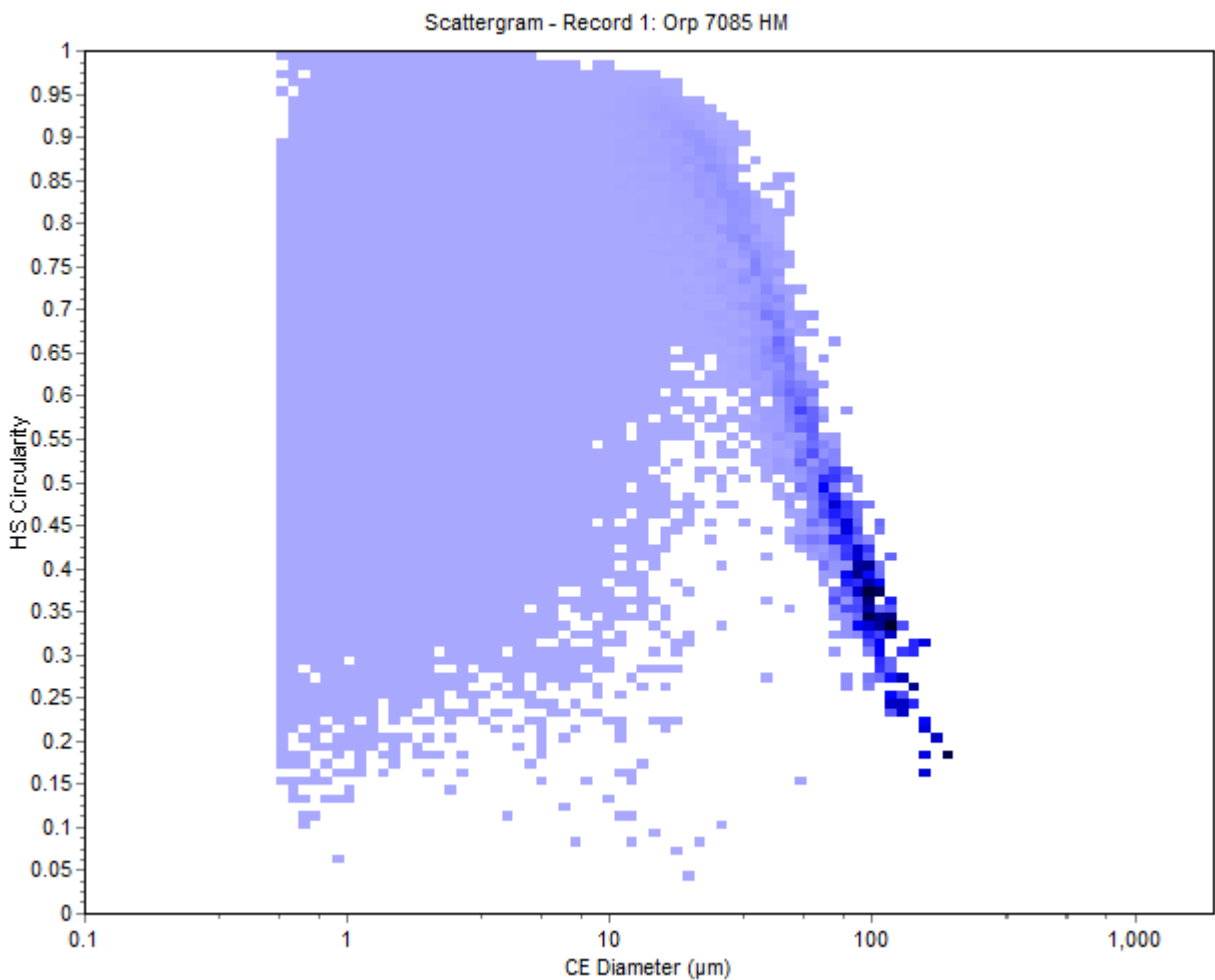

**Comments:** These particles were analysed from a file source