

# Intensity Mean Report - Number Distribution



## Measurement Details

**Sample Name:** Zeolite 5A

**SOP Name:** Materie prime 2.vsop

**Edited:** False

**User Name:**

**Edited On:** 06 May 2014 20:14:05

**Date:** 06 May 2014 20:14:05

## Analysis

**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 50x

## Result

**Mean Intensity Minimum:** 33

**Mean Intensity D[n, 0.1]:** 55

**Mean Intensity Maximum:** 129

**Mean Intensity D[n, 0.5]:** 79

**Mean Intensity Mean:** 83


**Mean Intensity D[n, 0.9]:** 121

**Particles Counted:** 8093

**Mean Intensity STDV:** 23

**Mean Intensity RSD (%):** 27.05

Intensity Mean smoothed over 11 points

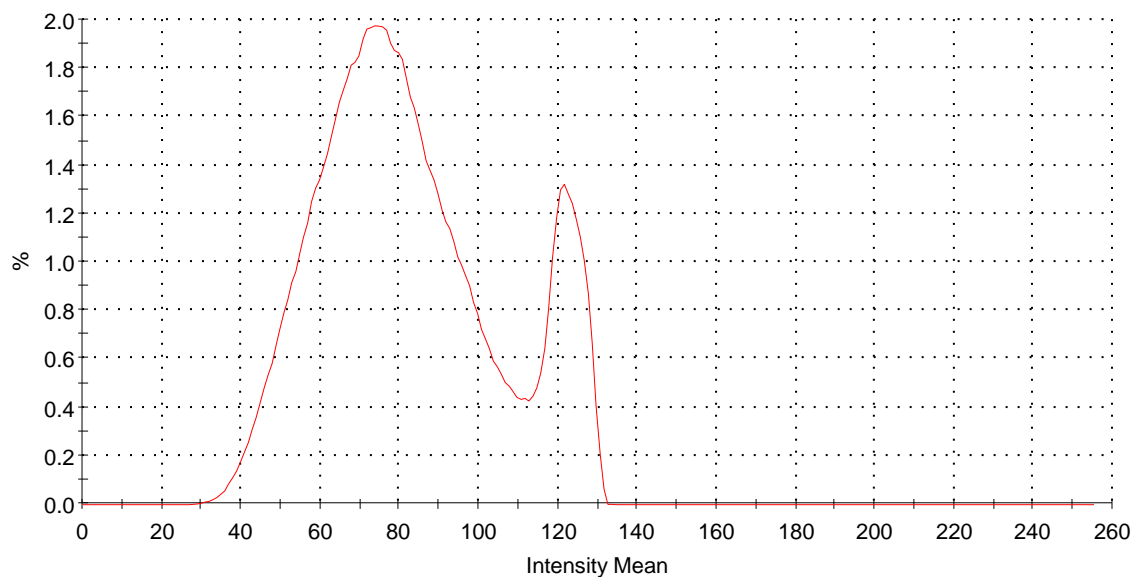

Record 1: Zeolite 5A

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)