

Intensity Mean Report - Number Distribution



Measurement Details

Sample Name: MP 2100

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name: Morphologi

Edited On: 14 April 2014 14:33:09

Date: 14 April 2014 13:58:10

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x

Result

Mean Intensity Minimum: 35

Mean Intensity D[n, 0.1]: 62

Mean Intensity Maximum: 152

Mean Intensity D[n, 0.5]: 123


Mean Intensity Mean: 115

Mean Intensity D[n, 0.9]: 149

Particles Counted: 3008

Mean Intensity STDV: 33

Mean Intensity RSD (%): 28.36

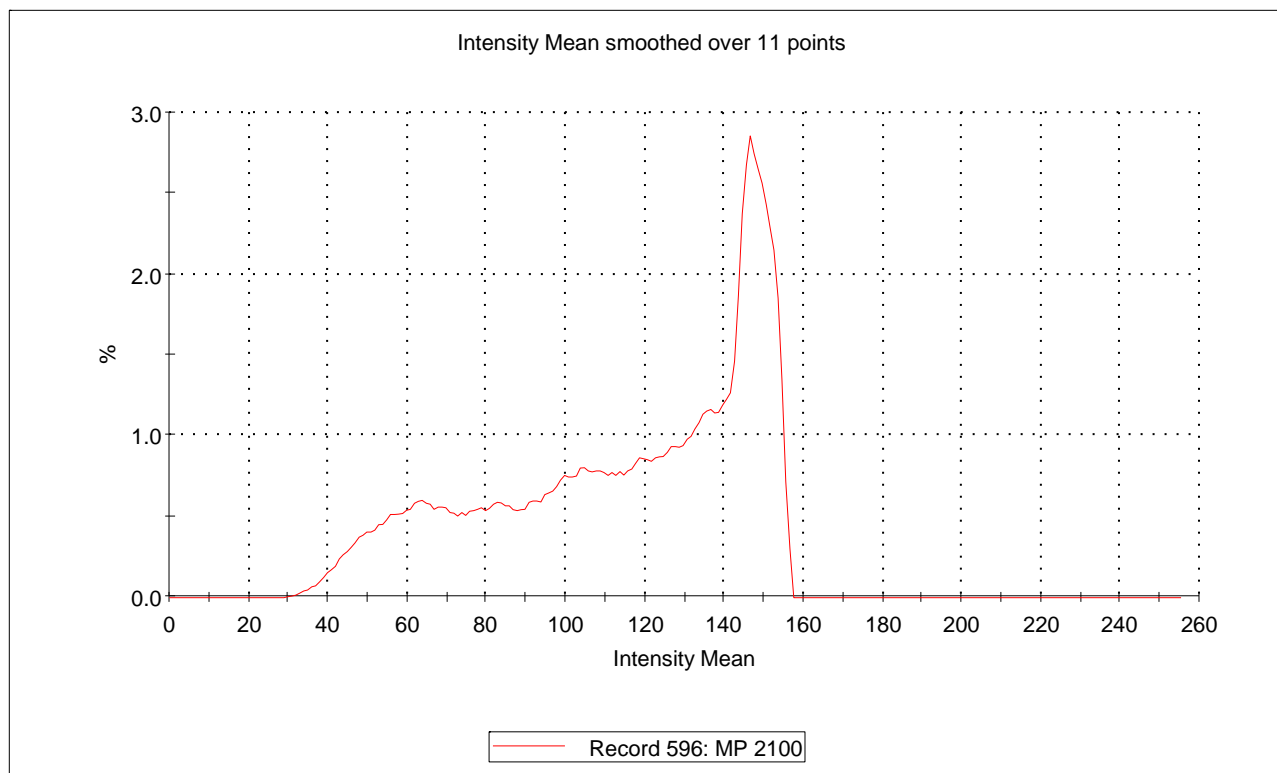

Comments: