

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: Tylose MH 15002 P6

SOP Name: AnalyseFromFile.cfg

Edited: False

User Name: Morphologi

Edited On: 25 November 2015 11:45:56

Date: 25 November 2015 11:45:56

Analysis


SOP Analysis: 2.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 100

SOP Optic(s) used: 10x

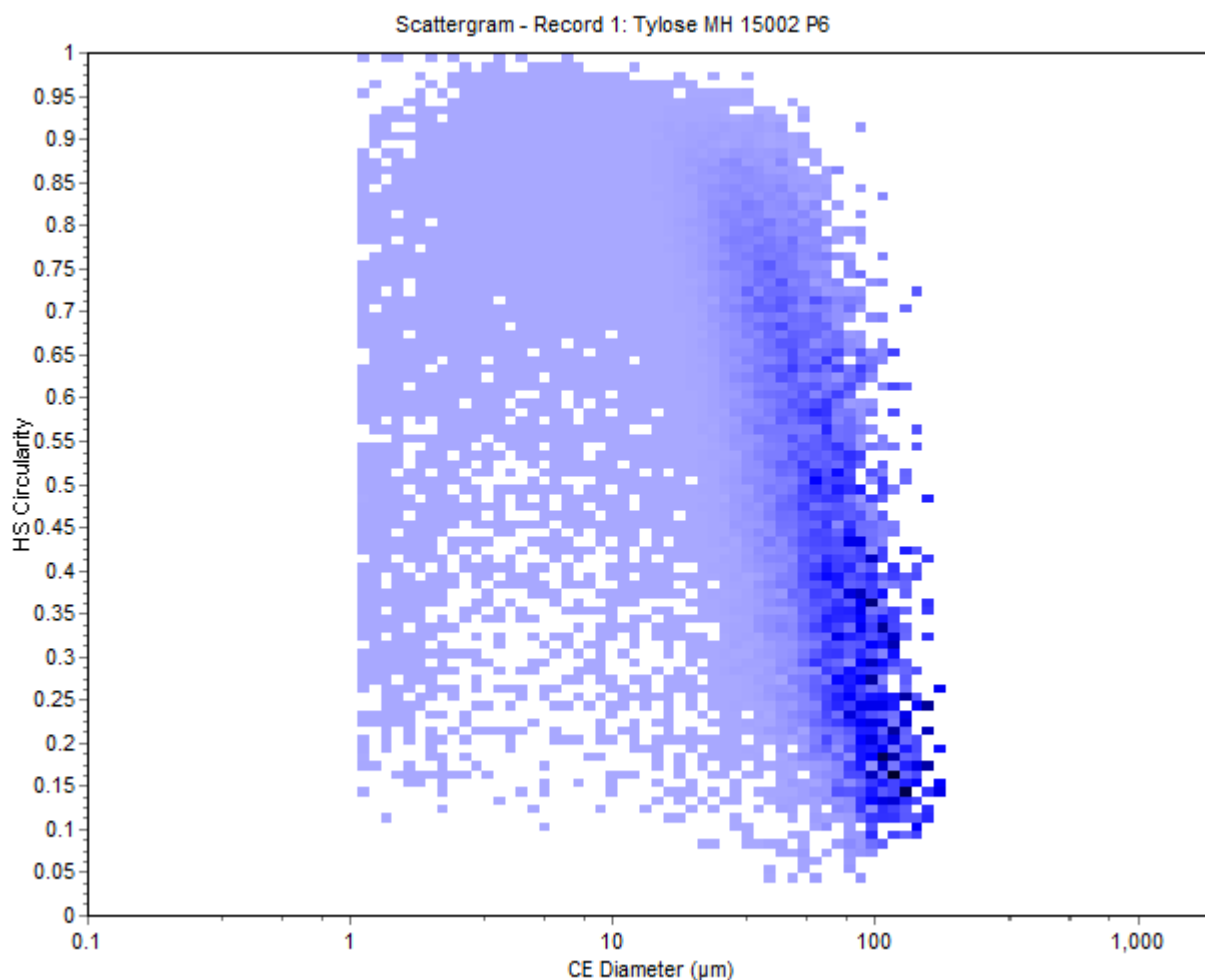

Comments: These particles were analysed from a file source

Morphologi

Malvern Instruments Worldwide

www.malvern.com