

# HS Circularity - Number Distribution



## Measurement Details

**Sample Name:** PENTACHEM - PENTARAPID CR 1001

**SOP Name:** MATERIE PRIME.vsop

**User Name:** Unknown

**Date:** 13 May 2014 16:34:11

**Edited:** True

**Edited On:** 13 May 2014 16:47:01

## Analysis

**SOP Analysis:** 3.0

**SOP Segmentation:** None

**SOP Optic(s) used:** 20x

**SOP Fill Holes:** True

**SOP Trash Size:** 10

## Result

**HS Circularity Minimum:** 0.076

**HS Circularity Maximum:** 1.000

**HS Circularity Mean:** 0.824

**Particles Counted:** 99232


**HS Circularity D[n, 0.1]:** 0.607

**HS Circularity D[n, 0.5]:** 0.871

**HS Circularity D[n, 0.9]:** 0.957

**HS Circularity STDV:** 0.145

**HS Circularity RSD (%):** 17.623

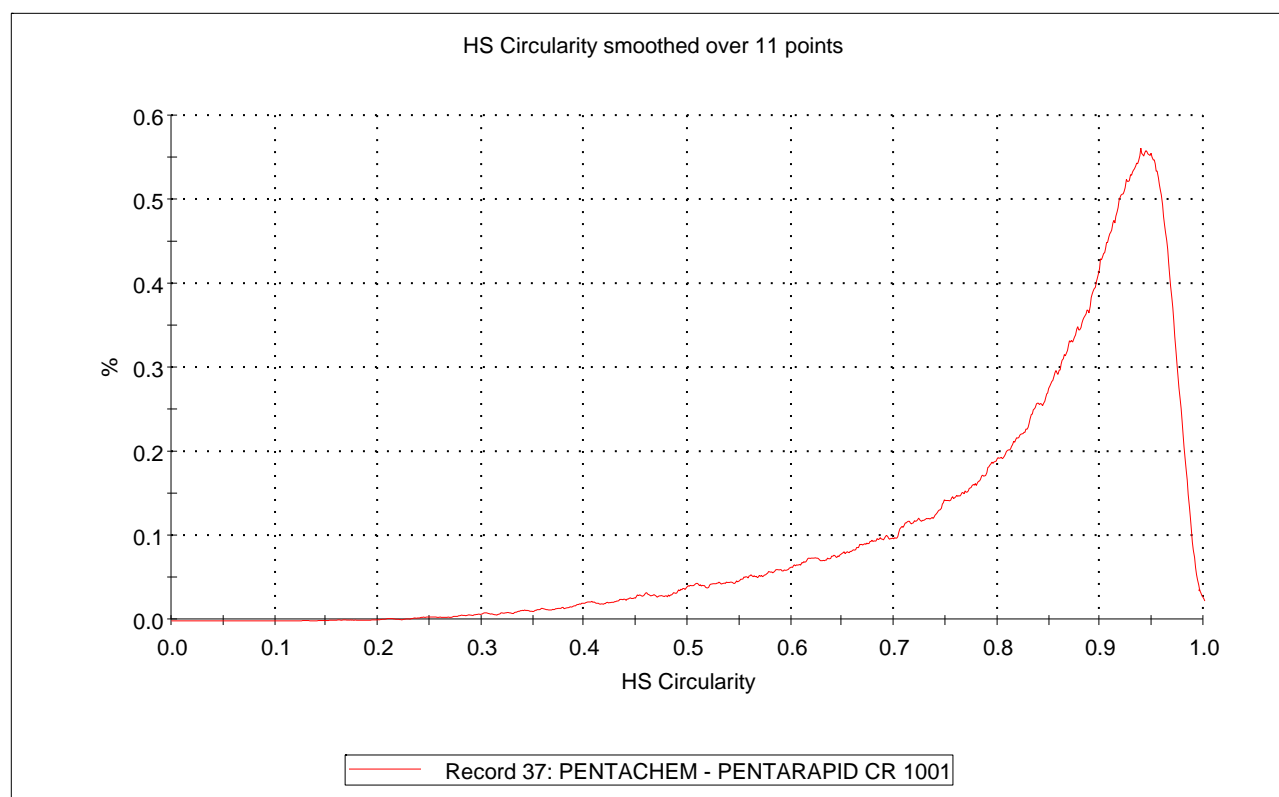

## Comments: