

# Intensity Mean Report - Number Distribution



## Measurement Details

**Sample Name:** Microsfere ESPHERES SL 300

**SOP Name:** MATERIE PRIME.vsop

**Edited:** False

**User Name:** Morphologi

**Edited On:** 24 April 2014 14:09:12

**Date:** 24 April 2014 14:09:12

## Analysis

**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 20x

## Result

**Mean Intensity Minimum:** 43

**Mean Intensity D[n, 0.1]:** 80

**Mean Intensity Maximum:** 147

**Mean Intensity D[n, 0.5]:** 103


**Mean Intensity Mean:** 102

**Mean Intensity D[n, 0.9]:** 118

**Particles Counted:** 3323

**Mean Intensity STDV:** 15

**Mean Intensity RSD (%):** 14.57

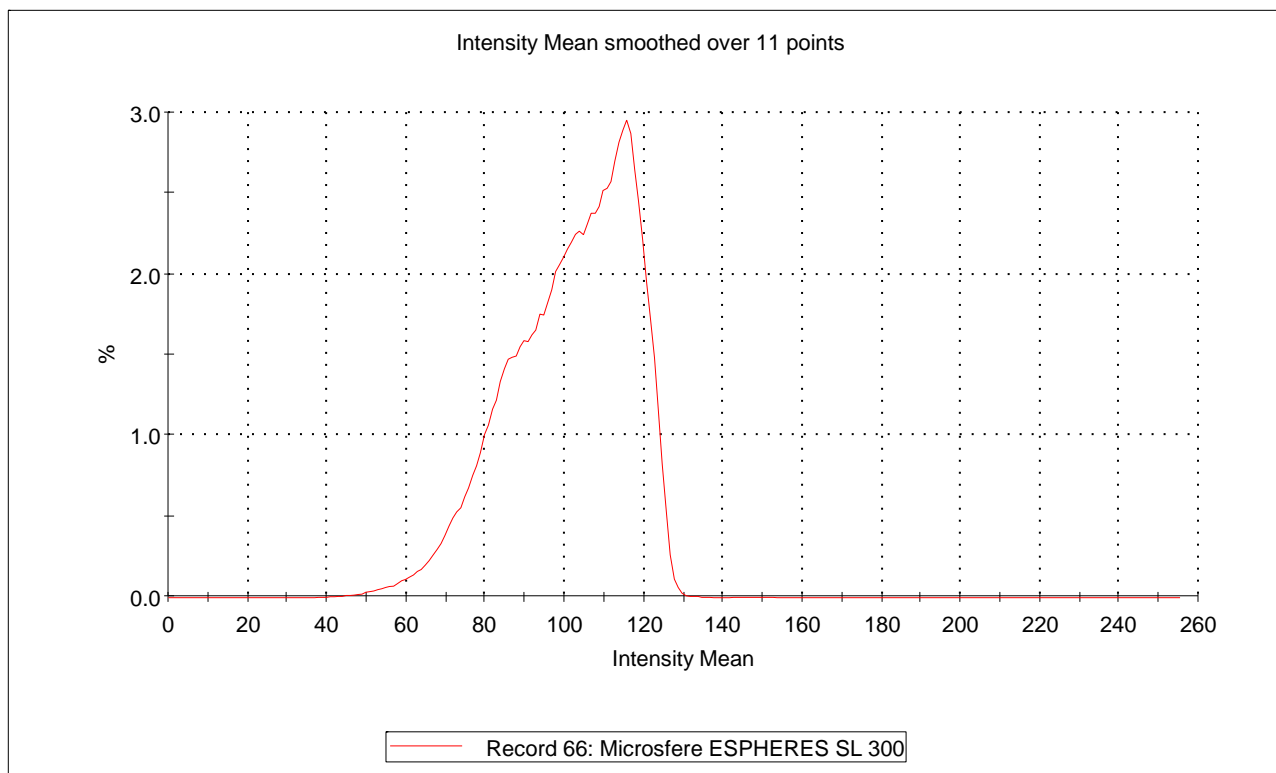

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)