

# Scattergram CE Diameter VS HS Circularity



## Measurement Details

**Sample Name:** Anidrite fluorsid

**SOP Name:** GESSI.vsop

**Edited:** True

**User Name:** Antonio Roberto

**Edited On:** 16 June 2014 13:12:20

**Date:** 16 June 2014 13:05:50

## Analysis


**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 50x

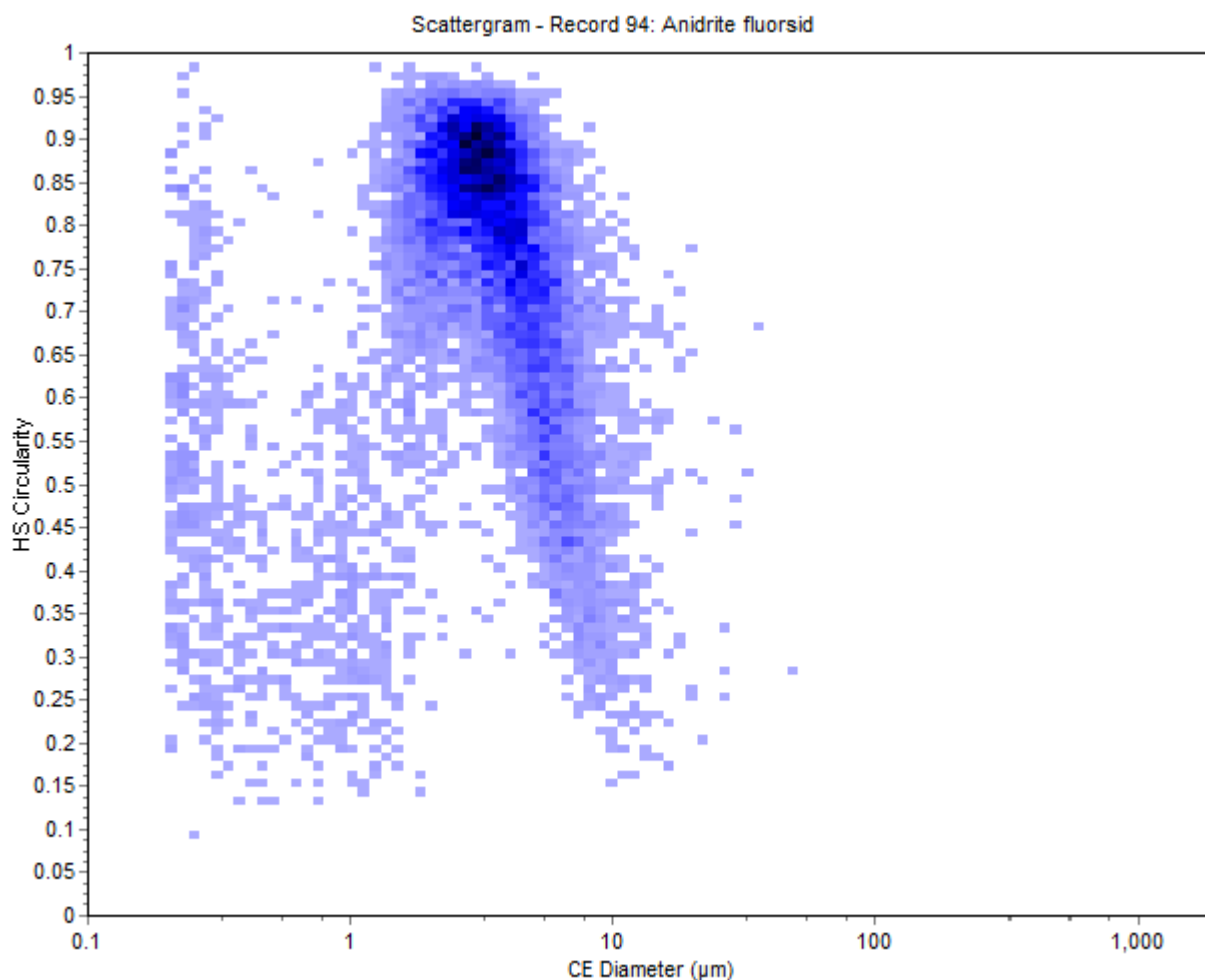

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)