HS Circularity - Number Distribution

Malvern

Measurement Details

Sample Name: COPRA 900

SOP Name: MATERIE PRIME.vsop

User Name: Morfologi

Date: 22 April 2014 14:06:36

Edited: True

Edited On: 22 April 2014 14:49:57

Analysis

SOP Analysis: 3.0

SOP Segmentation: None

SOP Optic(s) used: 10x, 50x

SOP Fill Holes: True

SOP Trash Size: 10

Result

HS Circularity Minimum: 0.066

HS Circularity Maximum: 1.000

HS Circularity Mean: 0.799

Particles Counted: 5397

HS Circularity D[n, 0.1]: 0.374

HS Circularity D[n, 0.5]: 0.903

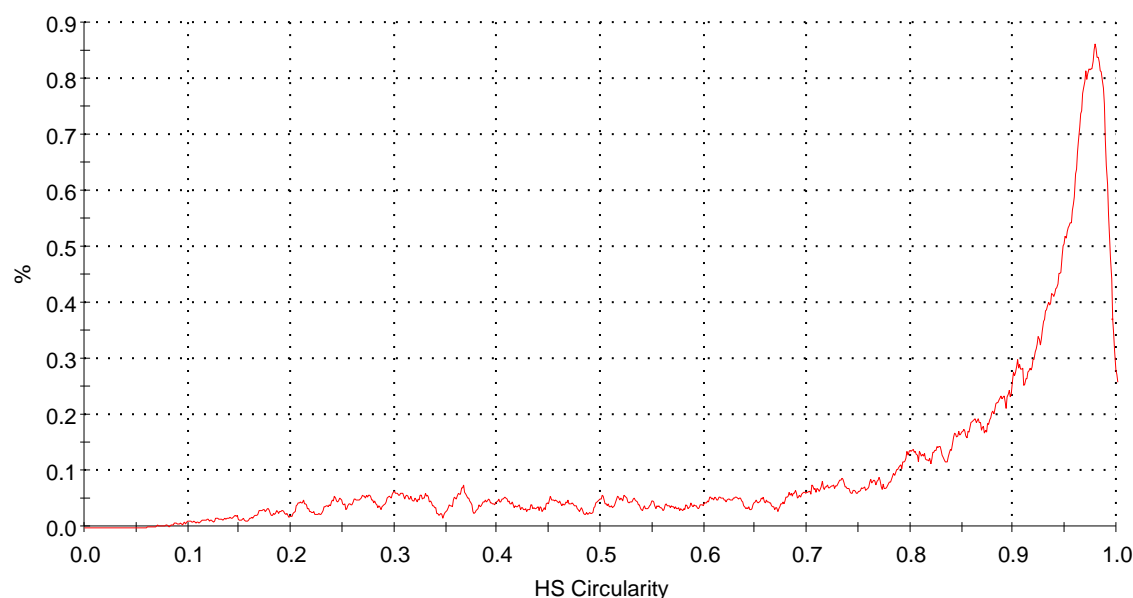**HS Circularity D[n, 0.9]:** 0.982

HS Circularity STDV: 0.232

HS Circularity RSD (%): 28.968

HS Circularity smoothed over 11 points

Record 27: COPRA 900

Comments:

Morfologi

Malvern Instruments Worldwide

www.malvern.com