

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: Bactiblock 101

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name: morfologi

Edited On: 22 April 2014 18:41:25

Date: 22 April 2014 18:34:02

Analysis


SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 10x, 50x

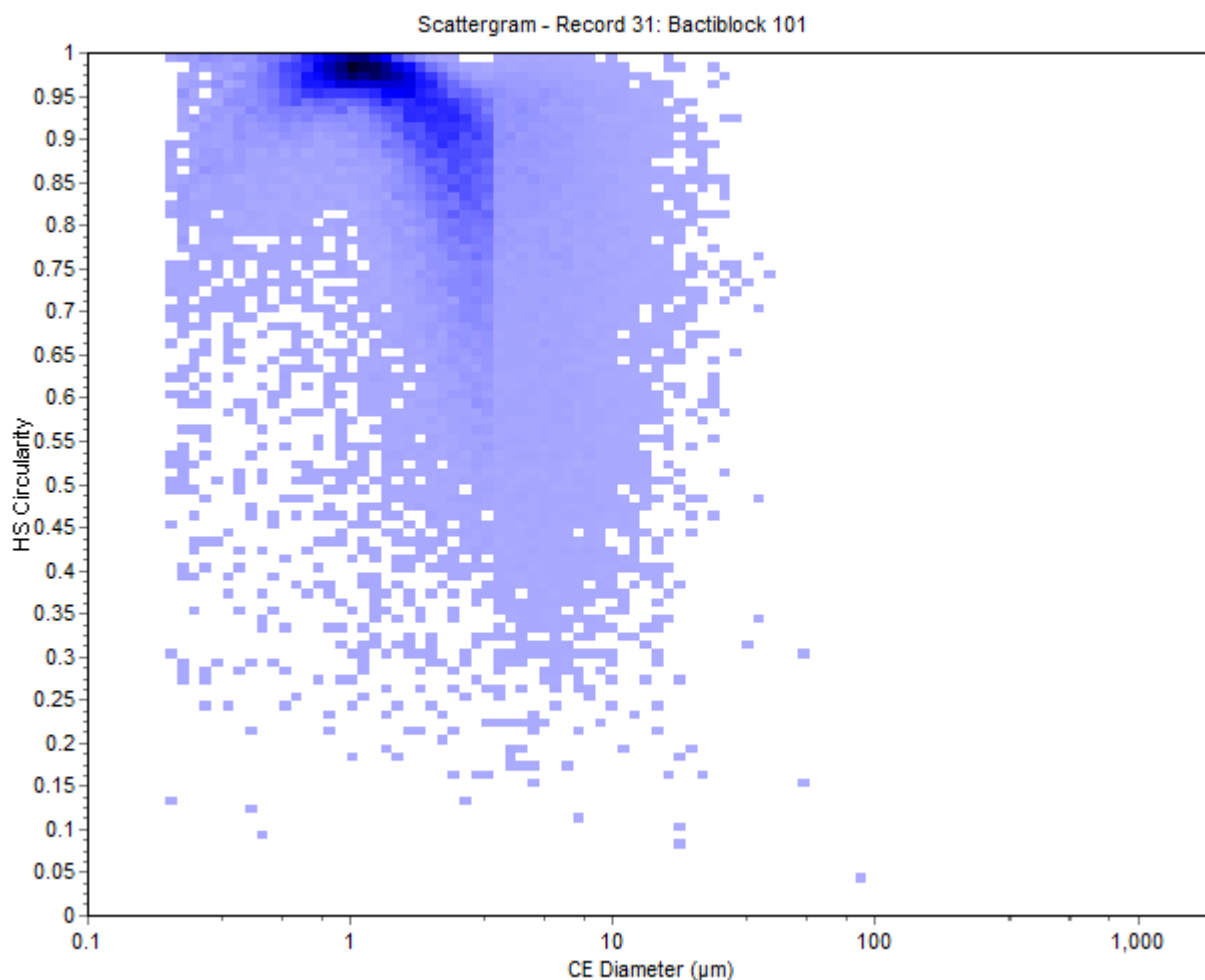

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com