


Customer	Dal Tile
Sample ID	QUARTZ 5020 Granusic
Test	AGGREGATES CHARACTERIZATION
Sample (g)	300
Lab address	PF Lab Services – Simbario (VV) – ITALY

CHEMICAL COMPOSITION: Quartz sand

MOISTURE CONCENTRATION: 0 %

Particles size distribution

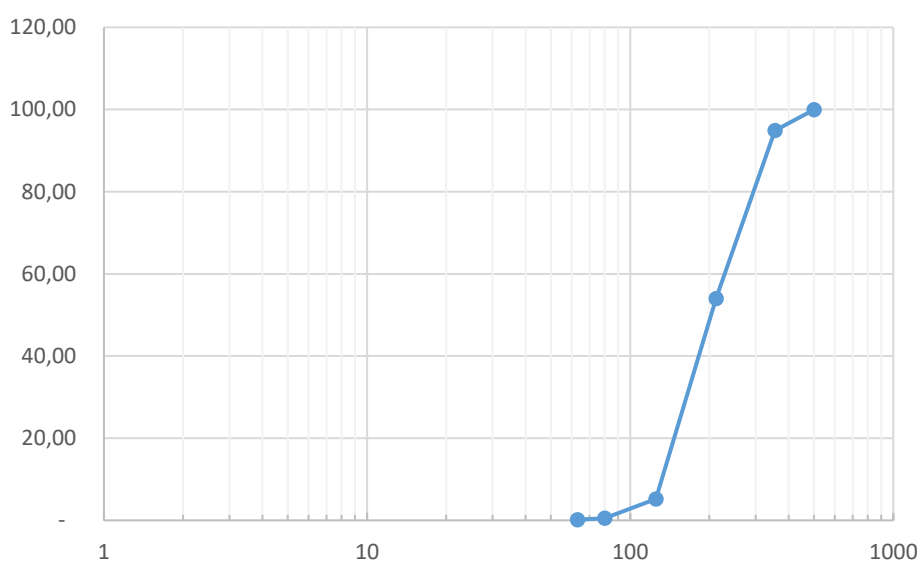

Particles size analysis

Diameter (µm)	Passing (%)
500	99,98
355	94,86
212	54,00
125	5,21
80	0,51
63	0,16

For the analysis were used Sieves mesh mall S Steel I.S.O. 3310 (UNI EN 933-2) and electric sieve shaker with timer (UNI EN 932-5 ISO 3310-1).