

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: Formiato Shandong

SOP Name: AnalyseFromFile.cfg

: Morphologi

Date: 27 November 2015 13:10:51

Edited: False

Edited On: 27 November 2015 13:10:51

Analysis


SOP Analysis: 2.0

SOP Segmentation: None

SOP Optic(s) used: 10x

SOP Fill Holes: True

SOP Trash Size: 100

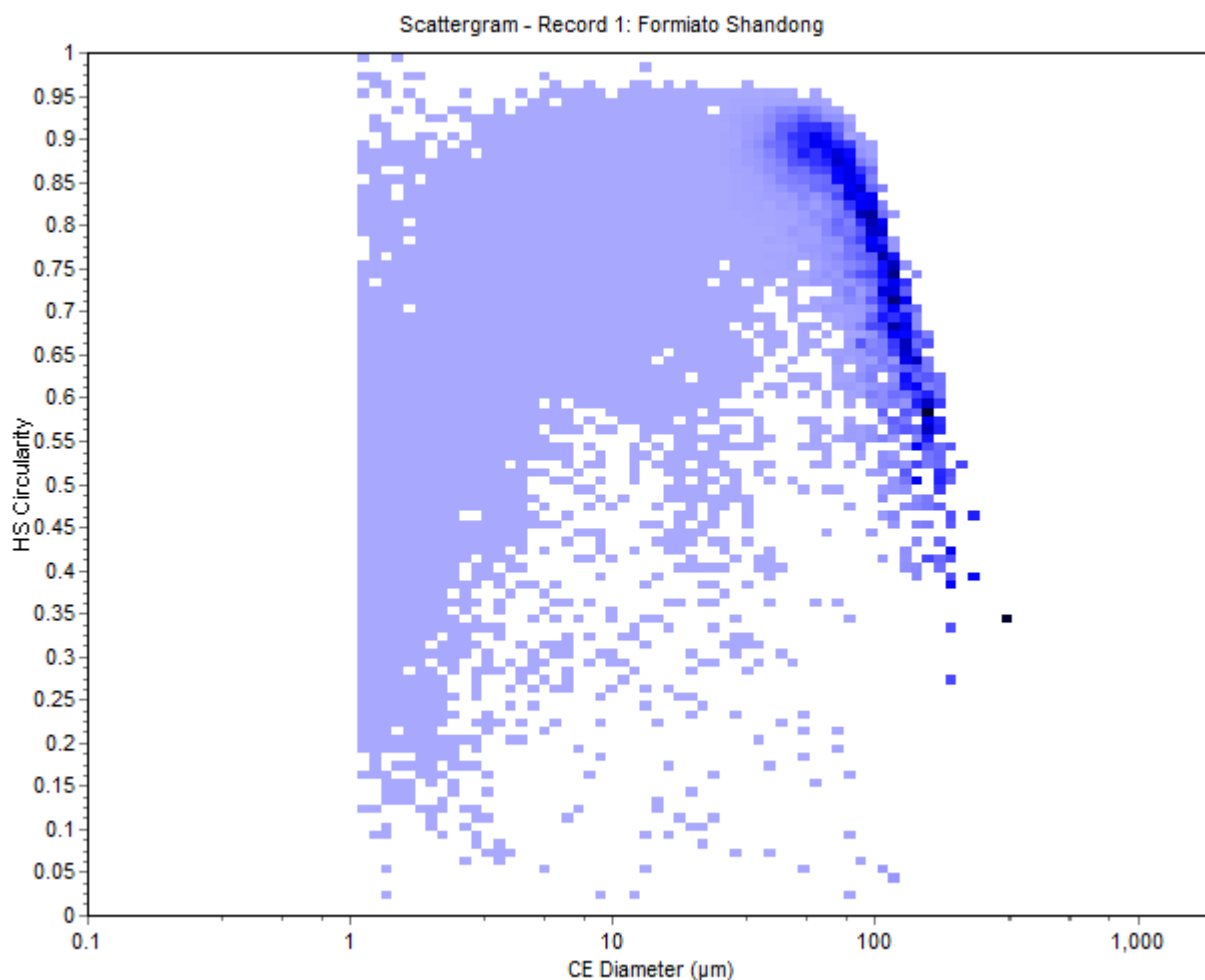

Comments: These particles were analysed from a file source

Morphologi

Malvern Instruments Worldwide

www.malvern.com