

# Scattergram CE Diameter VS HS Circularity



## Measurement Details

**Sample Name:** CRM

**SOP Name:** AnalyseFromFile.cfg

**Edited:** False

**User Name:** Morphologi

**Edited On:** 28 August 2015 10:52:26

**Date:** 28 August 2015 10:52:26

## Analysis


**SOP Analysis:** 2.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 100

**SOP Optic(s) used:** 5x

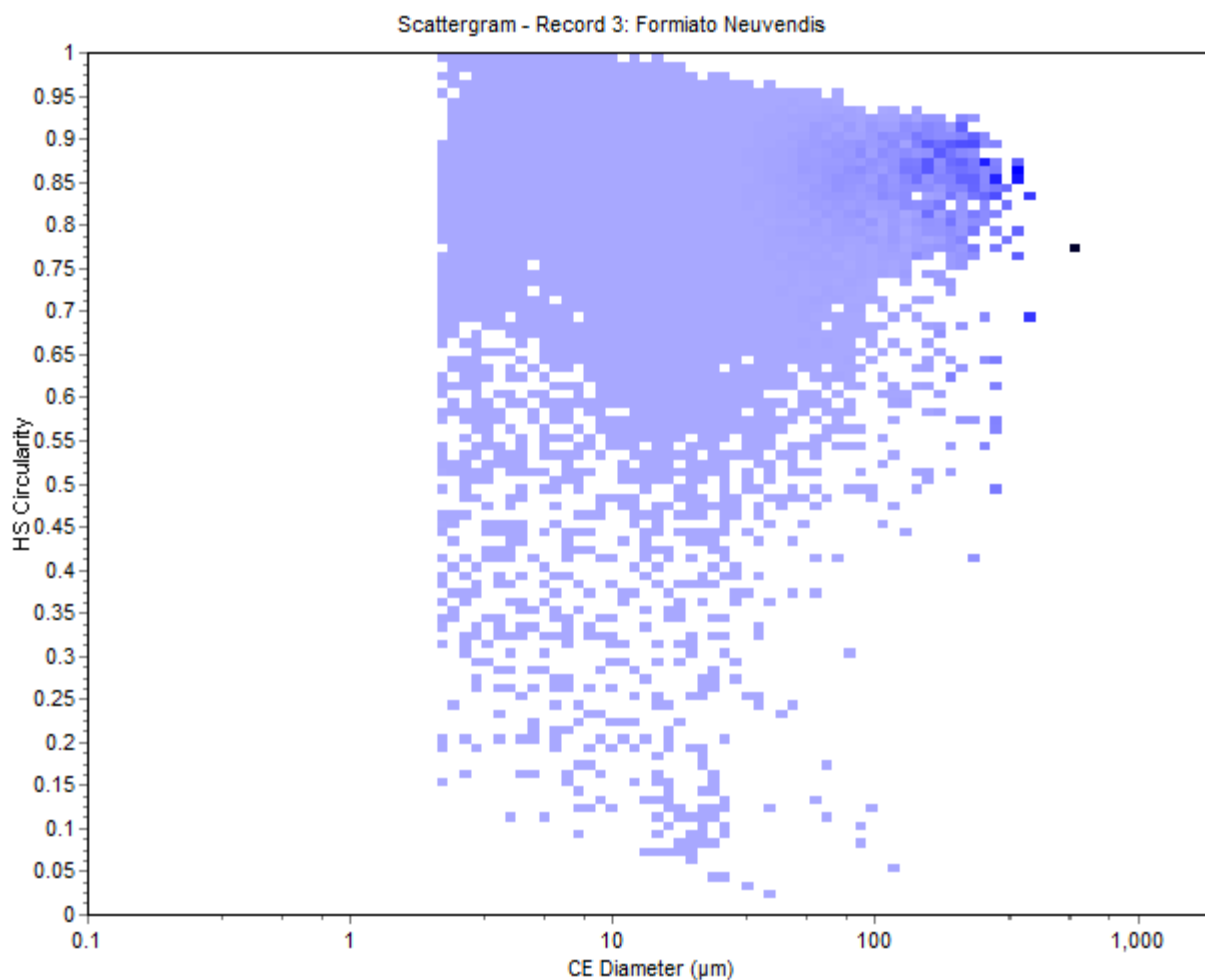

**Comments:** These particles were analysed from a file source

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)