

# Scattergram CE Diameter VS HS Circularity



## Measurement Details

**Sample Name:** PENTACHEM - PENTARAPID CR 1001

**SOP Name:** MATERIE PRIME.vsop

**Edited:** True

**User Name:** Unknown

**Edited On:** 13 May 2014 16:47:01

**Date:** 13 May 2014 16:34:11

## Analysis


**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 20x

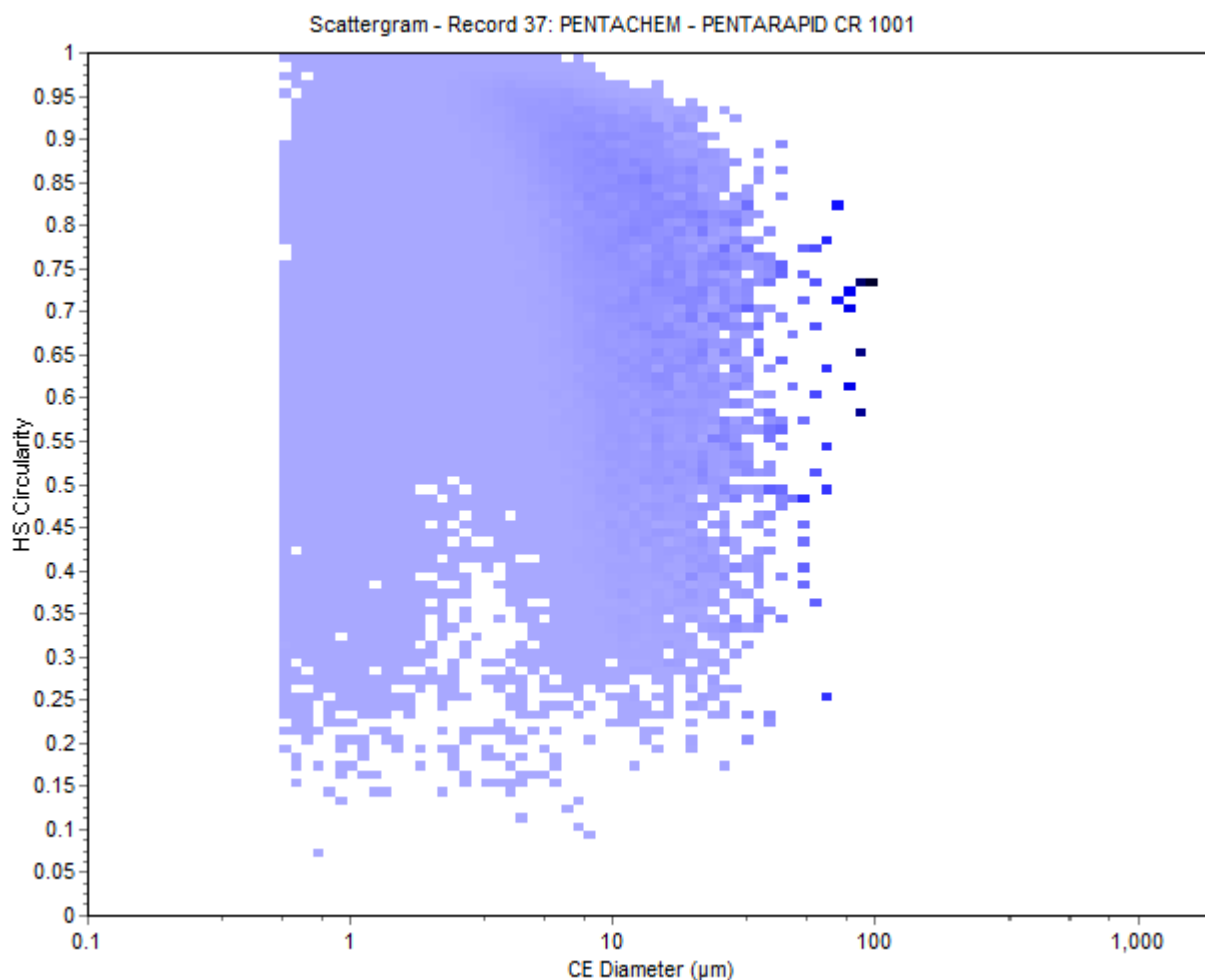

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)