

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sampl... SODIO GLUCONATO - EIGENMANN & VE...

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name:

Edited On: 20 May 2014 12:04:42

Date: 20 May 2014 12:00:09

Analysis


SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 5x

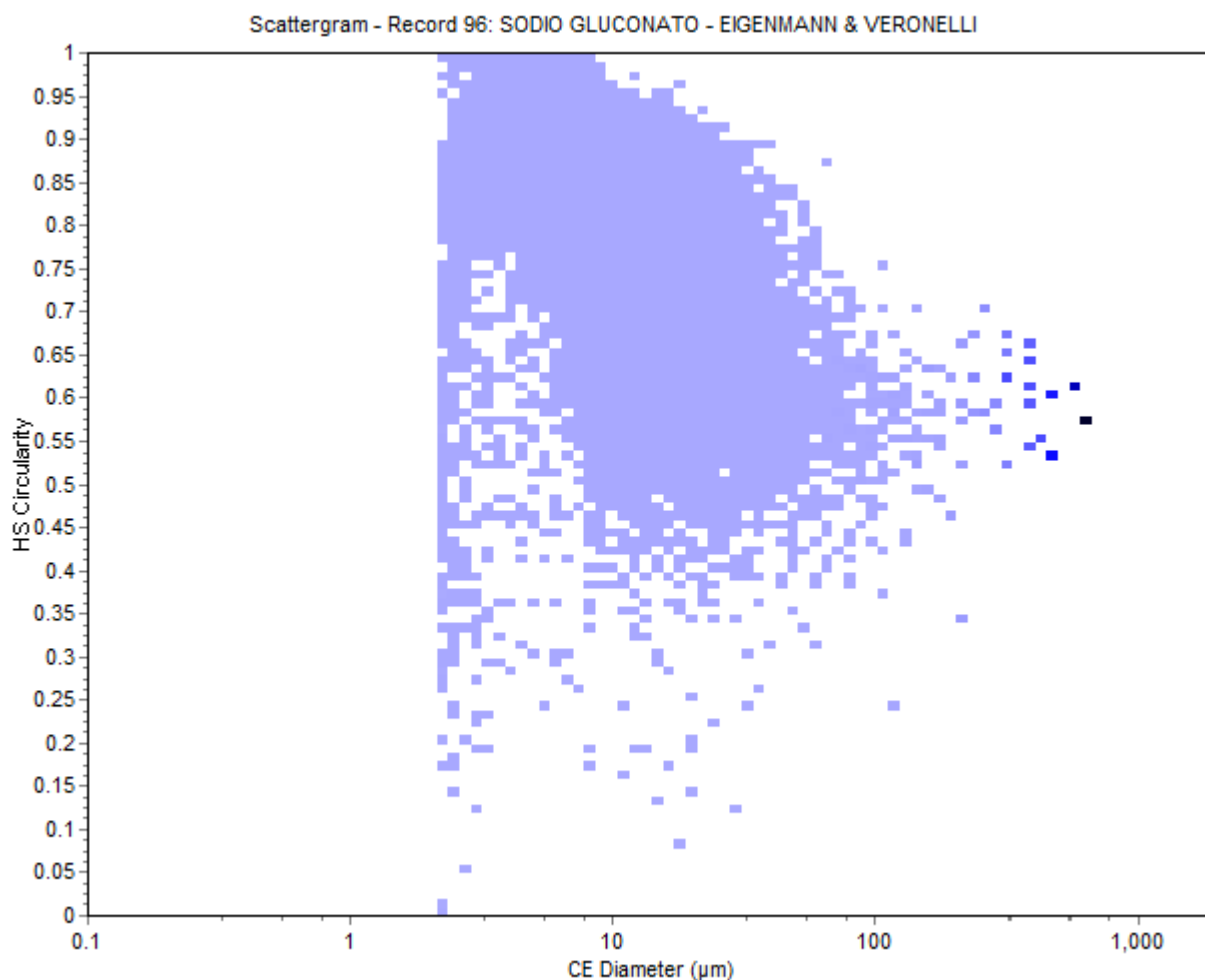

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com