

CE Diameter Report - Number Distribution



Measurement Details

Sample Name: OFL 190314 SG

SOP Name: MATERIE PRIME.vsop

Edited: False

User Name: MORPHOLOGI

Edited On: 29 April 2014 19:02:58

Date: 29 April 2014 19:02:58

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x, 50x

Particles Counted: 7005

Result

CE Diameter Minimum (μm): 0.22

CE Diameter D[n, 0.1] (μm): 1.07

CE Diameter Maximum (μm): 63.15

CE Diameter D[n, 0.5] (μm): 1.17


CE Diameter Mean (μm): 1.61

CE Diameter D[n, 0.9] (μm): 2.51

CE Diameter STDV (μm): 2.08

CE Diameter RSD (%): 128.79

CE Diameter (μm) smoothed over 11 points

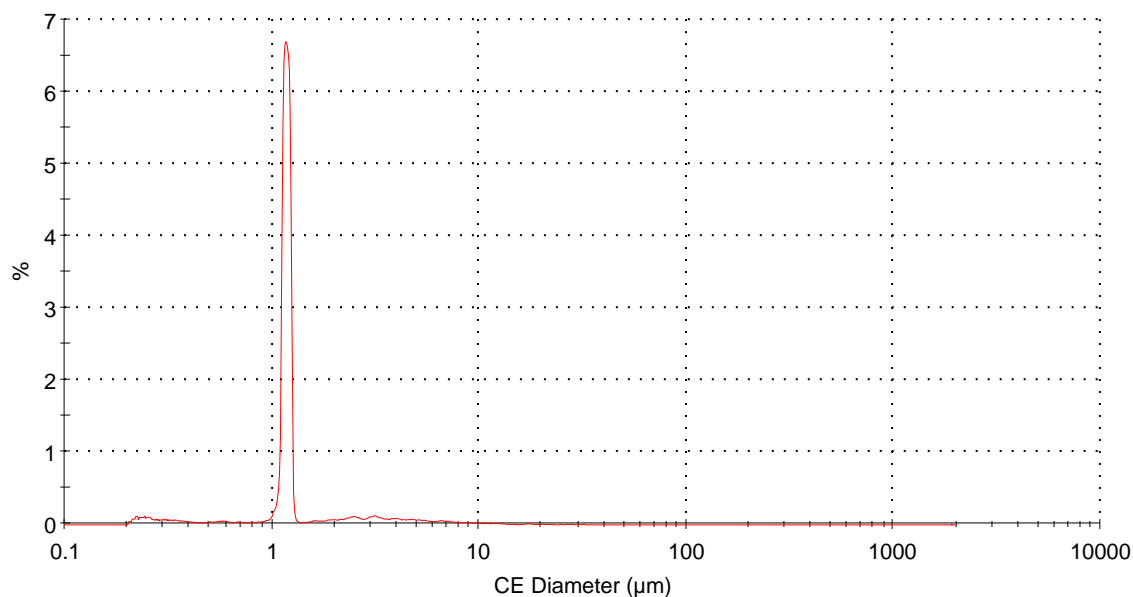

Record 93: OFL 190314 SG

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com