

HS Circularity - Number Distribution



Measurement Details

Sample Name: Vinnapas 7055E

SOP Name: MATERIE PRIME.vsop

User Name: Morphologi

Date: 14 April 2014 09:40:58

Edited: True

Edited On: 14 April 2014 09:58:36

Analysis

SOP Analysis: 3.0

SOP Segmentation: None

SOP Optic(s) used: 20x

SOP Fill Holes: True

SOP Trash Size: 10

Result

HS Circularity Minimum: 0.075

HS Circularity Maximum: 1.000

HS Circularity Mean: 0.791

Particles Counted: 4679


HS Circularity D[n, 0.1]: 0.541

HS Circularity D[n, 0.5]: 0.838

HS Circularity D[n, 0.9]: 0.957

HS Circularity STDV: 0.169

HS Circularity RSD (%): 21.377

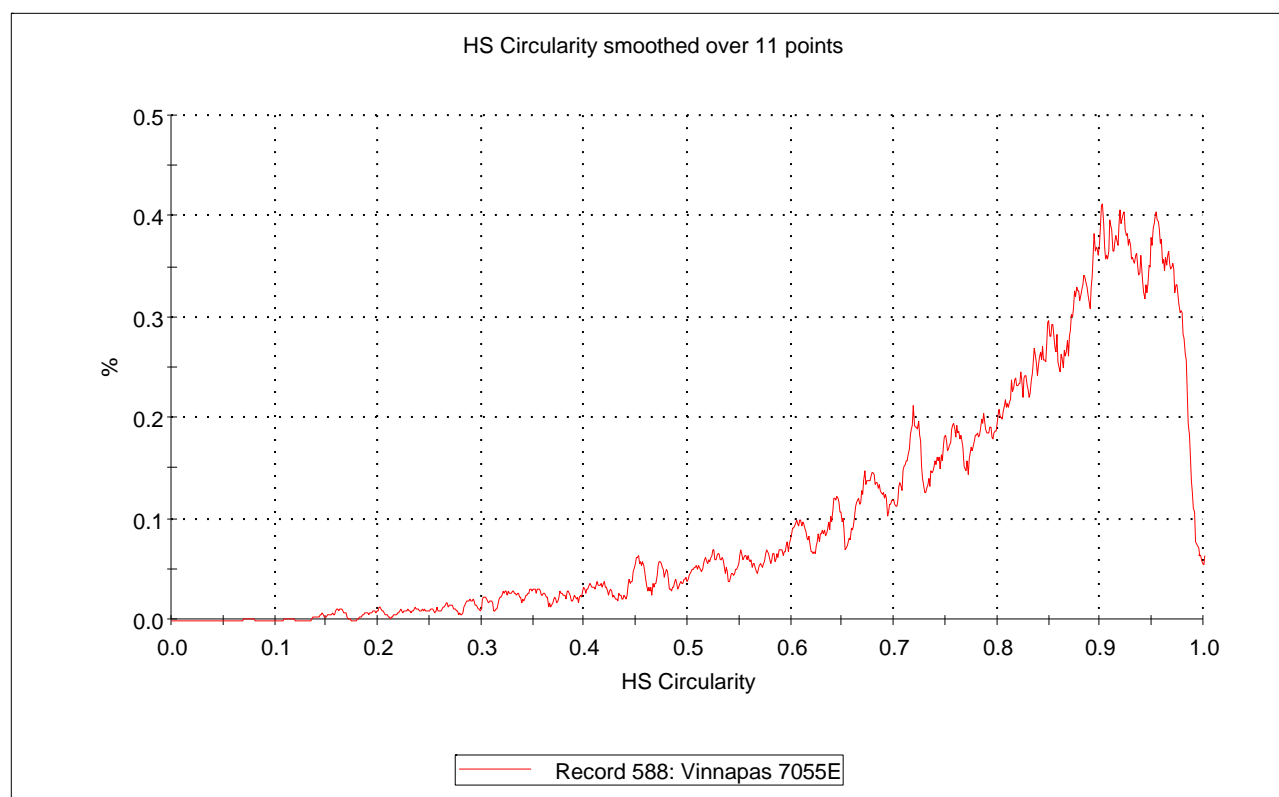

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com