

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: OMYACARB 1T UM +

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name:

Edited On: 27 May 2014 12:11:37

Date: 27 May 2014 11:57:01

Analysis


SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 50x

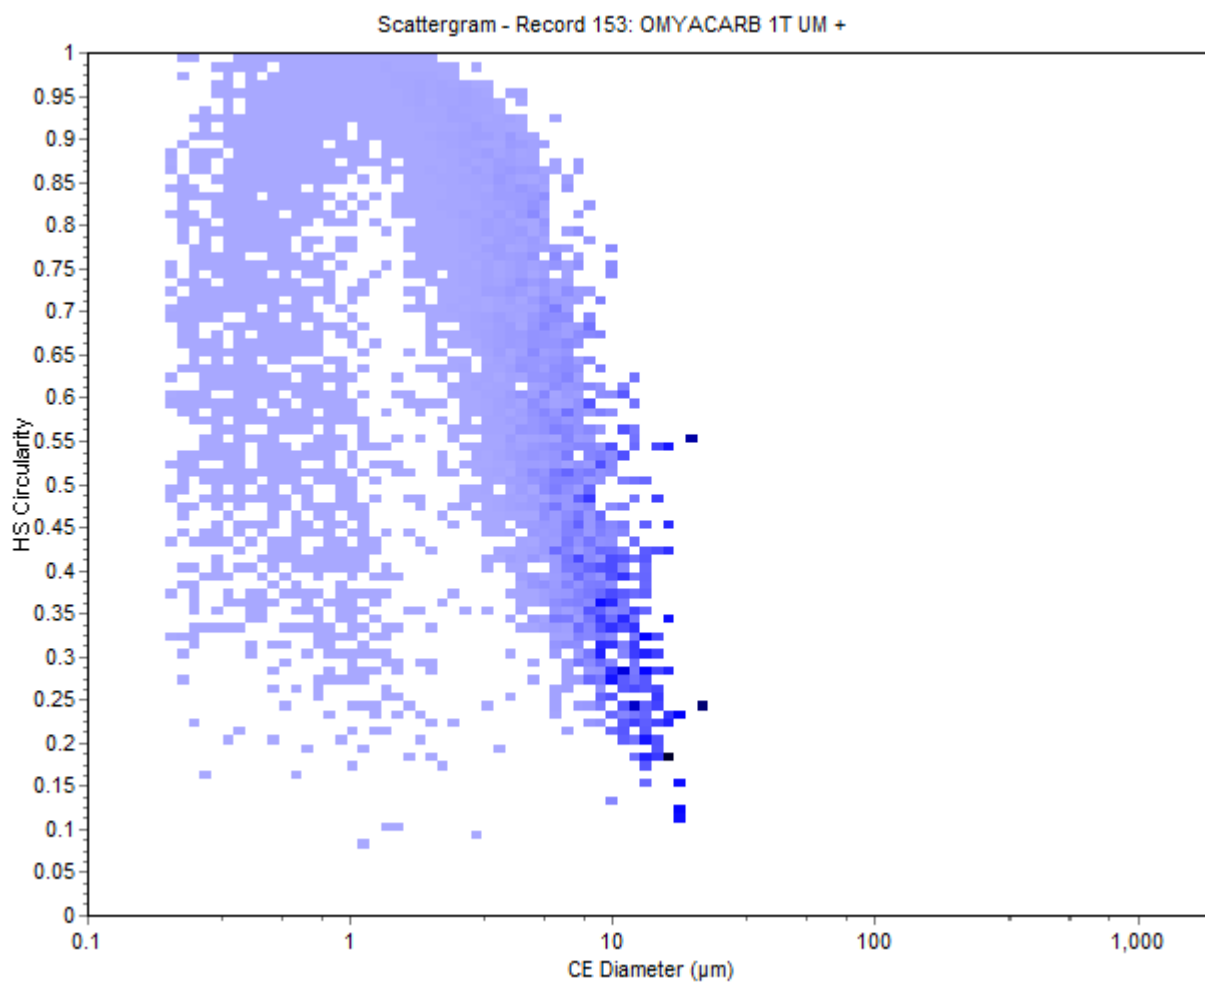

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com