

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: OFL 190314 SG

SOP Name: MATERIE PRIME.vsop

Edited: False

User Name: MORPHOLOGI

Edited On: 29 April 2014 19:02:58

Date: 29 April 2014 19:02:58

Analysis


SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x, 50x

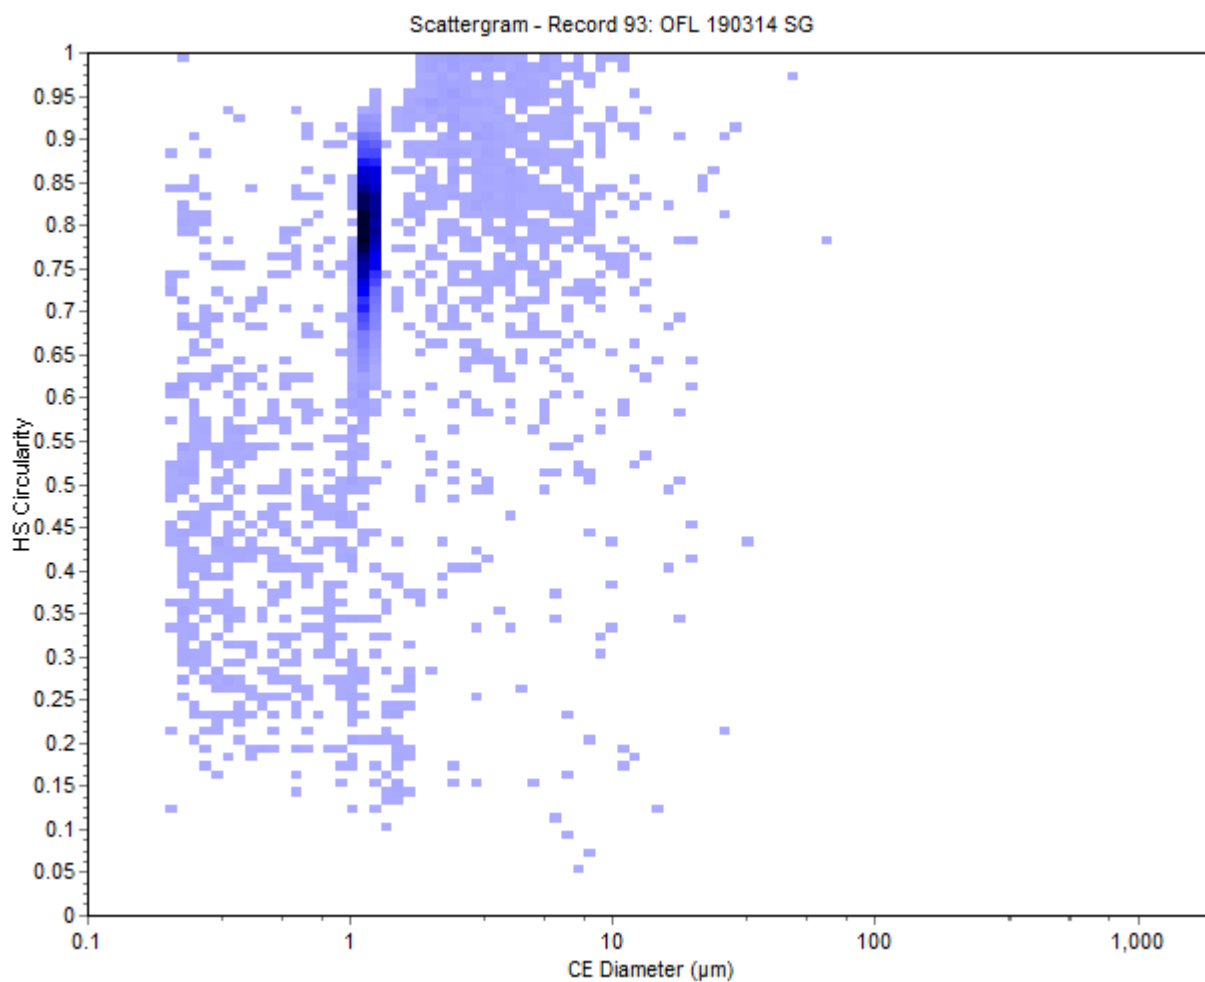

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com