

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: Calce Idrata - Vesci

SOP Name: Calci.vsop

Edited: True

User Name: roberto antonio

Edited On: 18 June 2014 17:48:28

Date: 18 June 2014 17:29:22

Analysis


SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 50x

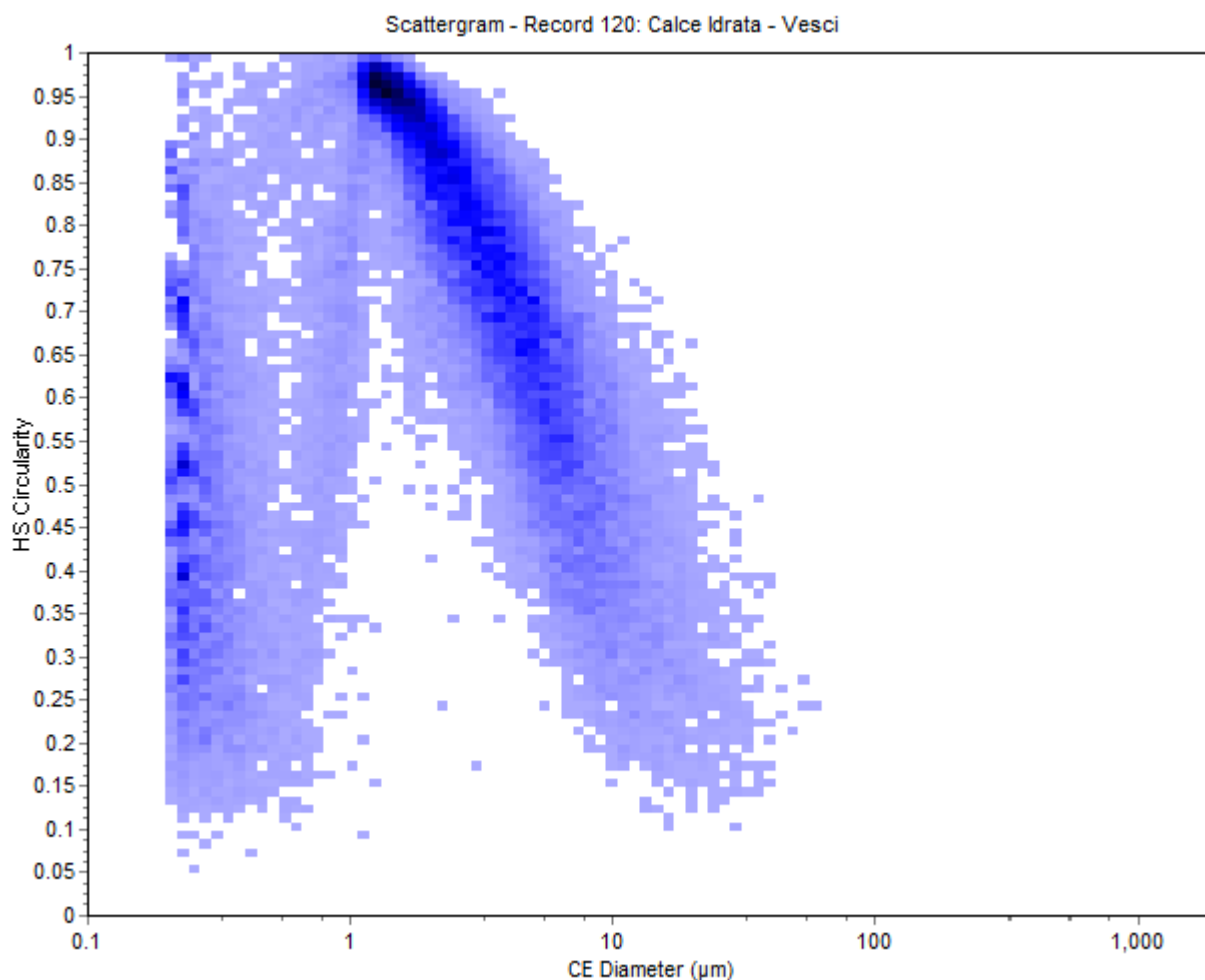

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com