

# Scattergram CE Diameter VS HS Circularity



## Measurement Details

**Sample Name:** Carbonato di Calcio Femia

**SOP Name:** Calci.vsop

**Edited:** False

**User Name:** Domenico

**Edited On:** 19 December 2014 17:56:38

**Date:** 19 December 2014 17:56:38

## Analysis


**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 50x

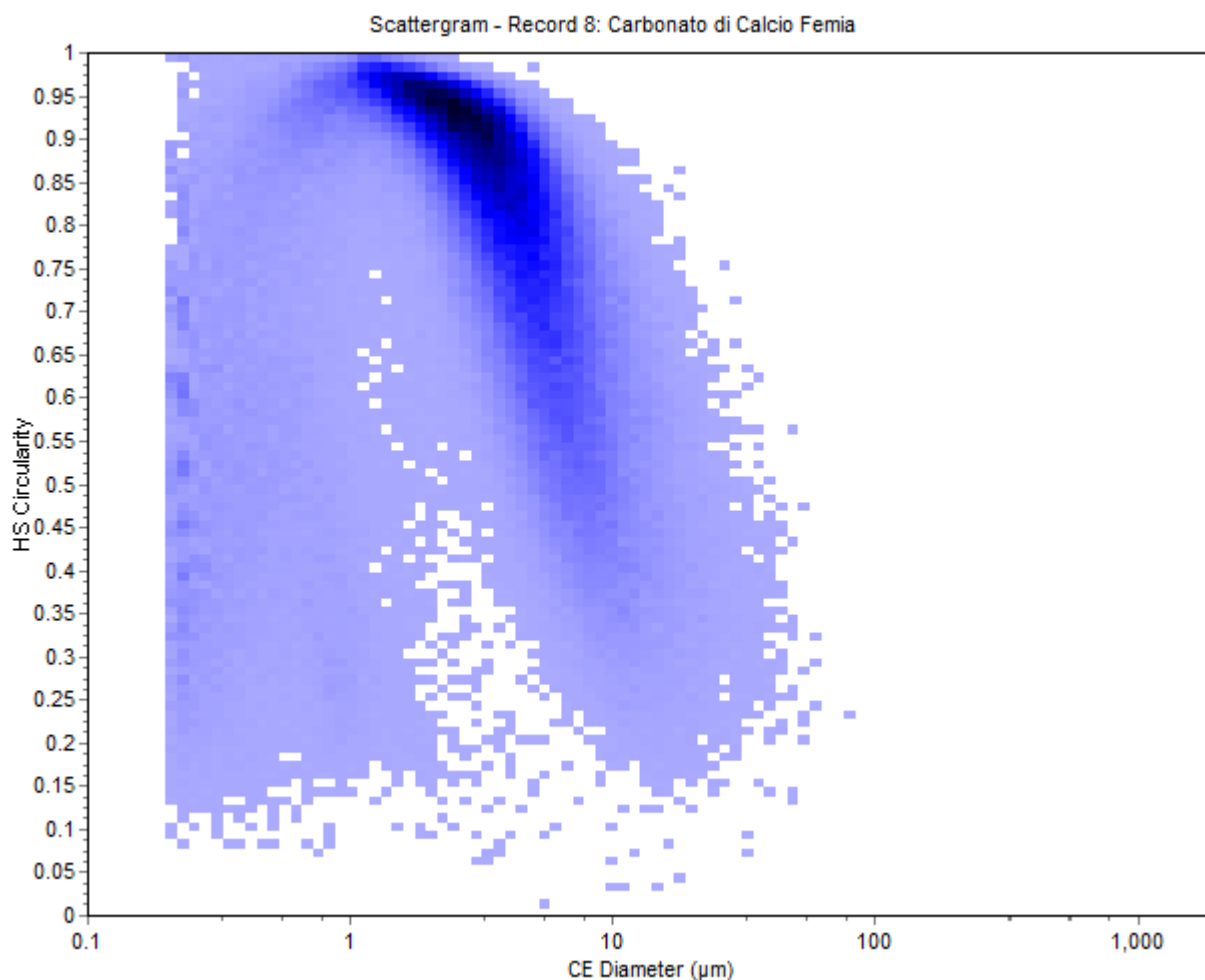

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)