

HS Circularity - Number Distribution



Measurement Details

Sample Name: Zeolite 5A

SOP Name: Materie prime 2.vsop

User Name:

Date: 06 May 2014 20:14:05

Edited: False

Edited On: 06 May 2014 20:14:05

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 50x

Result

HS Circularity Minimum: 0.003

HS Circularity Maximum: 0.995

HS Circularity Mean: 0.744

Particles Counted: 8093


HS Circularity D[n, 0.1]: 0.480

HS Circularity D[n, 0.5]: 0.791

HS Circularity D[n, 0.9]: 0.924

HS Circularity STDV: 0.177

HS Circularity RSD (%): 23.836

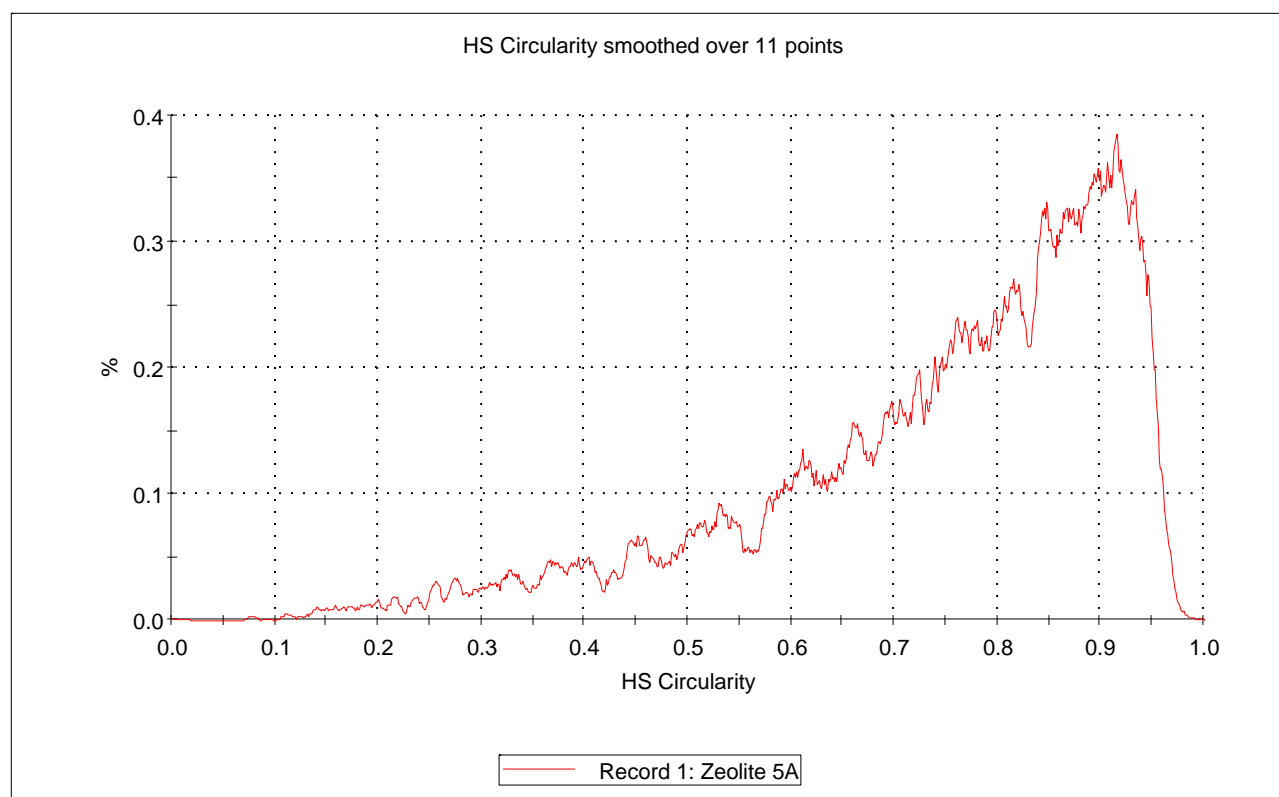

Comments: