

HS Circularity - Number Distribution



Measurement Details

Sample Name: OMYACARB 2UM

SOP Name: MATERIE PRIME.vsop

User Name:

Date: 27 May 2014 14:18:00

Edited: True

Edited On: 27 May 2014 14:26:23

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 50x

Result

HS Circularity Minimum: 0.067

HS Circularity D[n, 0.1]: 0.413

HS Circularity Maximum: 1.000

HS Circularity D[n, 0.5]: 0.793

HS Circularity Mean: 0.739


HS Circularity D[n, 0.9]: 0.966

Particles Counted: 63591

HS Circularity STDV: 0.213

HS Circularity RSD (%): 28.787

HS Circularity smoothed over 11 points

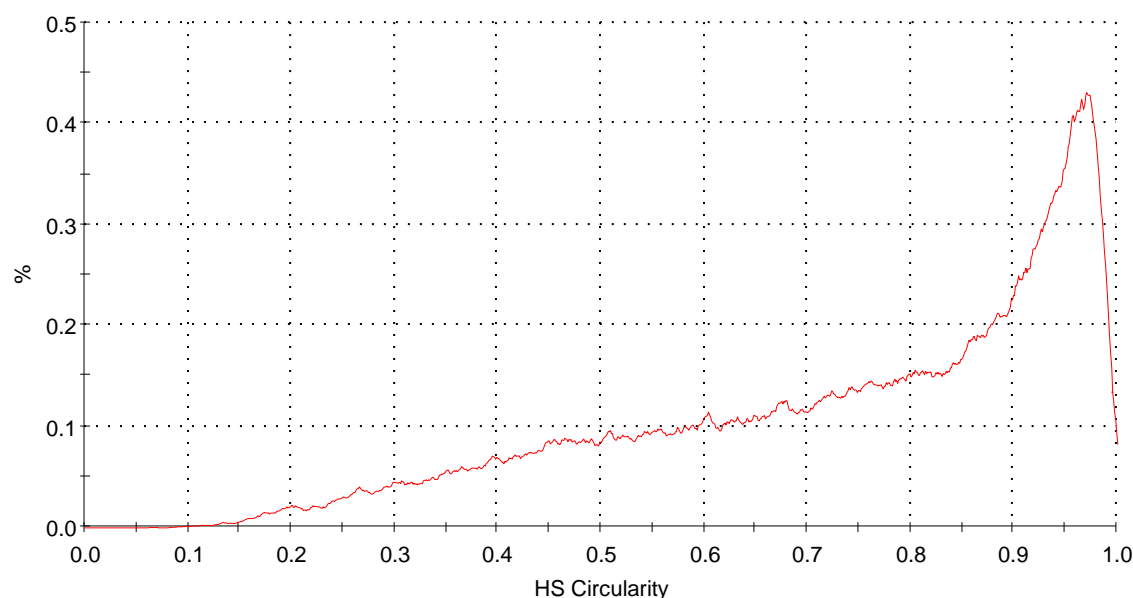

Record 155: OMYACARB 2UM

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com