

# HS Circularity - Number Distribution



## Measurement Details

**Sample Name:** PENTACHEM - PENTARAPID 99

**SOP Name:** MATERIE PRIME.vsop

**User Name:**

**Date:** 14 May 2014 12:32:35

**Edited:** True

**Edited On:** 14 May 2014 12:34:39

## Analysis

**SOP Analysis:** 3.0

**SOP Segmentation:** None

**SOP Optic(s) used:** 10x

**SOP Fill Holes:** True

**SOP Trash Size:** 10

## Result

**HS Circularity Minimum:** 0.040

**HS Circularity Maximum:** 1.000

**HS Circularity Mean:** 0.858

**Particles Counted:** 32191


**HS Circularity D[n, 0.1]:** 0.702

**HS Circularity D[n, 0.5]:** 0.886

**HS Circularity D[n, 0.9]:** 0.961

**HS Circularity STDV:** 0.121

**HS Circularity RSD (%):** 14.063

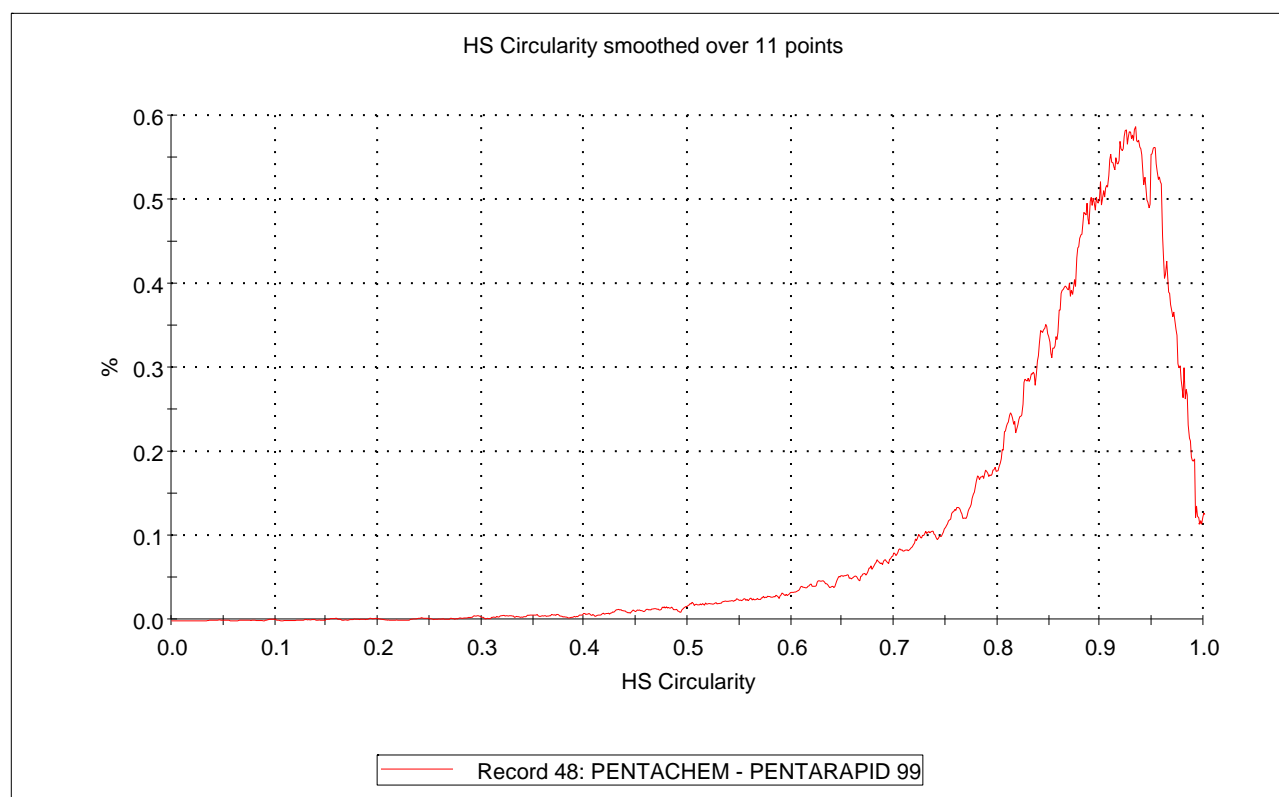

## Comments: